
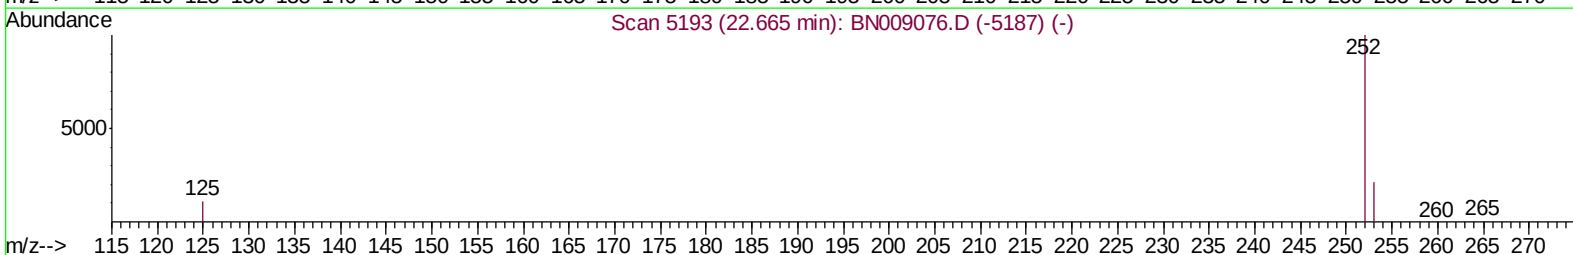
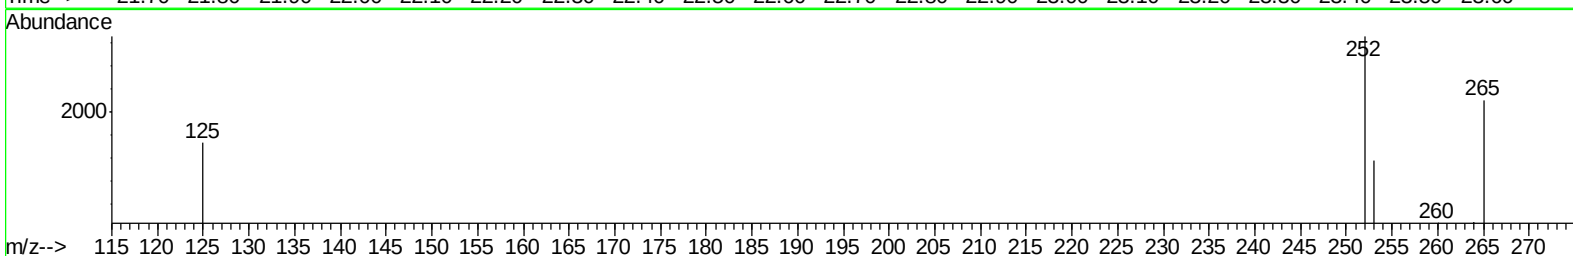


Data File : BN009078.D
Acq On : 20 Dec 2019 21:38
Operator : JU
Sample : K6171-17DL 5X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Quant Time: Dec 20 23:33:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

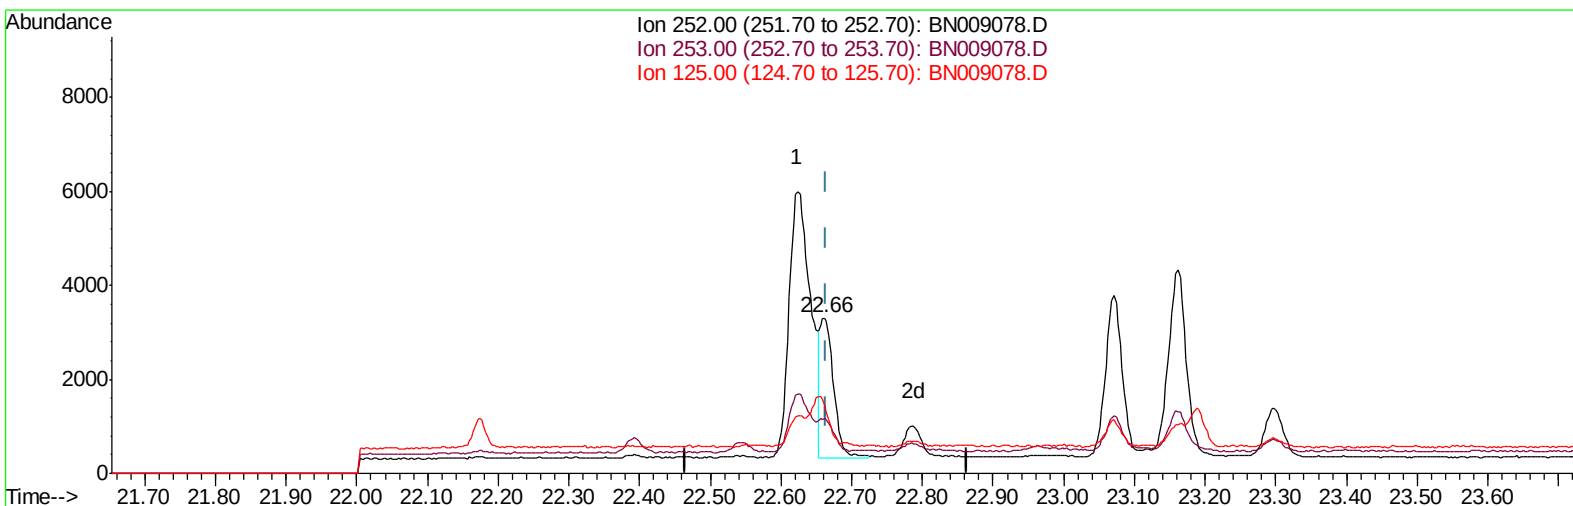

TIC: BN009078.D

(22) Benzo(k)fluoranthene

22.662min (-0.003) 0.10ng/ul m

response 3878

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	35.19#
125.00	15.50	44.06#
0.00	0.00	0.00