
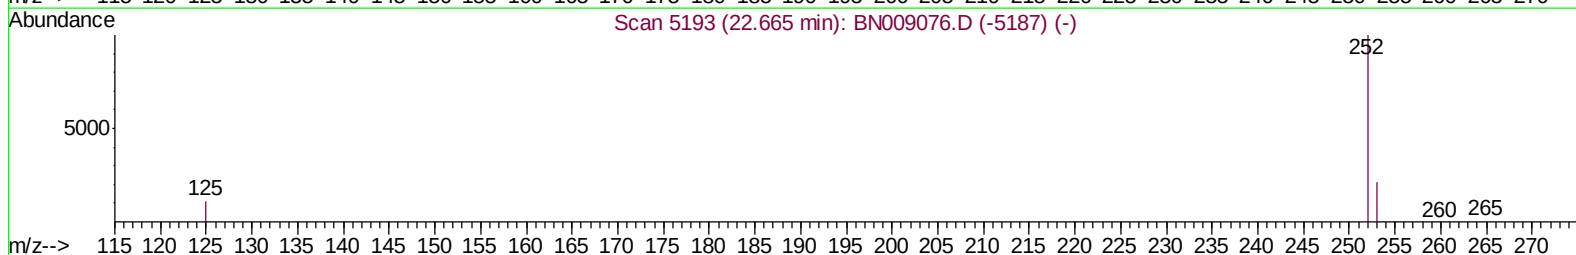
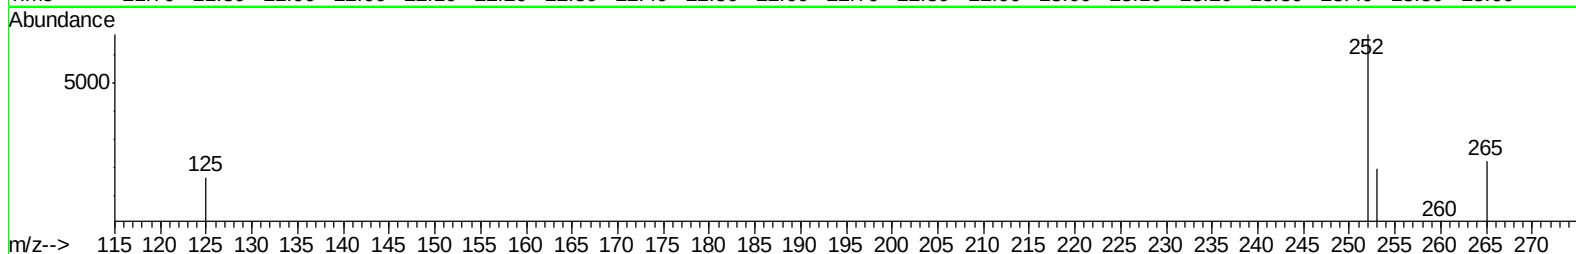


Data File : BN009079.D
Acq On : 20 Dec 2019 22:14
Operator : JU
Sample : K6171-18DL 5X
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Dec 20 23:33:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

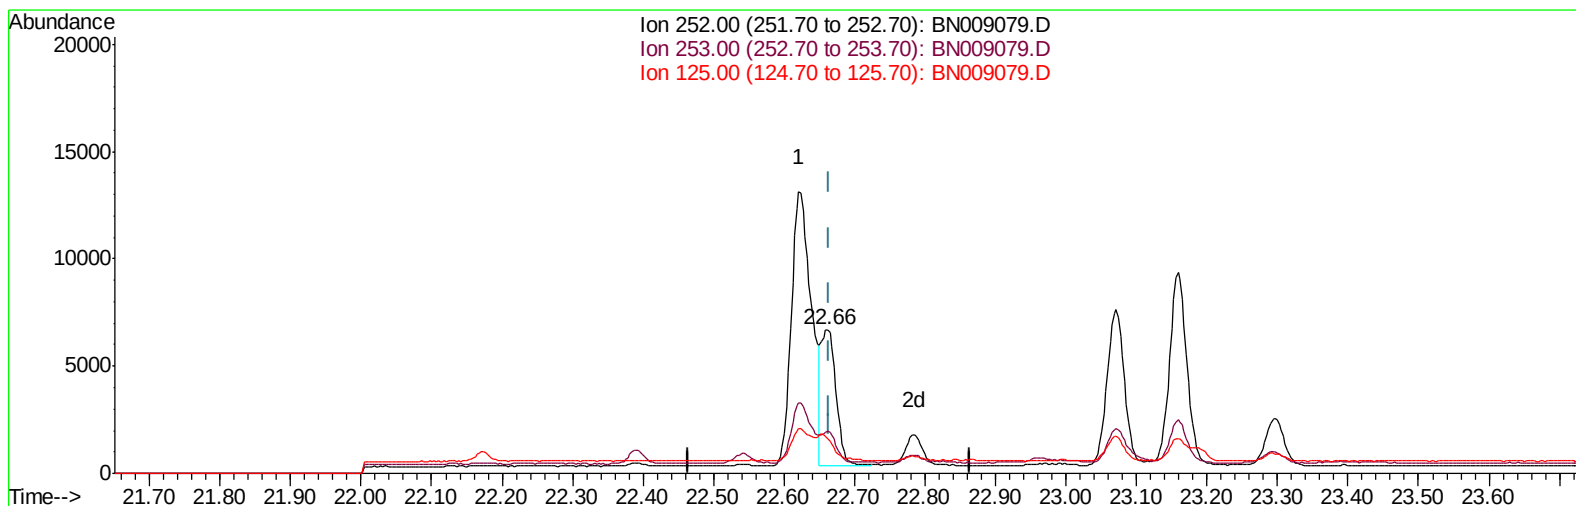

TIC: BN009079.D

(22) Benzo(k)fluoranthene

22.662min (-0.003) 0.24ng/ul m

response 9163

Ion	Exp%	Act%
252.00	100	100
253.00	24.20	28.94
125.00	15.50	24.40#
0.00	0.00	0.00