
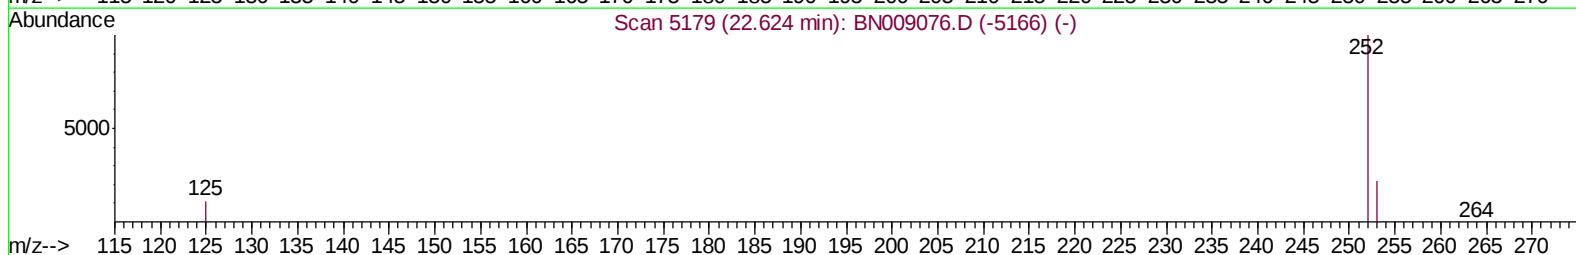
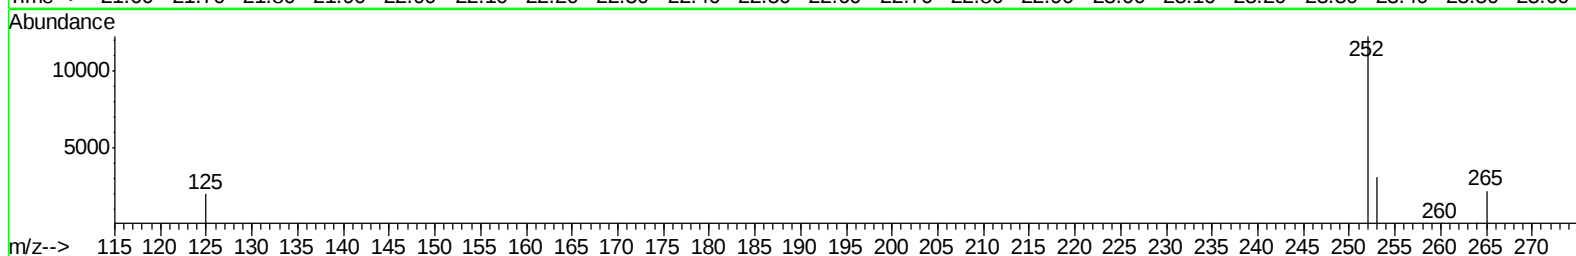


Data File : BN009080.D
Acq On : 20 Dec 2019 22:49
Operator : JU
Sample : K6171-19DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Dec 20 23:33:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 23:31:06 2019
Response via : Initial Calibration

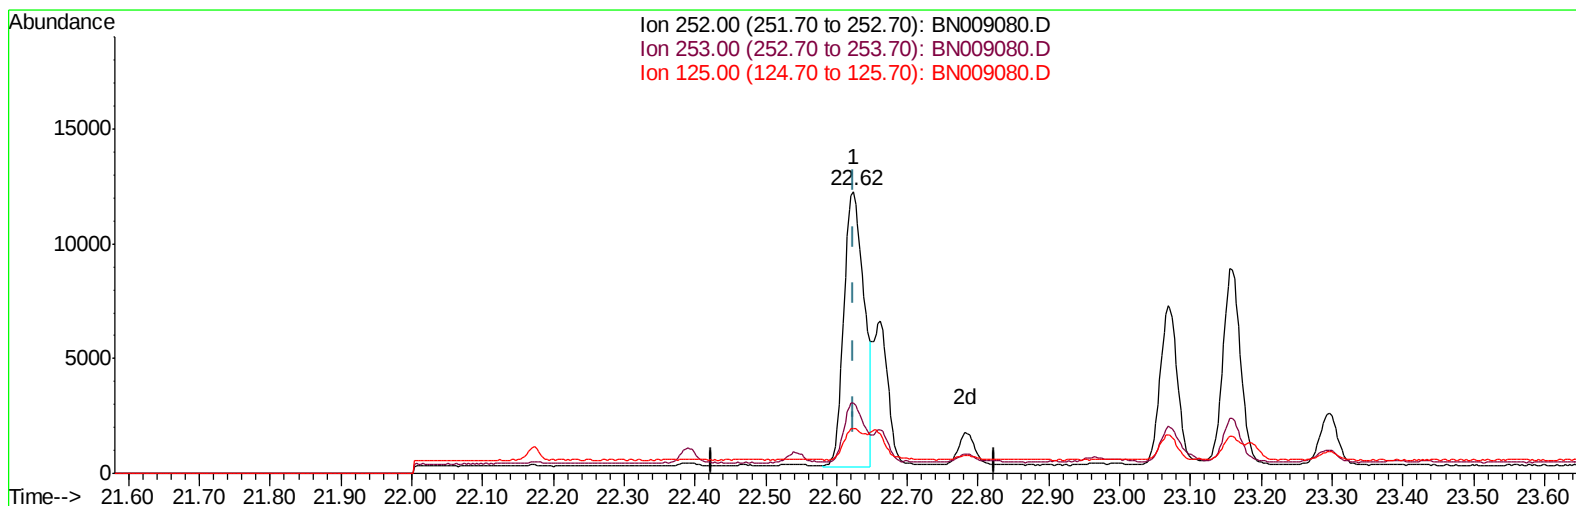

TIC: BN009080.D

(21) Benzo(b)fluoranthene

22.624min (+0.000) 0.65ng/ul m

response 23656

Ion	Exp%	Act%
252.00	100	100
253.00	24.10	25.20
125.00	15.00	16.04
0.00	0.00	0.00