

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009032.D
 Acq On : 19 Dec 2019 16:30
 Operator : JU
 Sample : K6171-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 20 05:05:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	2767	0.40	ng/ul	0.00
2) Naphthalene-d8	10.30	136	10598	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	6476	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.92
16) Chrysene-d12	21.12	240	9719	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8261	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	4584	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	13478	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.32	202	2003	0.040	ng/ul#	1
23) Benzo(a)pyrene	23.13	252	2836	0.084	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009032.D
Acq On : 19 Dec 2019 16:30
Operator : JU
Sample : K6171-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 20 05:05:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration

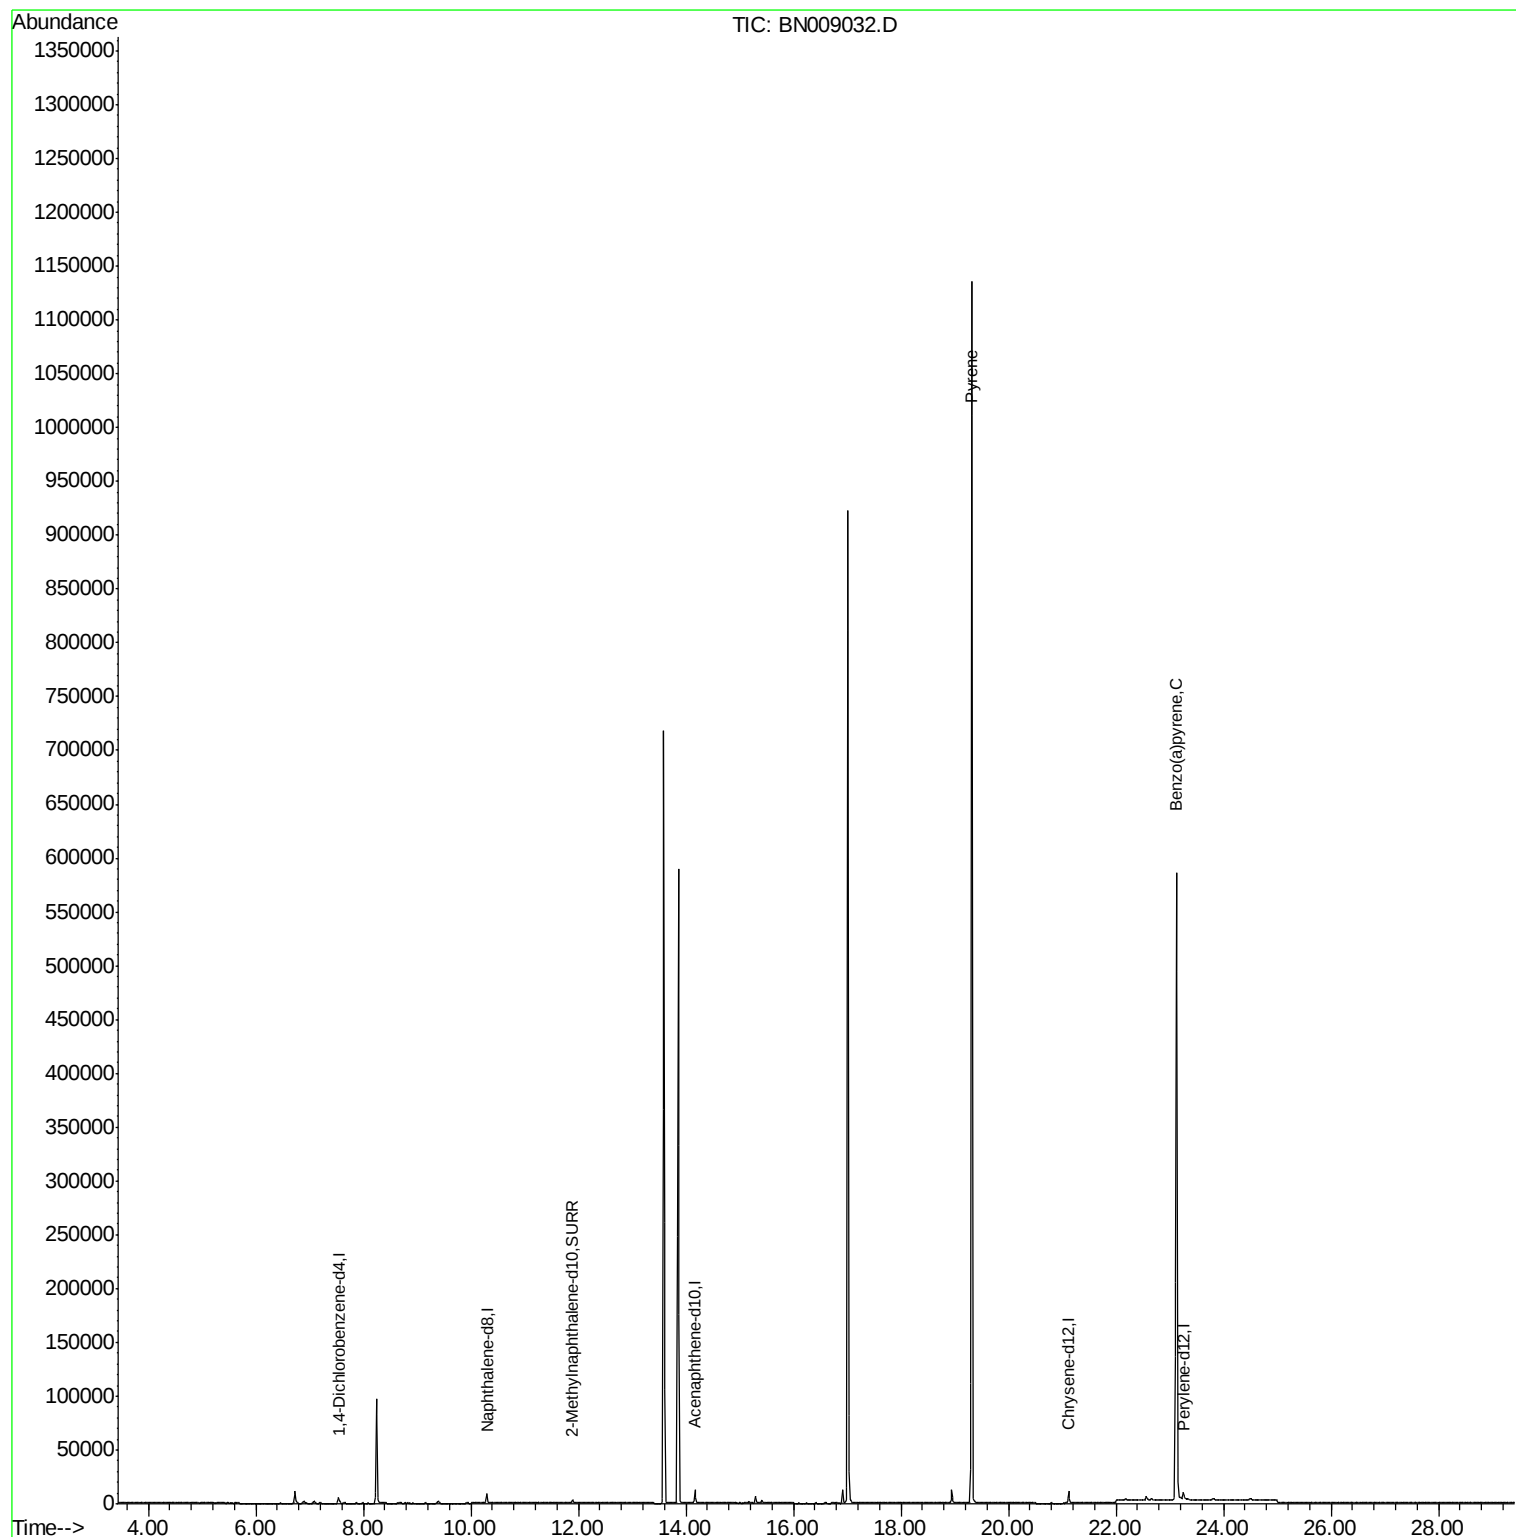

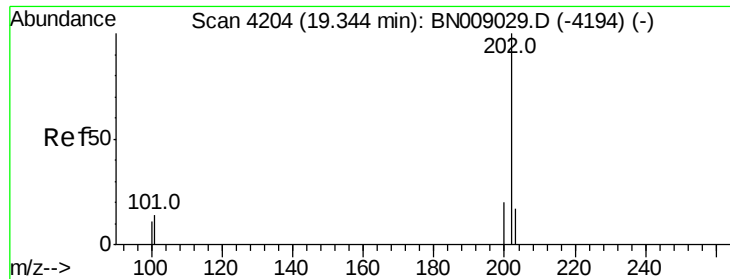

#17

Pvrene

Concen: 0.040 ng/ul

RT: 19.32 min Scan# 4198

Delta R.T. -0.03 min

Lab File: BN009032.D

Acq: 19 Dec 2019 16:30

Instrument :

BNA_N

ClientSampleId :


Tot Ion:202 Resp: 2003

Ion Ratio Lower Upper

202 100

101 167.9 10.9 16.3#




100 1139.9 9.0 13.6#

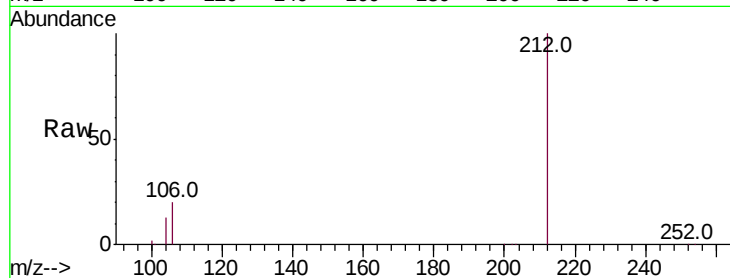

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

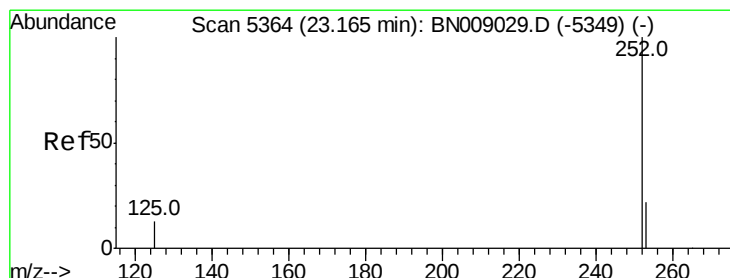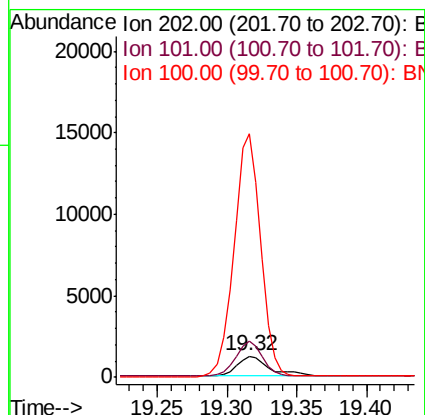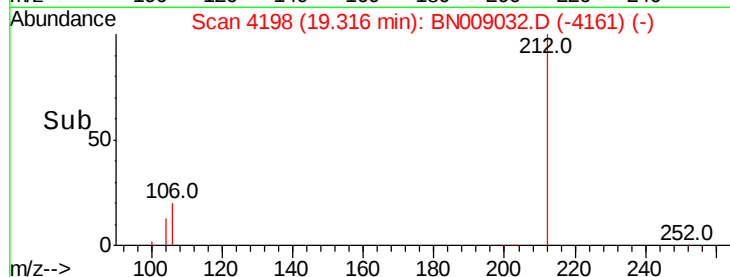

#23

Benzo(a)pyrene

Concen: 0.084 ng/ul

RT: 23.13 min Scan# 5351

Delta R.T. -0.04 min

Lab File: BN009032.D

Acq: 19 Dec 2019 16:30


Tgt Ion:252 Resp: 2836

Ion Ratio Lower Upper

252 100

253 46.1 20.2 30.4#

125 47.3 13.2 19.8#

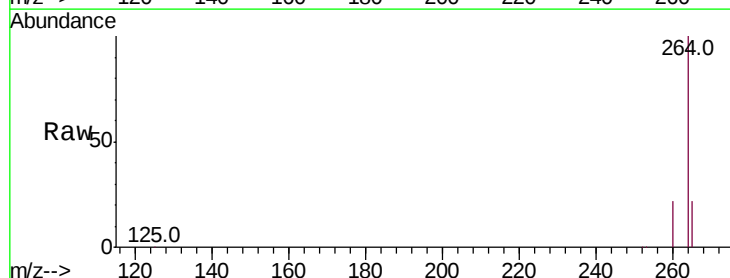

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

