

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009033.D
 Acq On : 19 Dec 2019 17:05
 Operator : JU
 Sample : K6171-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 20 05:05:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3048	0.40	ng/ul	0.00
2) Naphthalene-d8	10.30	136	12086	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	7441	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.92
16) Chrysene-d12	21.12	240	9614	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8686	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	5276	0.25	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	13130	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.32	202	2130	0.043	ng/ul#	1
23) Benzo(a)pyrene	23.13	252	2821	0.079	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009033.D
Acq On : 19 Dec 2019 17:05
Operator : JU
Sample : K6171-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 20 05:05:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration




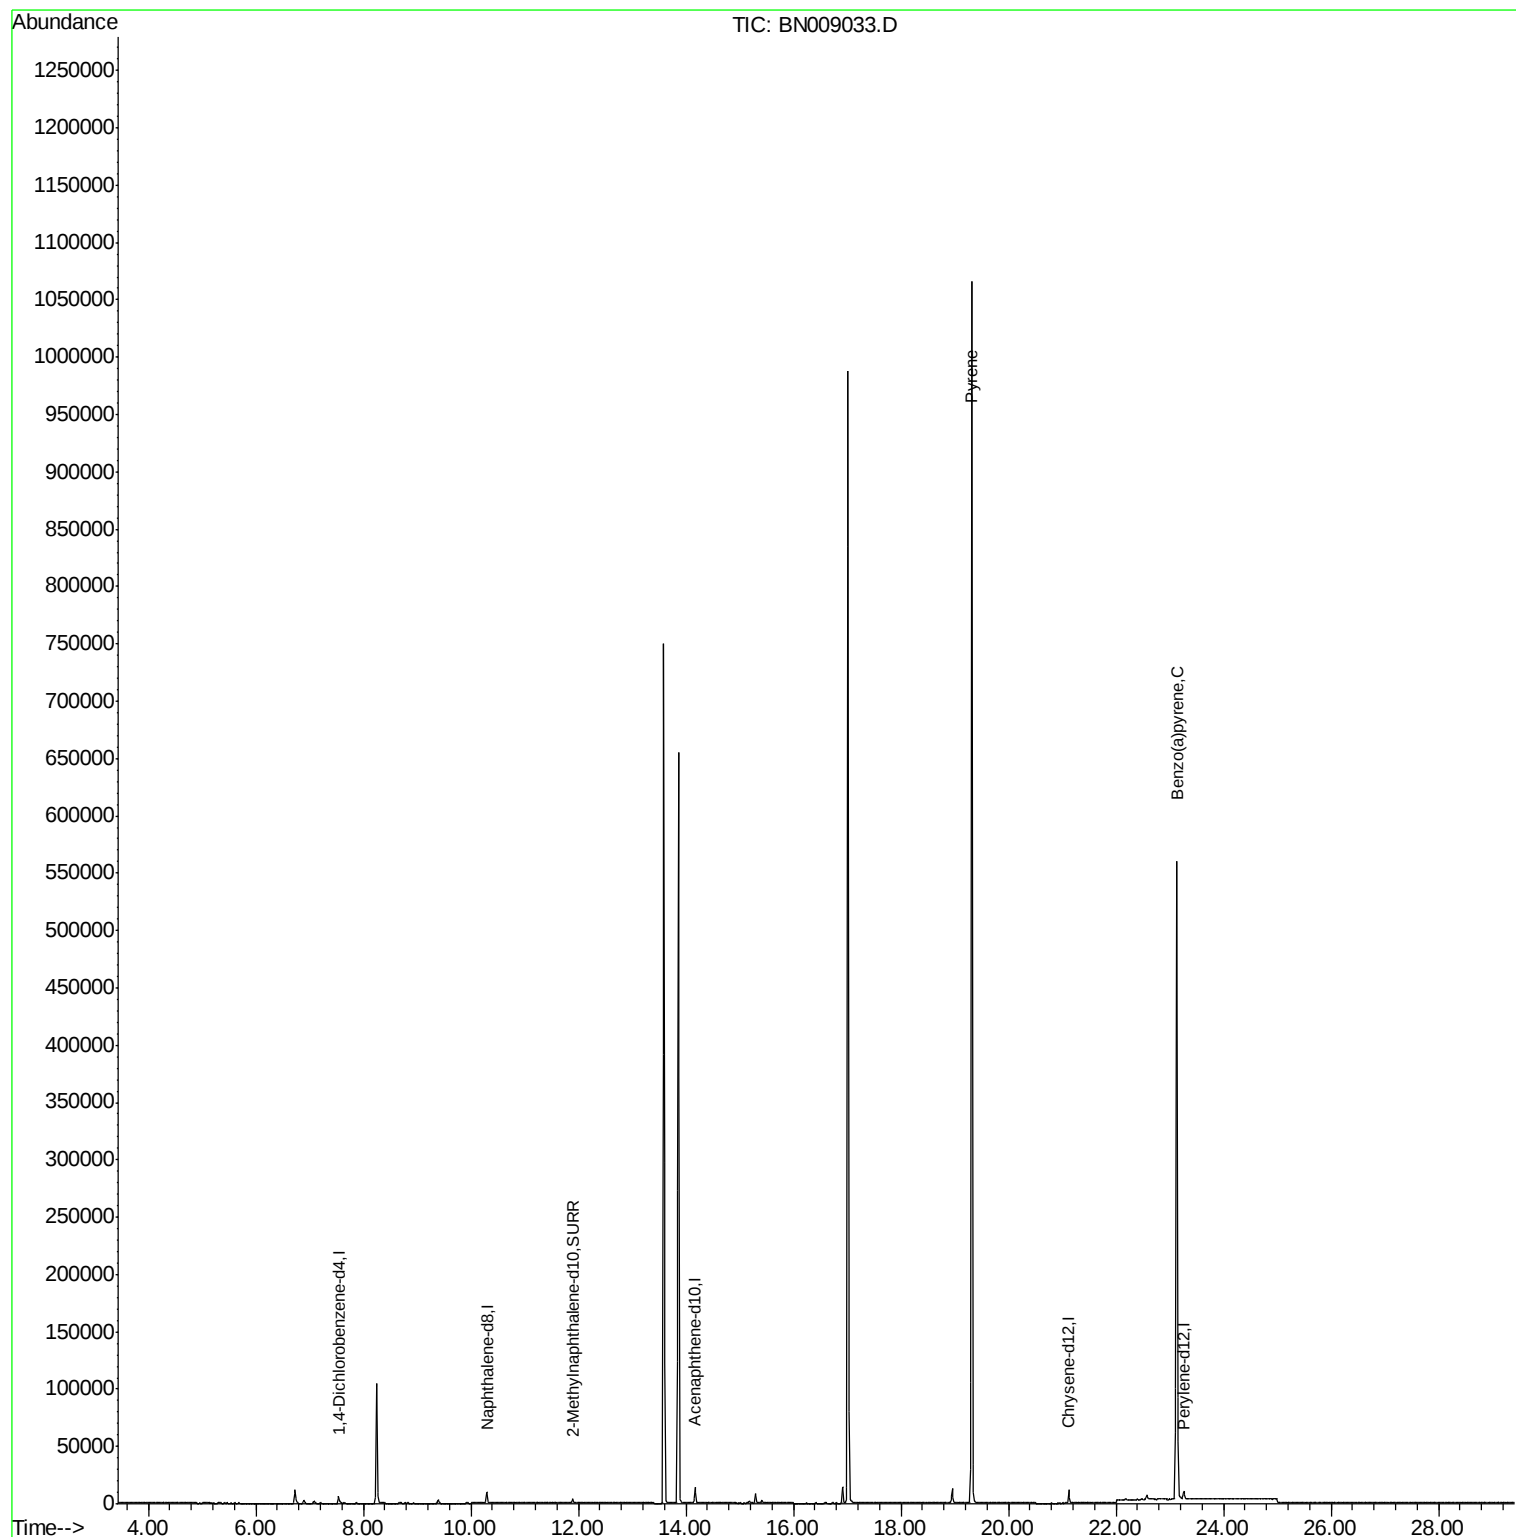


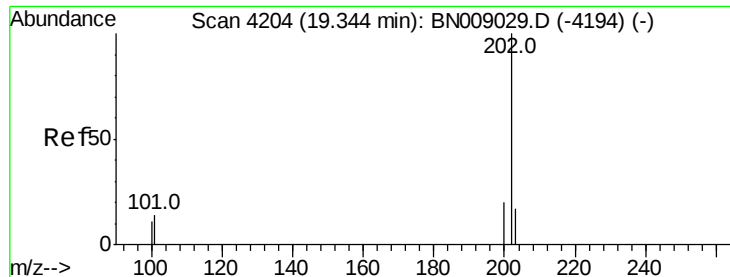

#17
Pvrene
Concen: 0.043 ng/ul
RT: 19.32 min Scan# 4198
Delta R.T. -0.03 min
Lab File: BN009033.D
Acq: 19 Dec 2019 17:05

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 2130
Ion Ratio Lower Upper
202 100
101 175.8 10.9 16.3#
100 1196.7 9.0 13.6#

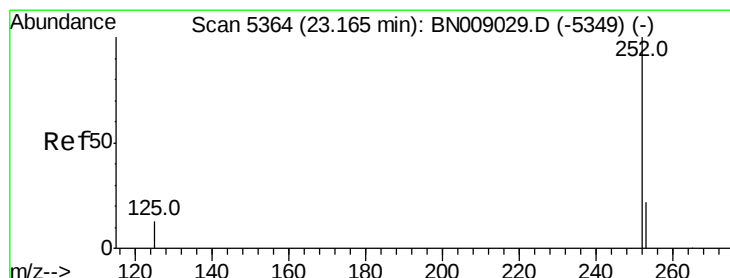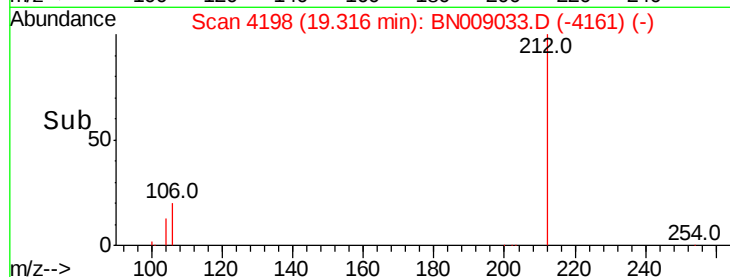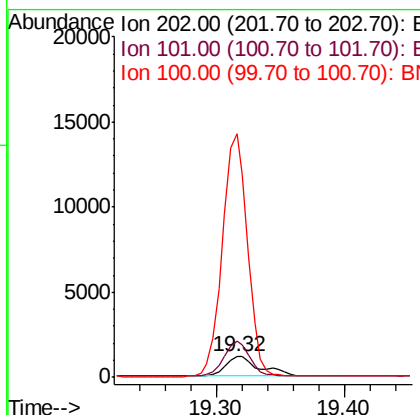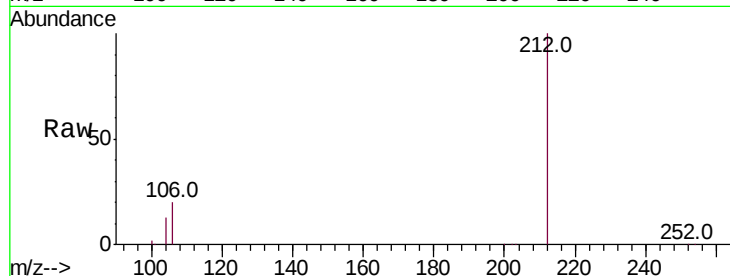

#23
Benzo(a)pyrene
Concen: 0.079 ng/ul
RT: 23.13 min Scan# 5352
Delta R.T. -0.04 min
Lab File: BN009033.D
Acq: 19 Dec 2019 17:05

Tgt Ion:252 Resp: 2821
Ion Ratio Lower Upper
252 100
253 46.7 20.2 30.4#
125 48.6 13.2 19.8#

