

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009034.D
 Acq On : 19 Dec 2019 17:41
 Operator : JU
 Sample : K6171-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 20 05:05:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3002	0.40	ng/ul	0.00
2) Naphthalene-d8	10.30	136	11870	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	7271	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.92
16) Chrysene-d12	21.12	240	10012	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8763	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	4958	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	13074	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.32	202	1949	0.038	ng/ul#	1
23) Benzo(a)pyrene	23.13	252	2614	0.073	ng/ul#	45


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009034.D
Acq On : 19 Dec 2019 17:41
Operator : JU
Sample : K6171-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 20 05:05:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration

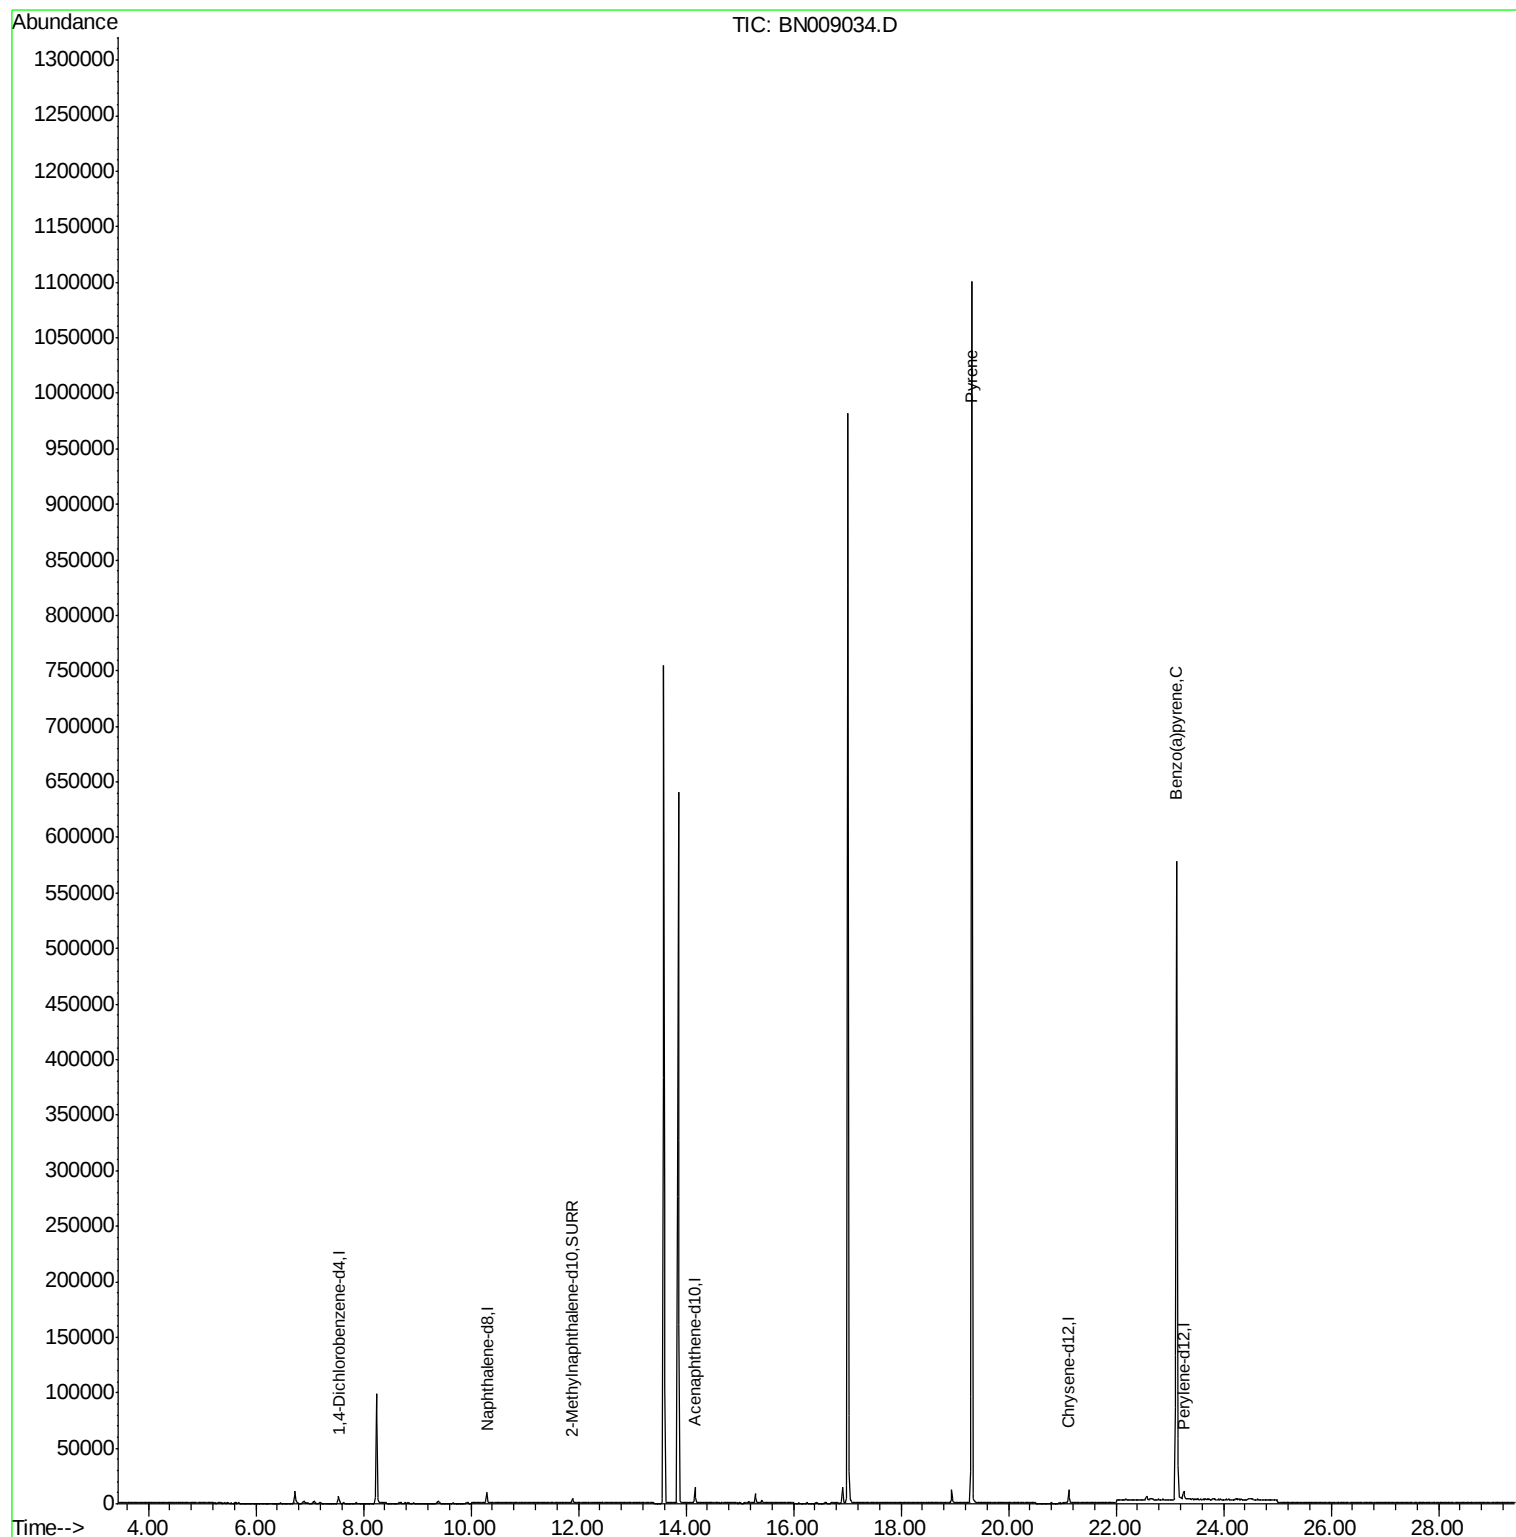


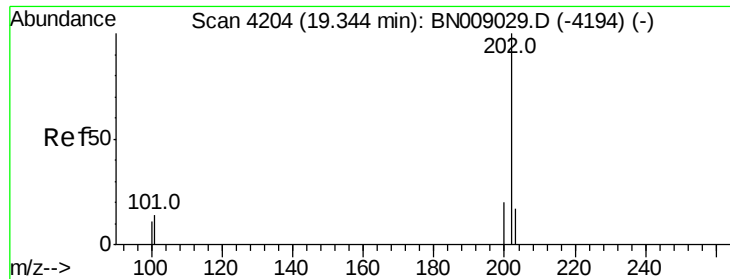




#17
Pvrene
Concen: 0.038 ng/ul
RT: 19.32 min Scan# 4198
Delta R.T. -0.03 min
Lab File: BN009034.D
Acq: 19 Dec 2019 17:41

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 1949
Ion Ratio Lower Upper
202 100
101 165.0 10.9 16.3#
100 1138.2 9.0 13.6#

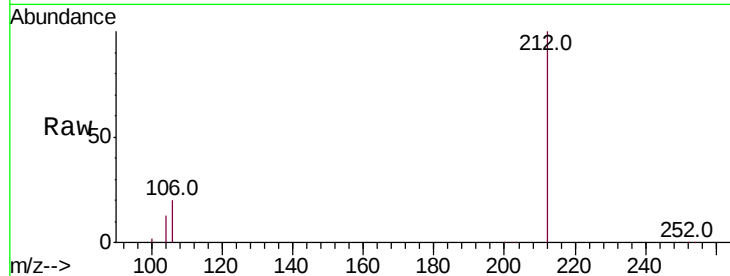


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): B

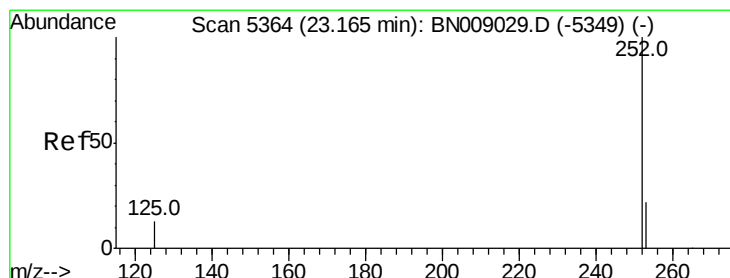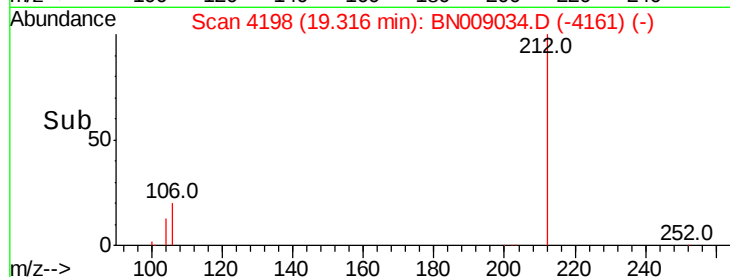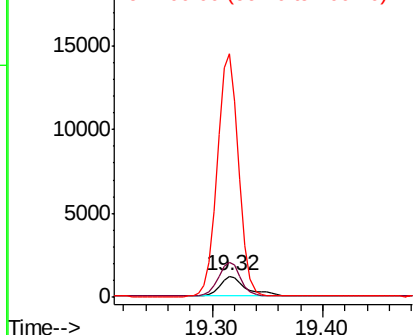

#23
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.13 min Scan# 5352
Delta R.T. -0.04 min
Lab File: BN009034.D
Acq: 19 Dec 2019 17:41

Tgt Ion:252 Resp: 2614
Ion Ratio Lower Upper
252 100
253 47.1 20.2 30.4#
125 48.3 13.2 19.8#

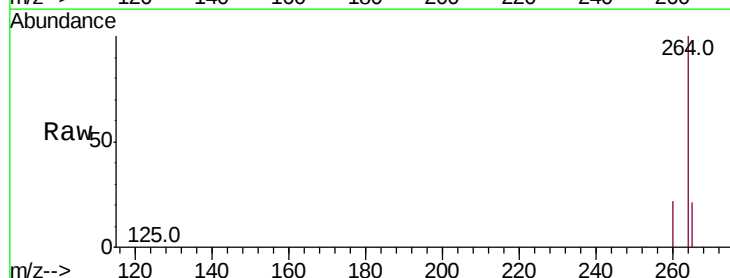

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

