

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009044.D
 Acq On : 19 Dec 2019 23:38
 Operator : JU
 Sample : K6170-20
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 20 05:06:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3292	0.40	ng/ul	0.00
2) Naphthalene-d8	10.29	136	13146	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	8058	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.92
16) Chrysene-d12	21.12	240	11508	0.40	ng/ul	0.00
20) Perylene-d12	23.25	264	10075	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	5823	0.25	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	14533	0.00	ng/ul	0.00
Target Compounds						
9) Fluorene	15.17	166	2008	0.051	ng/ul#	14
17) Pyrene	19.32	202	1905	0.032	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009044.D
Acq On : 19 Dec 2019 23:38
Operator : JU
Sample : K6170-20
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 20 05:06:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration

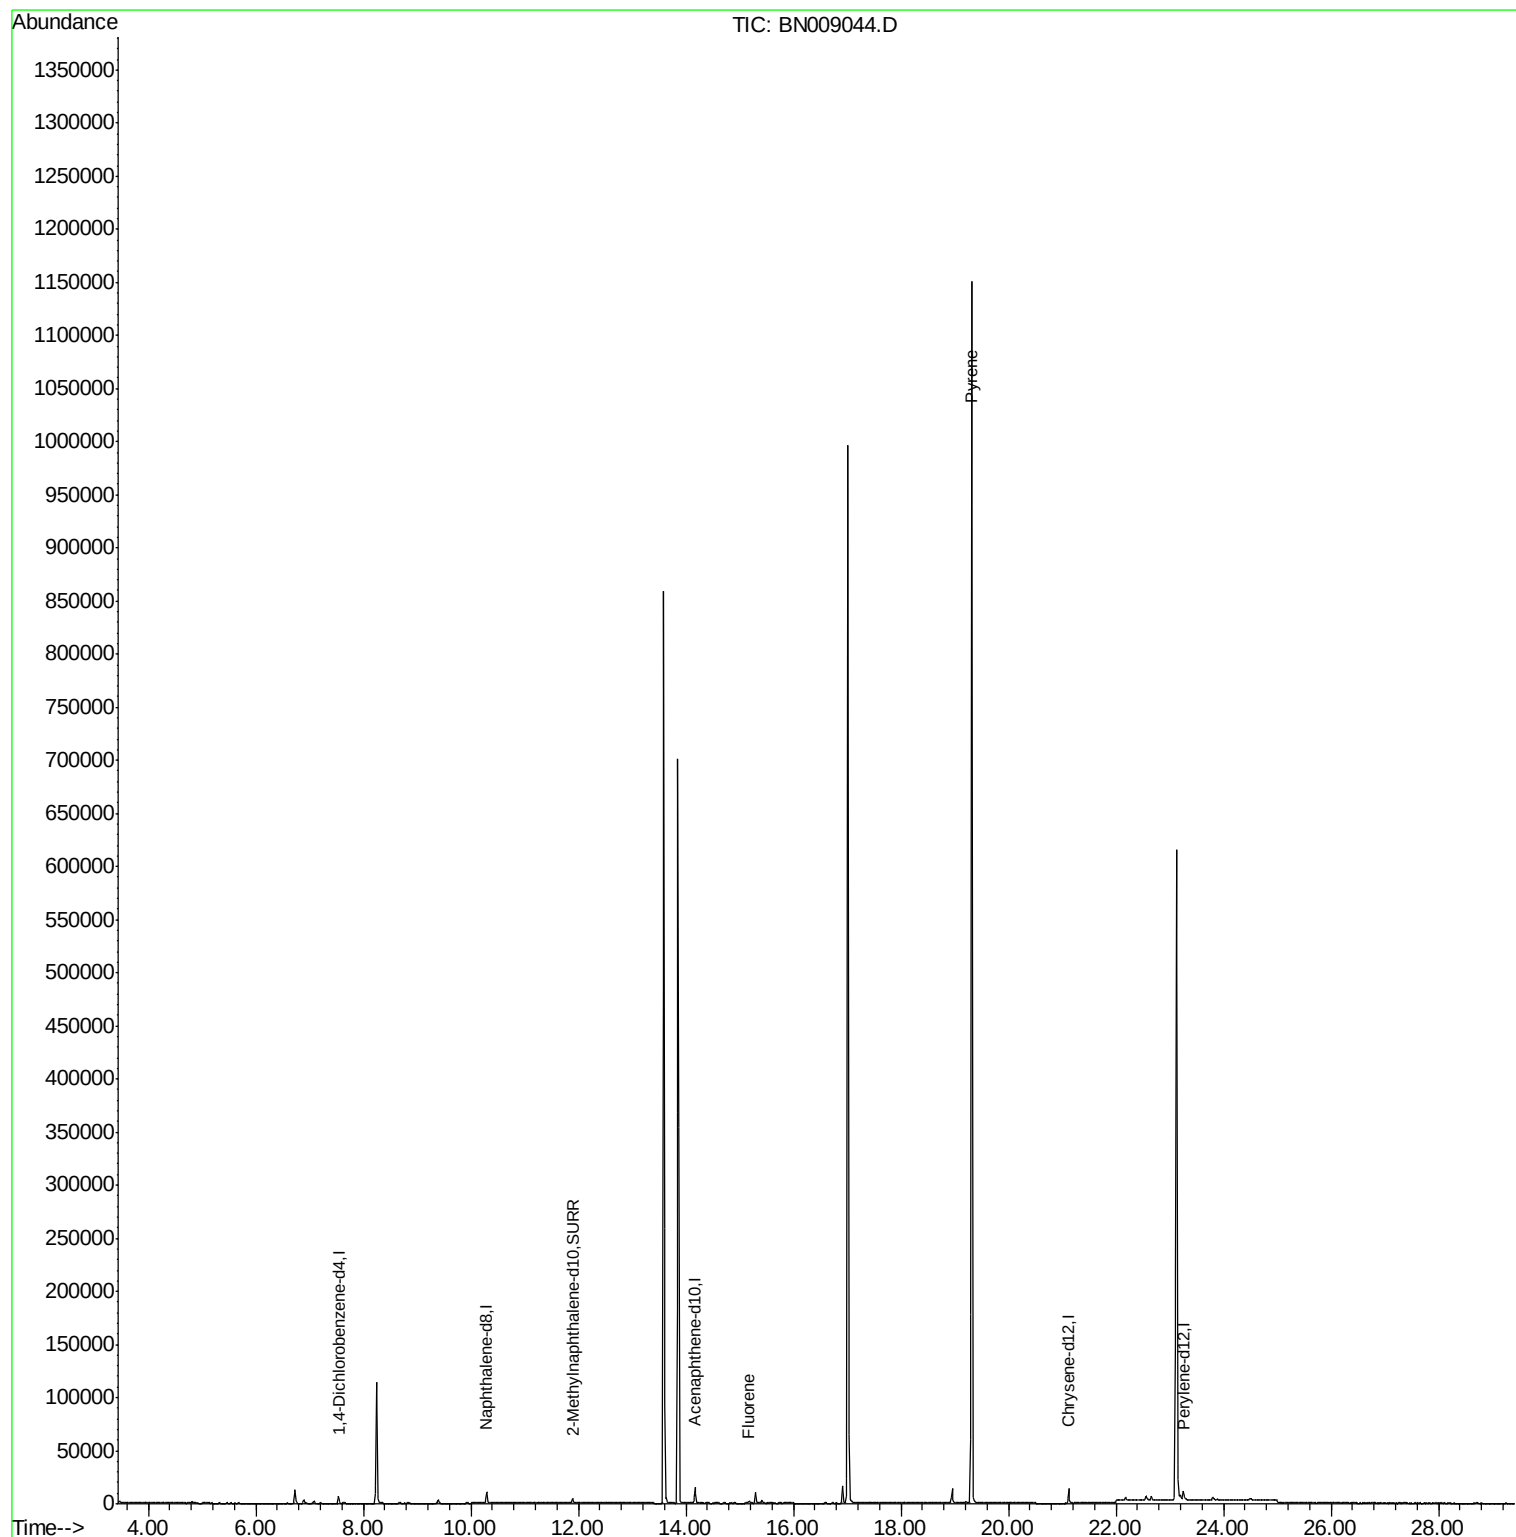

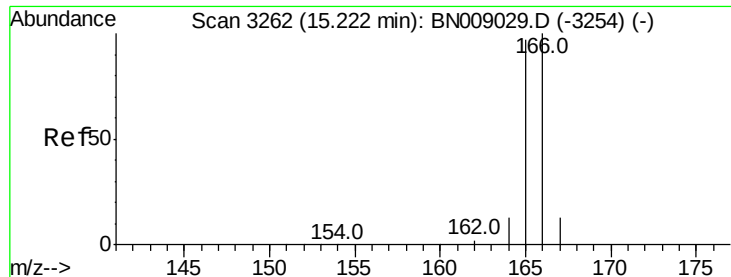

#9

Fluorene

Concen: 0.051 ng/ul

RT: 15.17 min Scan# 3251

Delta R.T. -0.05 min

Lab File: BN009044.D

Acq: 19 Dec 2019 23:38

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 2008

Ion Ratio Lower Upper

166 100

165 9.3 78.2 117.4#

167 37.2 11.0 16.6#

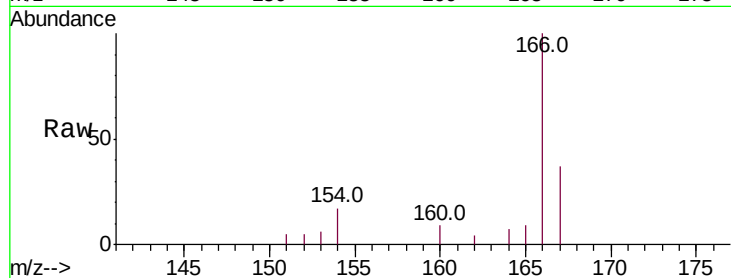


Abundance



Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

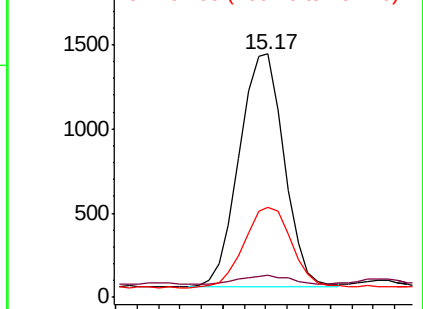

Time--> 15.10 15.15 15.20

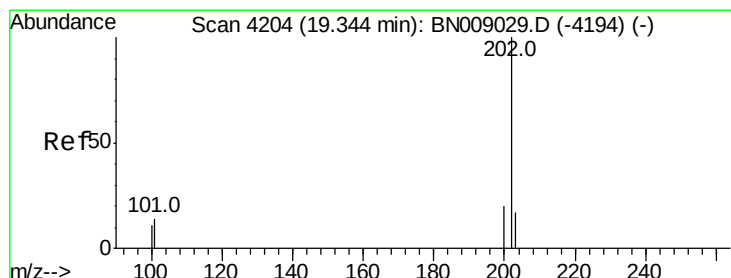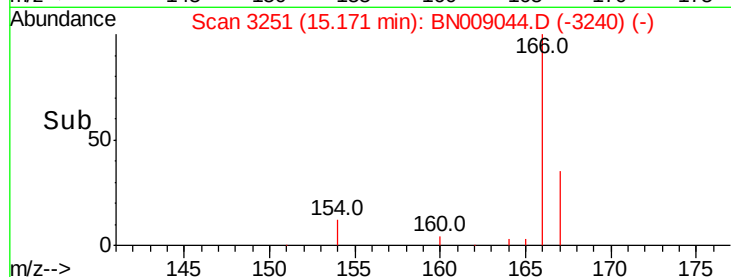

#17

Pyrene

Concen: 0.032 ng/ul

RT: 19.32 min Scan# 4198

Delta R.T. -0.03 min

Lab File: BN009044.D

Acq: 19 Dec 2019 23:38


Tgt Ion:202 Resp: 1905

Ion Ratio Lower Upper

202 100

101 170.4 10.9 16.3#

100 1087.6 9.0 13.6#

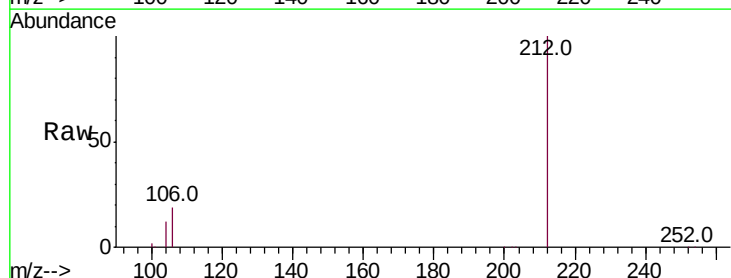


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

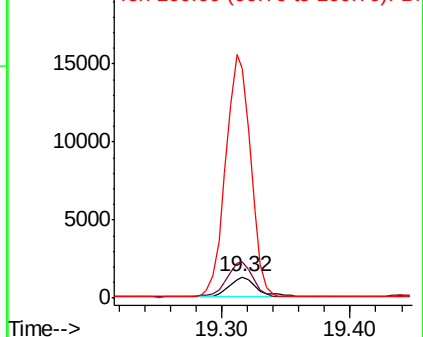

Time--> 19.30 19.40

