

Data File : BN009070.D
Acq On : 20 Dec 2019 16:17
Operator : JU
Sample : K6171-10DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BT2DL

Quant Time: Dec 20 22:58:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	4160	0.40	ng/ul	0.00
2) Naphthalene-d8	10.29	136	15872	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	8501	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.91	188	16715	0.40	ng/ul	0.00
16) Chrysene-d12	21.12	240	9228	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8720	0.40	ng/ul	0.00

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.89	152	786	0.03	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	1635	0.03	ng/ul	0.00


Target Compounds				Qvalue		
12) Phenanthrene	16.95	178	22992	0.396	ng/ul	99
13) Anthracene	17.04	178	4105	0.079	ng/ul	95
15) Fluoranthene	18.98	202	76080	1.144	ng/ul	98
17) Pyrene	19.34	202	60699	1.289	ng/ul	97
18) Benzo(a)anthracene	21.10	228	25131	0.613	ng/ul	98
19) Chrysene	21.15	228	25761	0.626	ng/ul	97
21) Benzo(b)fluoranthene	22.63	252	41529	1.020	ng/ul	98
22) Benzo(k)fluoranthene	22.63	252	41529	1.012	ng/ul	98
23) Benzo(a)pyrene	23.16	252	20437	0.573	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	25.35	276	14366	0.370	ng/ul#	91
25) Dibenzo(a,h)anthracene	25.36	278	3244	0.105	ng/ul#	69
26) Benzo(g,h,i)perylene	25.99	276	14007	0.428	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009070.D
Acq On : 20 Dec 2019 16:17
Operator : JU
Sample : K6171-10DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BT2DL

Quant Time: Dec 20 22:58:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 20 22:55:30 2019
Response via : Initial Calibration

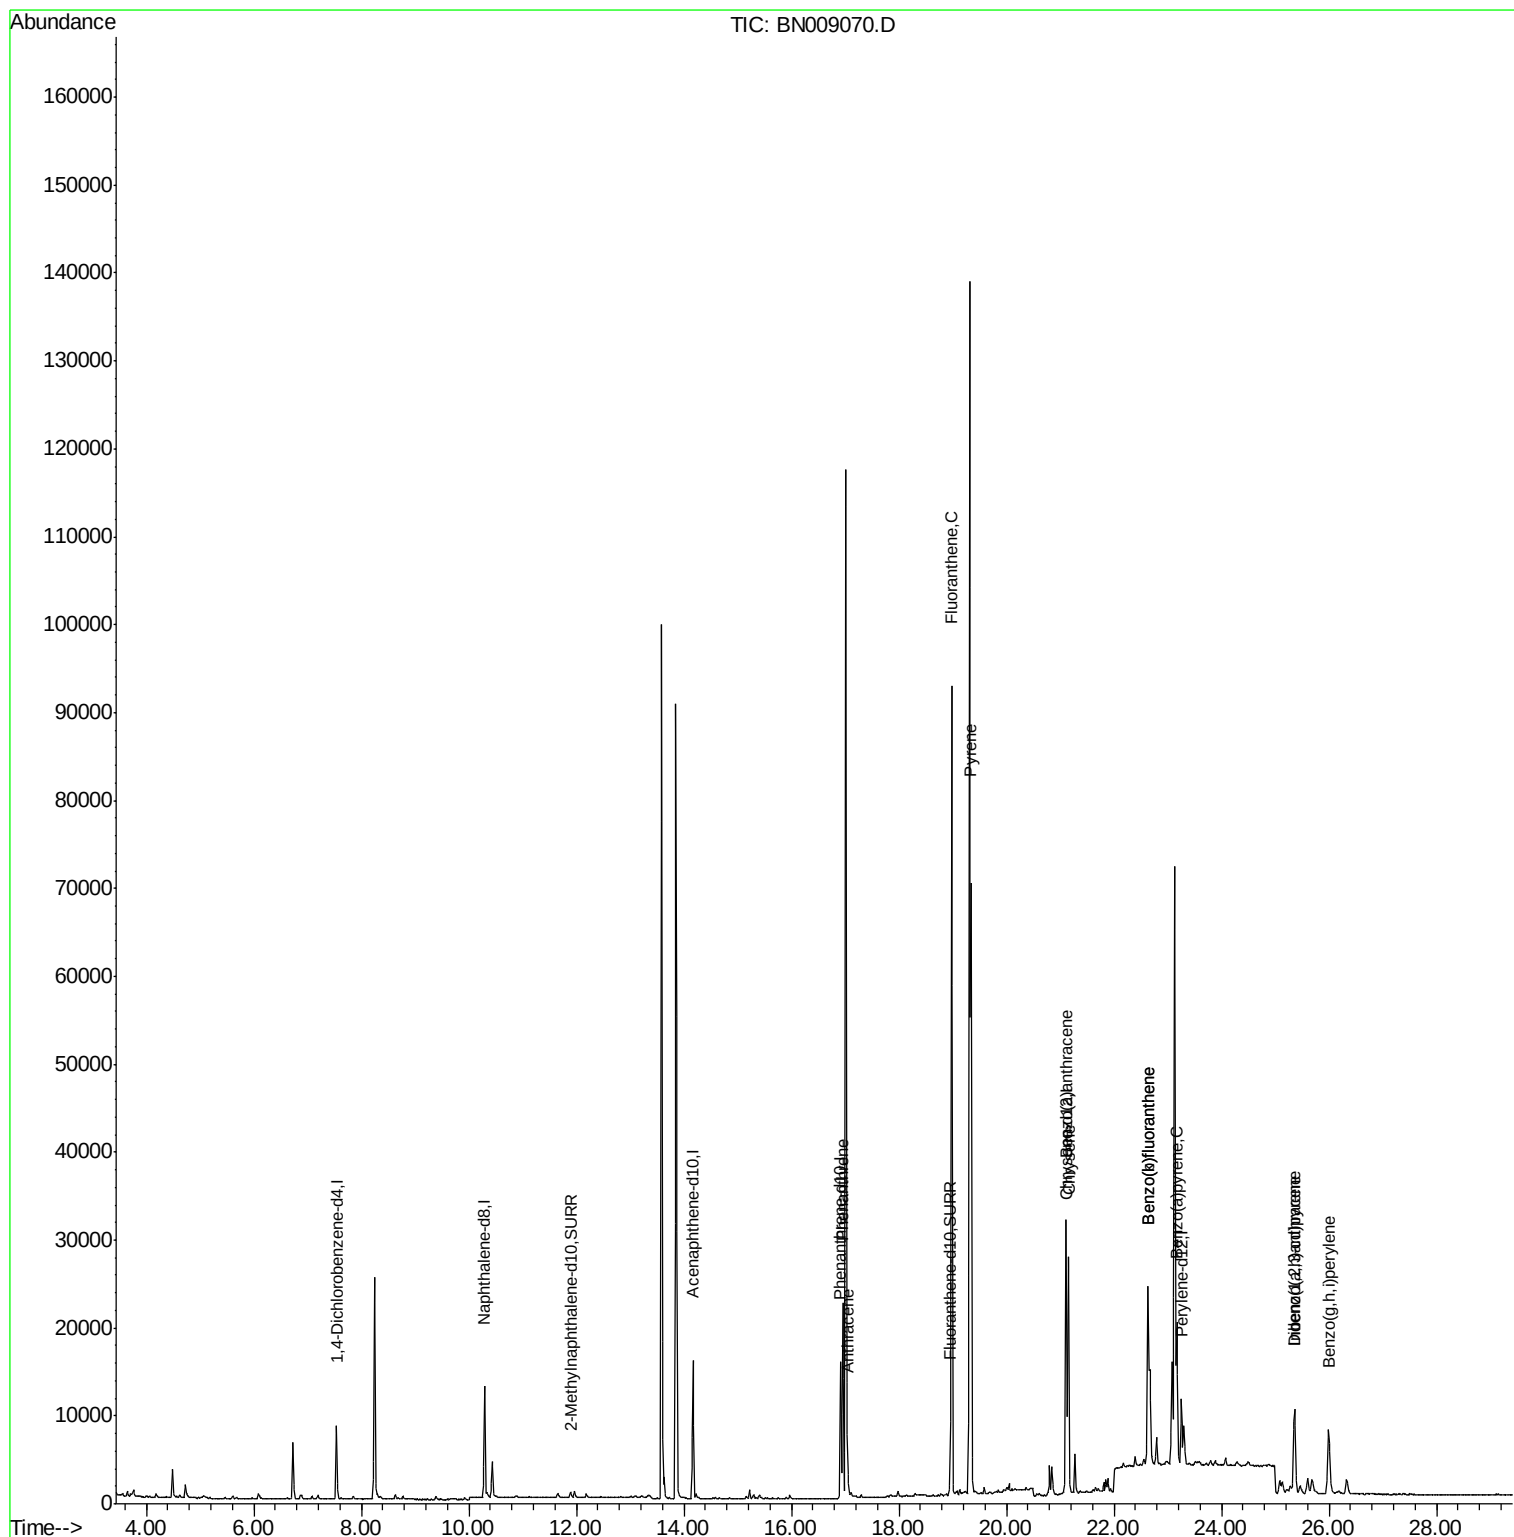



#12

Phenanthrene

Concen: 0.396 ng/ul

RT: 16.95 min Scan# 3656

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17

Instrument :

BNA_N

ClientSampleId :

C0BT2DL





Tgt Ion:178 Resp: 22992

Ion Ratio Lower Upper

178 100

179 15.9 12.3 18.5

176 18.9 15.1 22.7

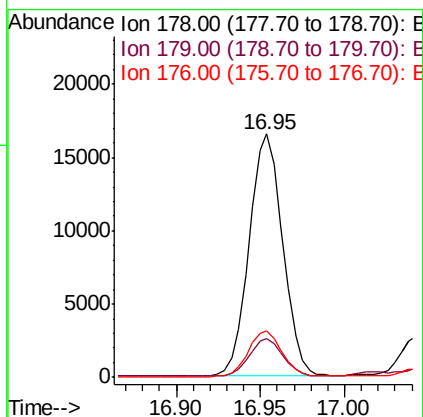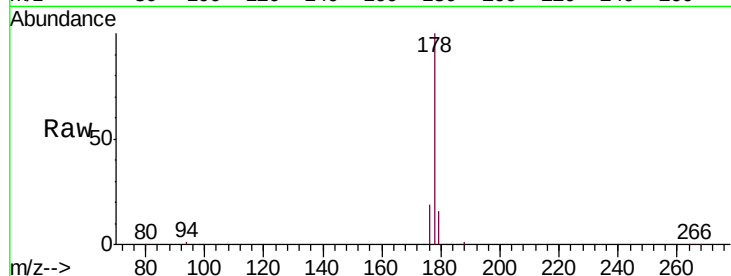

#13

Anthracene

Concen: 0.079 ng/ul

RT: 17.04 min Scan# 3677

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17




Tgt Ion:178 Resp: 4105


Ion Ratio Lower Upper

178 100

179 18.4 12.5 18.7

176 20.1 14.9 22.3

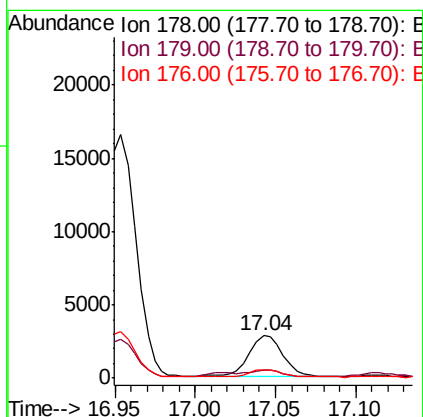

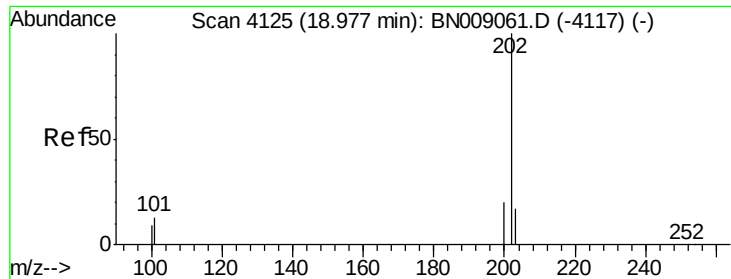

#15

Fluoranthene

Concen: 1.144 ng/ul

RT: 18.98 min Scan# 4125

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17

Instrument :

BNA_N

ClientSampleId :

C0BT2DL


Tgt Ion:202 Resp: 76080

Ion Ratio Lower Upper

202 100

101 12.3 0.0 31.5




100 9.4 0.0 28.9

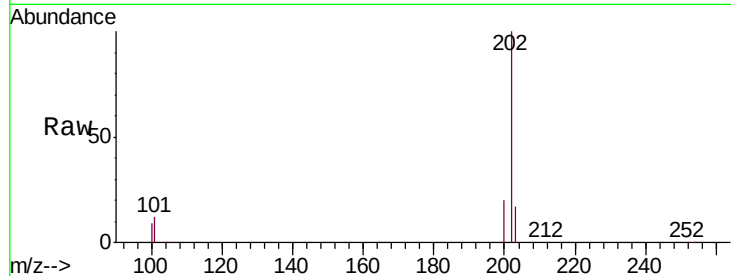

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

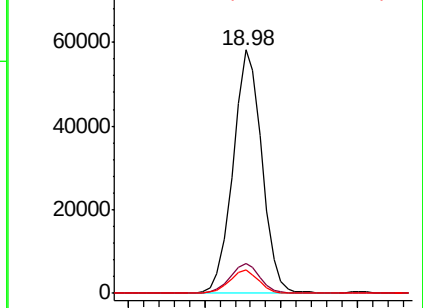

#17

Pyrene

Concen: 1.289 ng/ul

RT: 19.34 min Scan# 4203

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17


Tgt Ion:202 Resp: 60699

Ion Ratio Lower Upper

202 100

101 14.9 10.9 16.3



100 12.2 9.0 13.6




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

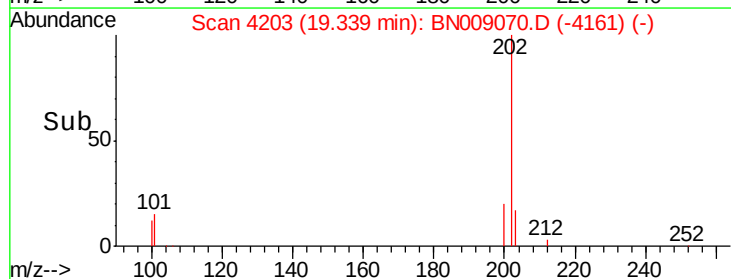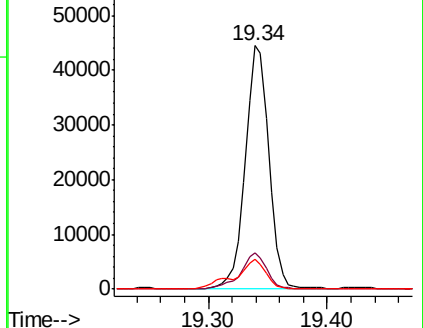

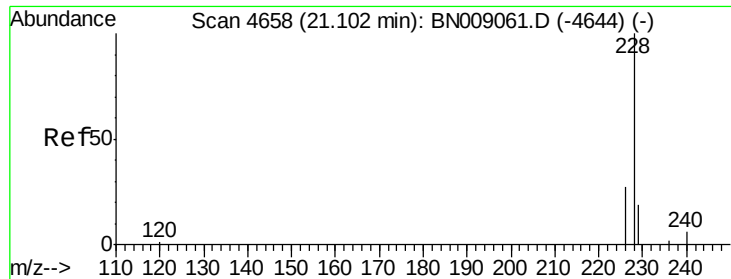

#18

Benzo(a)anthracene

Concen: 0.613 ng/ul

RT: 21.10 min Scan# 4658

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17

Instrument :

BNA_N

ClientSampleId :

C0BT2DL


Tgt Ion:228 Resp: 25131

Ion Ratio Lower Upper




228 100

229 20.4 15.5 23.3

226 28.2 21.7 32.5

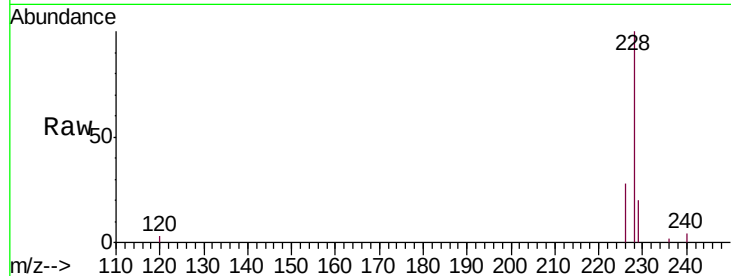

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

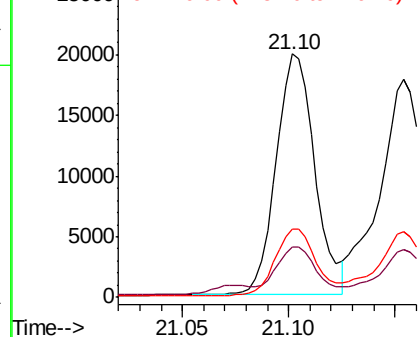

#19

Chrysene

Concen: 0.626 ng/ul

RT: 21.15 min Scan# 4676

Delta R.T. -0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17


Tgt Ion:228 Resp: 25761

Ion Ratio Lower Upper



228 100


226 30.1 23.7 35.5

229 22.2 15.4 23.0



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

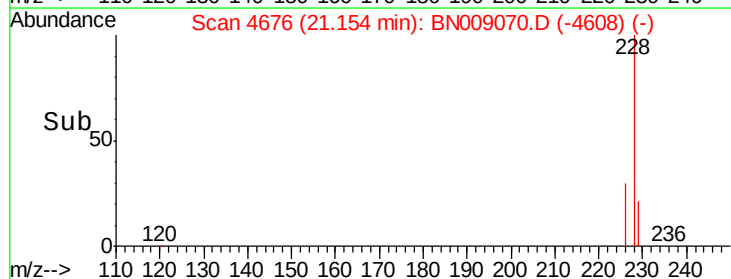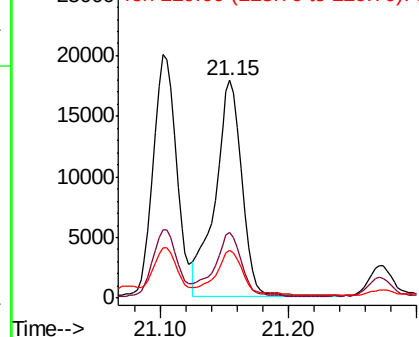

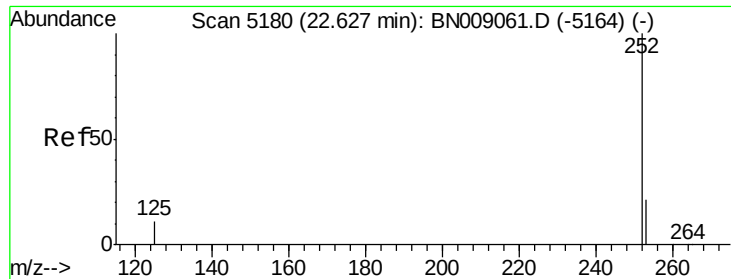

#21

Benzo(b)fluoranthene

Concen: 1.020 ng/ul

RT: 22.63 min Scan# 5181

Delta R.T. 0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17

Instrument :

BNA_N

ClientSampleId :

C0BT2DL


Tgt Ion:252 Resp: 41529

Ion Ratio Lower Upper

252 100

253 24.9 0.0 48.2




125 16.3 0.0 30.0



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

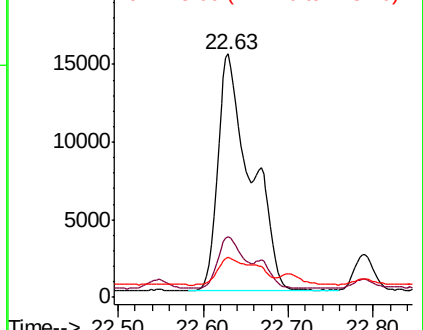

#22

Benzo(k)fluoranthene

Concen: 1.012 ng/ul

RT: 22.63 min Scan# 5181

Delta R.T. -0.04 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17


Tgt Ion:252 Resp: 41529

Ion Ratio Lower Upper

252 100

253 24.9 19.4 29.0



125 16.3 12.4 18.6




Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

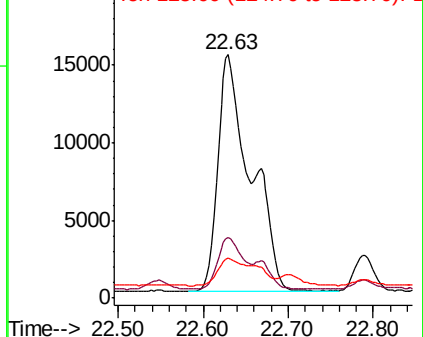

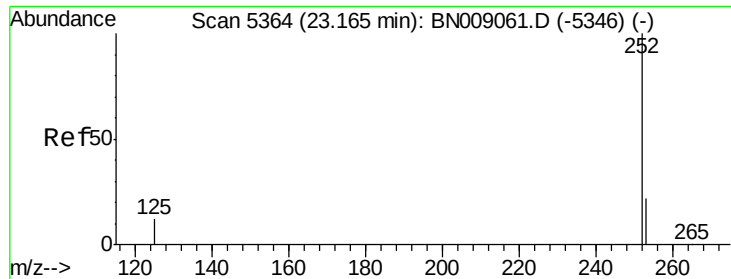

#23

Benzo(a)pyrene

Concen: 0.573 ng/ul

RT: 23.16 min Scan# 5364

Delta R.T. 0.00 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17

Instrument :

BNA_N

ClientSampleId :

C0BT2DL


Tgt Ion:252 Resp: 20437

Ion Ratio Lower Upper

252 100

253 26.3 20.2 30.4




125 18.4 13.2 19.8



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

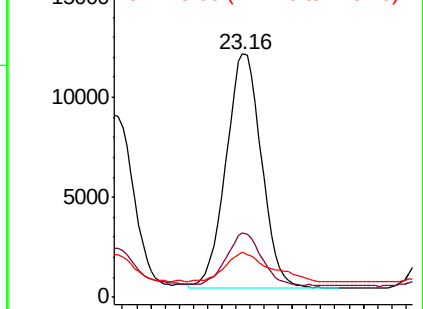

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.370 ng/ul

RT: 25.35 min Scan# 6097

Delta R.T. -0.01 min

Lab File: BN009070.D

Acq: 20 Dec 2019 16:17


Tgt Ion:276 Resp: 14366

Ion Ratio Lower Upper

276 100

138 23.4 22.4 33.6



227 0.5 0.2 0.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E




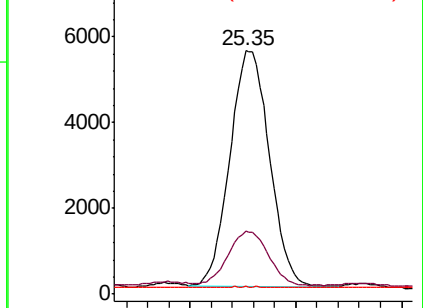




#25
Dibenzo(a,h)anthracene
Concen: 0.105 ng/ul
RT: 25.36 min Scan# 6100
Delta R.T. -0.01 min
Lab File: BN009070.D
Acq: 20 Dec 2019 16:17

Instrument :
BNA_N
ClientSampleId :
C0BT2DL

Tgt Ion: 278 Resp: 3244
Ion Ratio Lower Upper
278 100
139 34.0 16.2 24.2#
279 41.7 20.3 30.5#

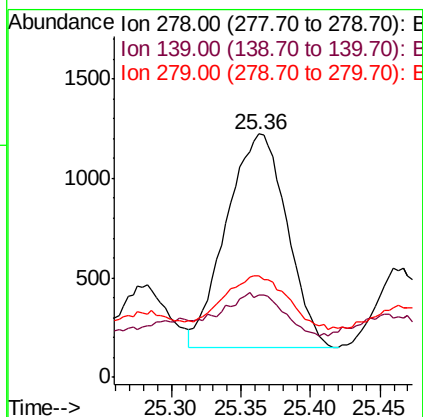

#26
Benzo(g,h,i)perylene
Concen: 0.428 ng/ul
RT: 25.99 min Scan# 6288
Delta R.T. 0.00 min
Lab File: BN009070.D
Acq: 20 Dec 2019 16:17

Tgt Ion: 276 Resp: 14007
Ion Ratio Lower Upper
276 100
138 26.9 20.6 30.8
277 25.8 19.6 29.4

