


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009032.D
Acq On : 19 Dec 2019 16:30
Operator : JU
Sample : K6170-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BR7

Manual Integrations
APPROVED

Sohil
12/20/2019 4:29:26 PM

Quant Time: Dec 20 05:39:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration

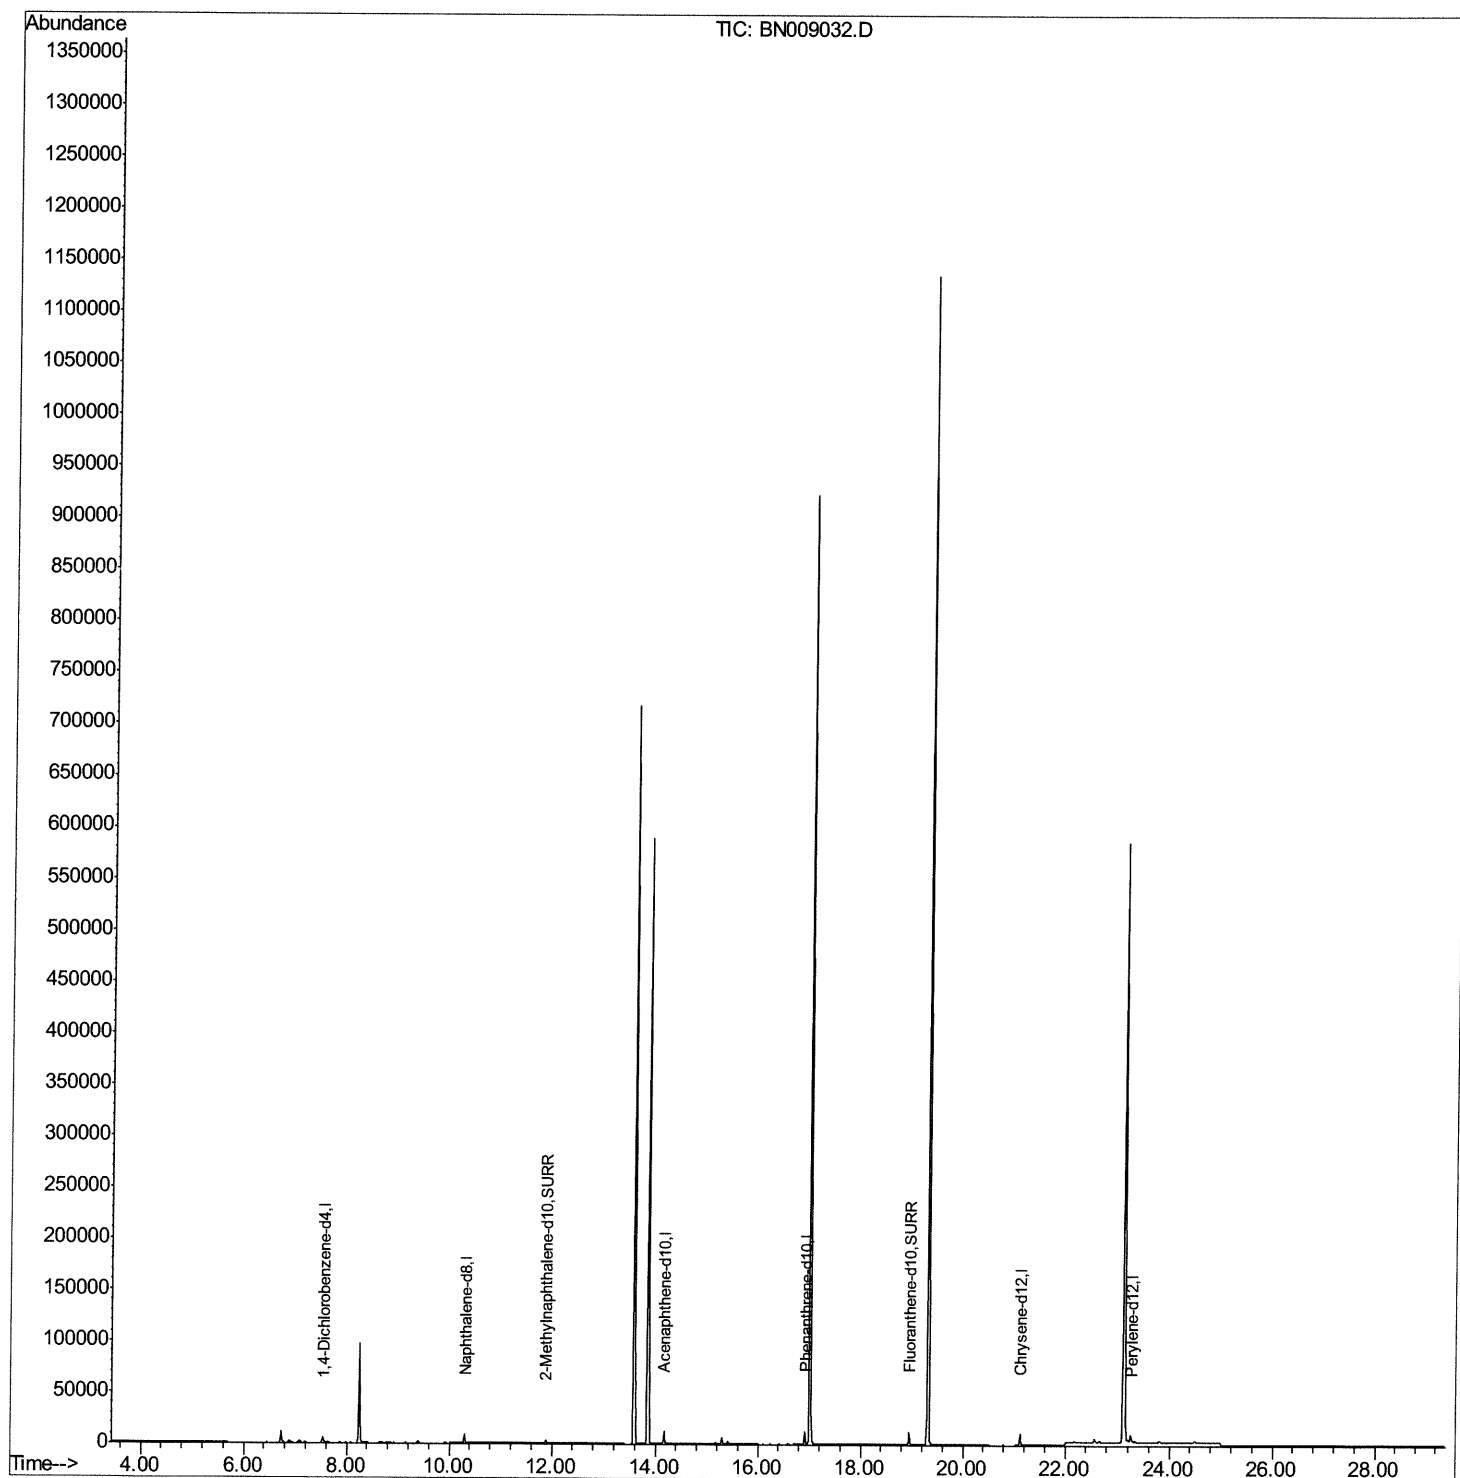

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009032.D
 Acq On : 19 Dec 2019 16:30
 Operator : JU
 Sample : K6170-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BR7

Manual Integrations
APPROVED

Sohil
 12/20/2019 4:29:26 PM

Quant Time: Dec 20 05:05:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

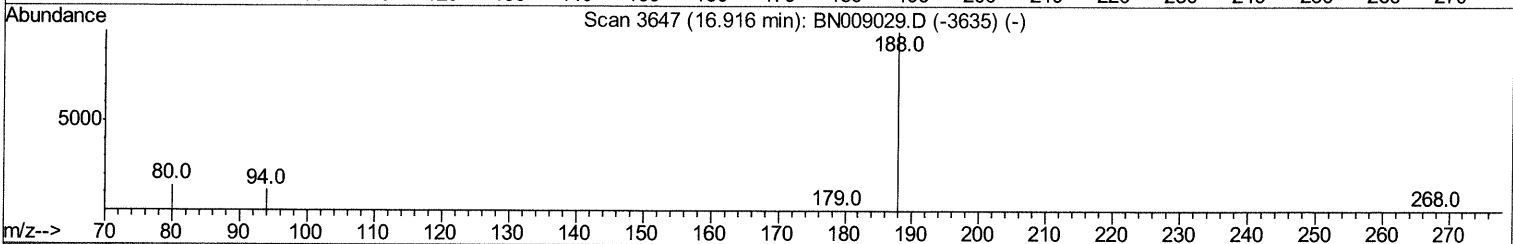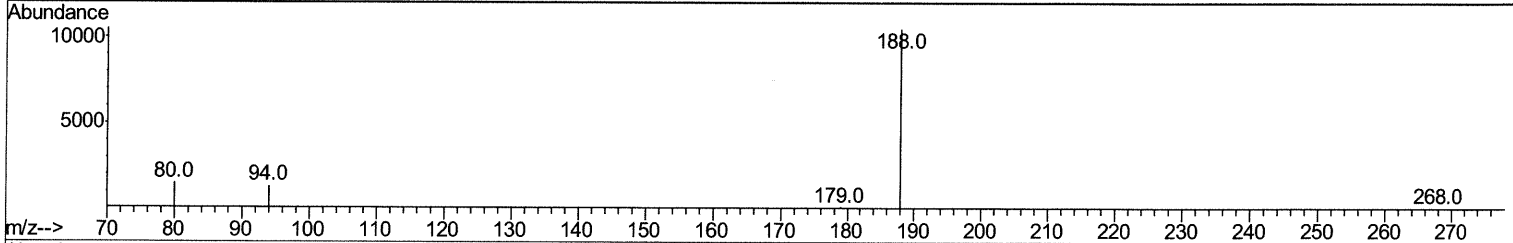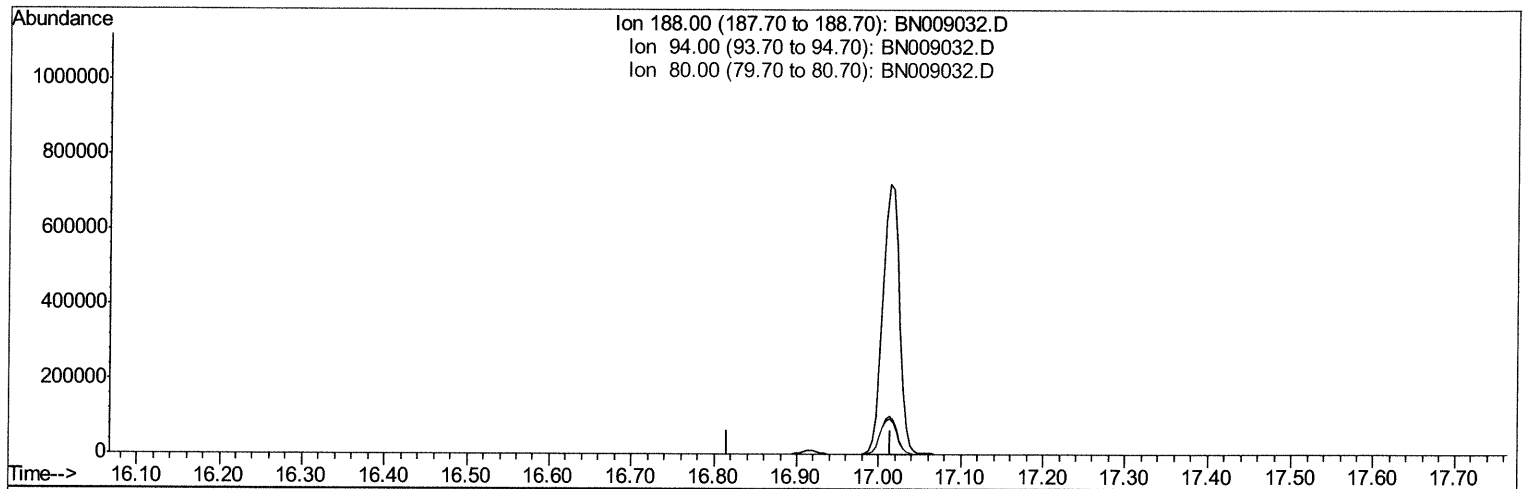

TIC: BN009032.D

(10) Phenanthrene-d10 (I)

16.916min (-16.916) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009032.D
 Acq On : 19 Dec 2019 16:30
 Operator : JU
 Sample : K6170-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BR7

Manual Integrations
 APPROVED

Sohil
 12/20/2019 4:29:26 PM

Quant Time: Dec 20 05:05:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

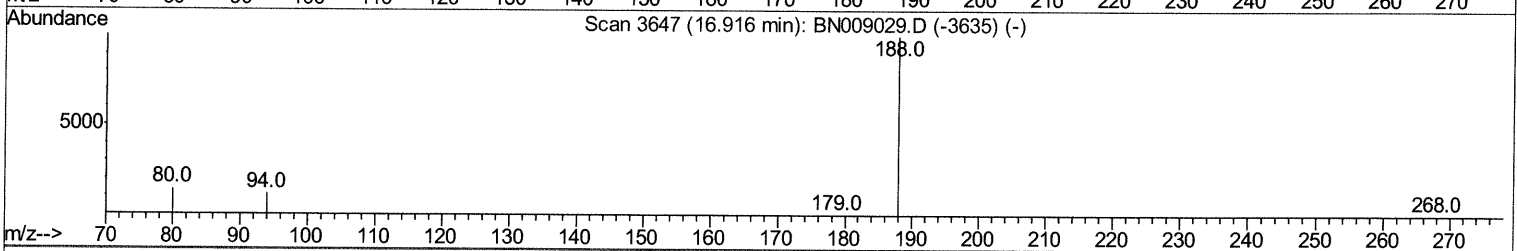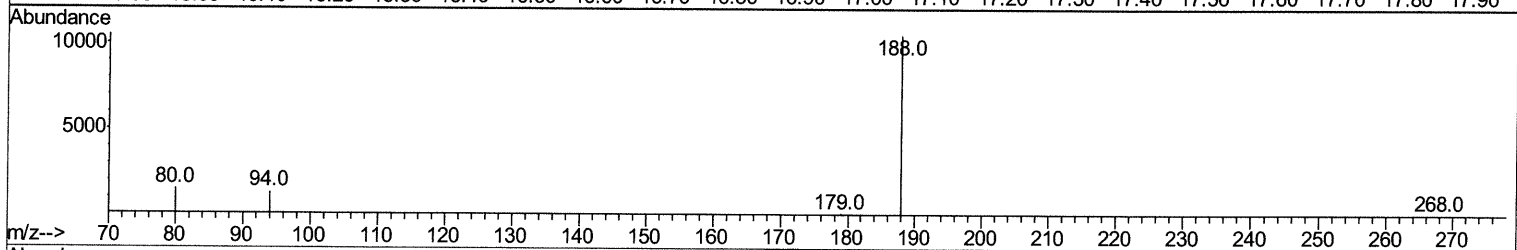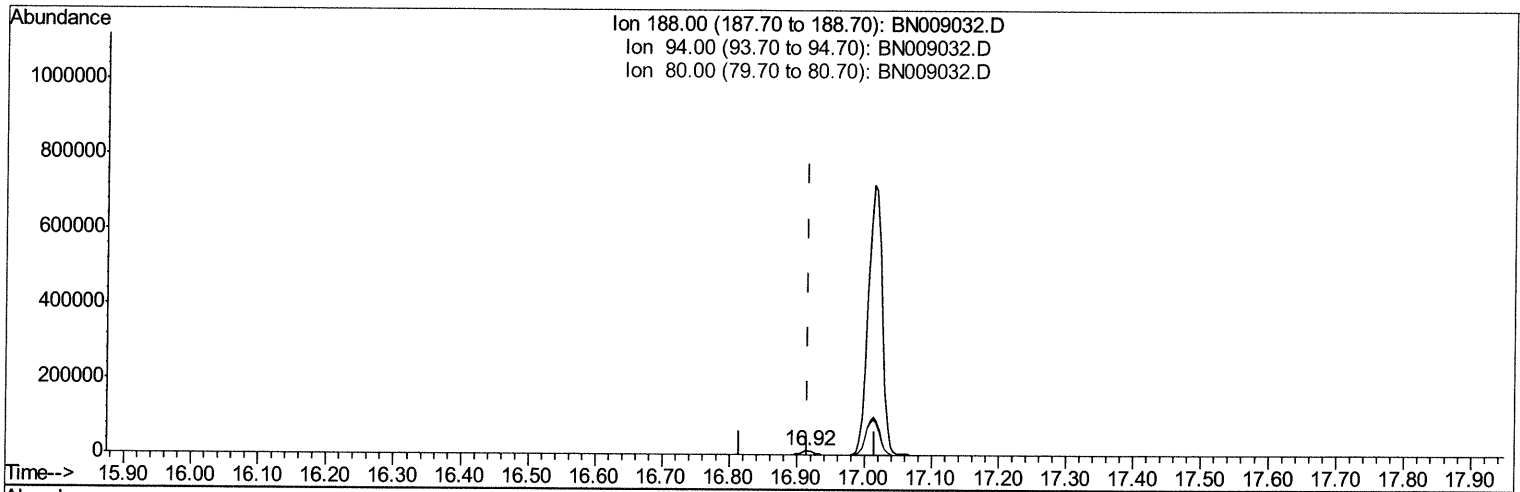

TIC: BN009032.D

(10) Phenanthrene-d10 (I)

16.916min (-0.000) 0.40ng/ul m

JU 12/23/19

response 14508

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	12.15
80.00	13.70	14.04
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009032.D
 Acq On : 19 Dec 2019 16:30
 Operator : JU
 Sample : K6170-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BR7

Manual Integrations
 APPROVED

Sohil
 12/20/2019 4:29:26 PM

Quant Time: Dec 20 05:39:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	2767	0.40	ng/ul	0.00
2) Naphthalene-d8	10.30	136	10598	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	6476	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.92	188	14508m	0.40	ng/ul	0.00
16) Chrysene-d12	21.12	240	9719	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	8261	0.40	ng/ul	0.00

Ju 12/23/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.89	152	4584	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	13478	0.32	ng/ul	0.00

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed