


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
Data File : BN009042.D
Acq On : 19 Dec 2019 22:27
Operator : JU
Sample : K6170-16
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0BW6

Manual Integrations
APPROVED

Sohil
12/20/2019 4:29:34 PM

Quant Time: Dec 20 06:11:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 19 15:54:16 2019
Response via : Initial Calibration

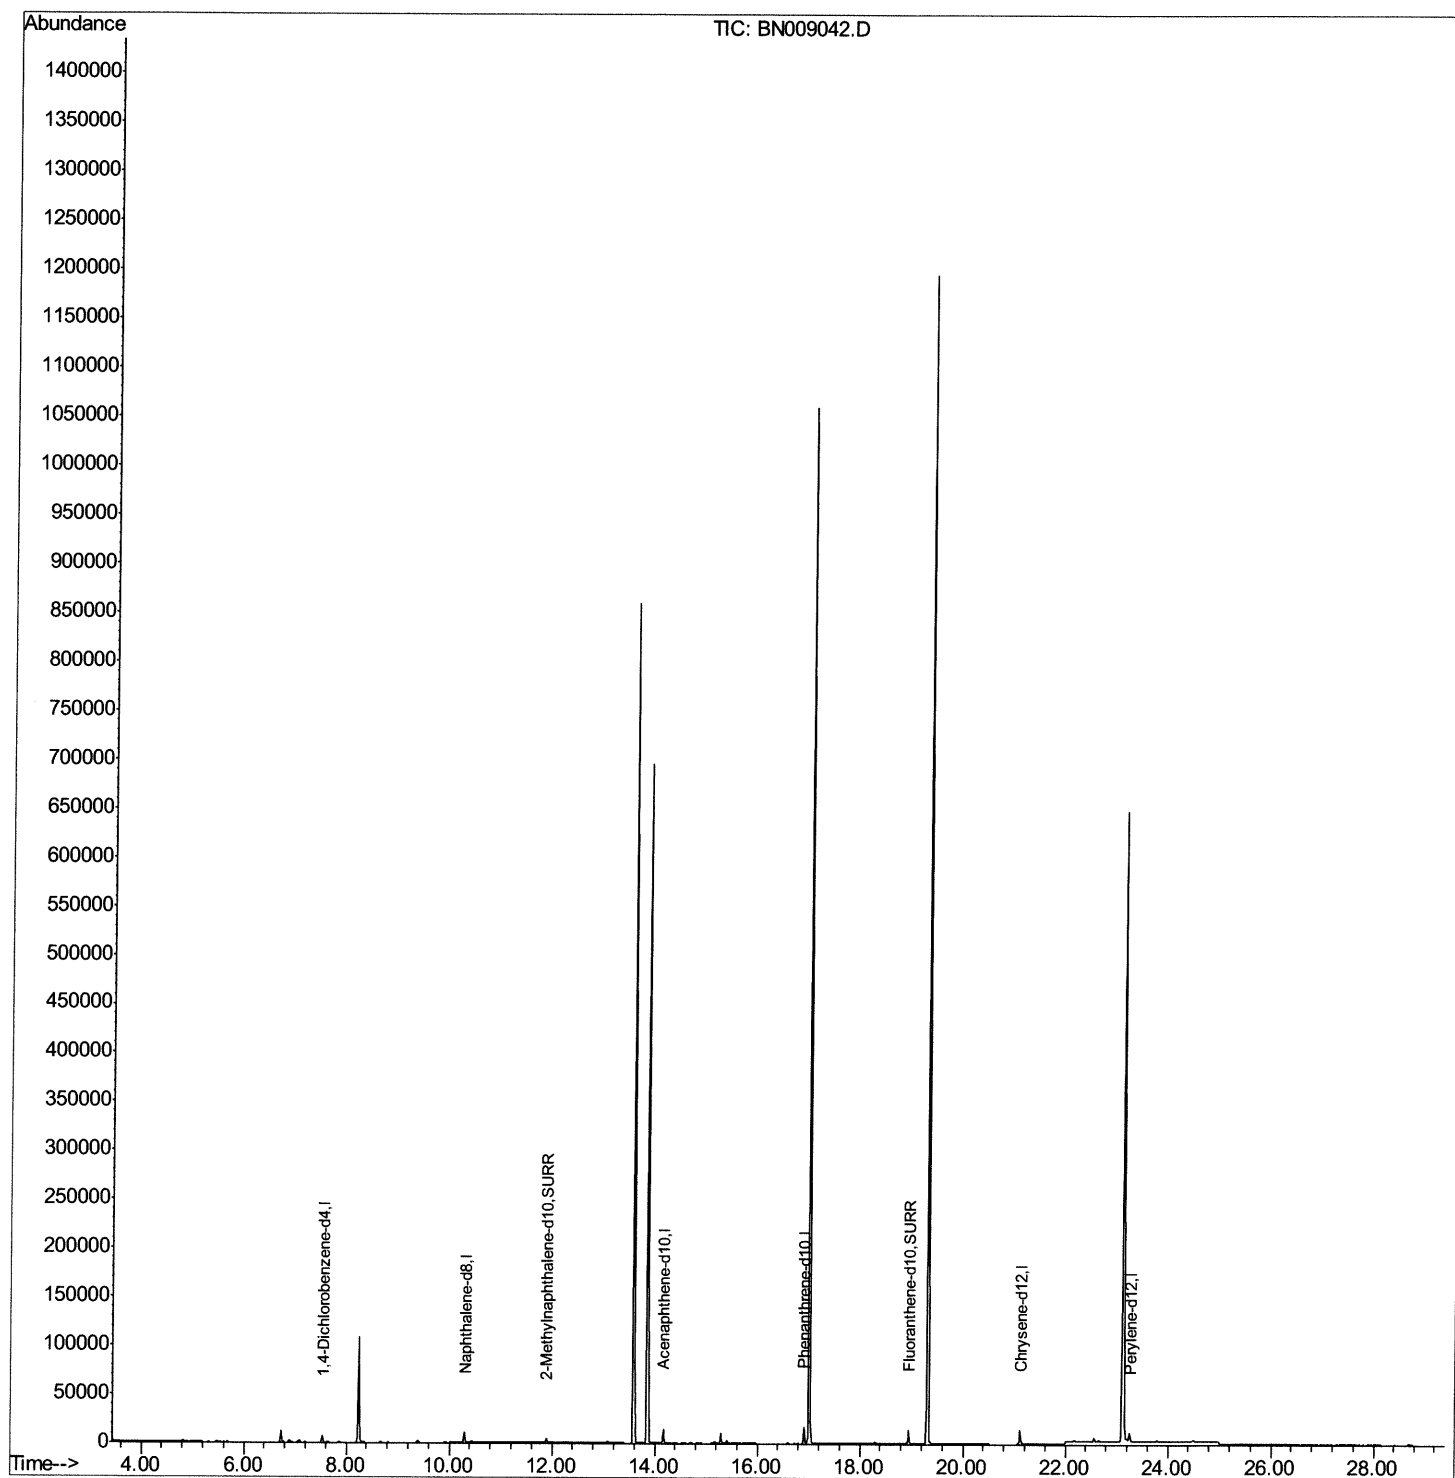

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009042.D
 Acq On : 19 Dec 2019 22:27
 Operator : JU
 Sample : K6170-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
ClientSampleId :
 C0BW6

Manual Integrations
APPROVED

Sohil
 12/20/2019 4:29:34 PM

Quant Time: Dec 20 05:06:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

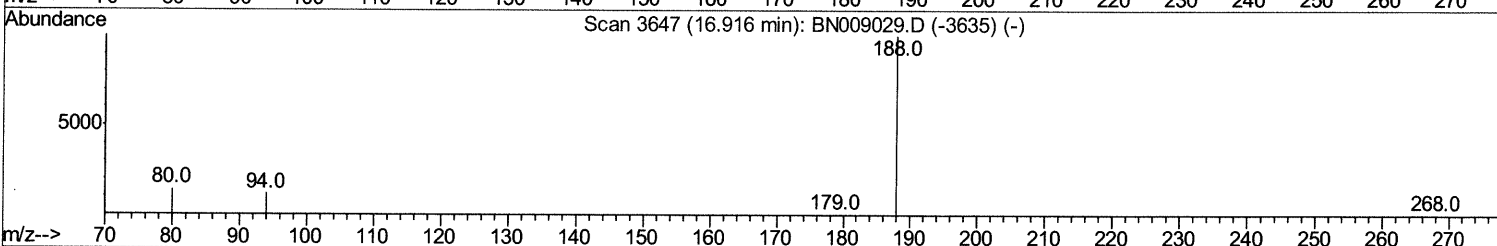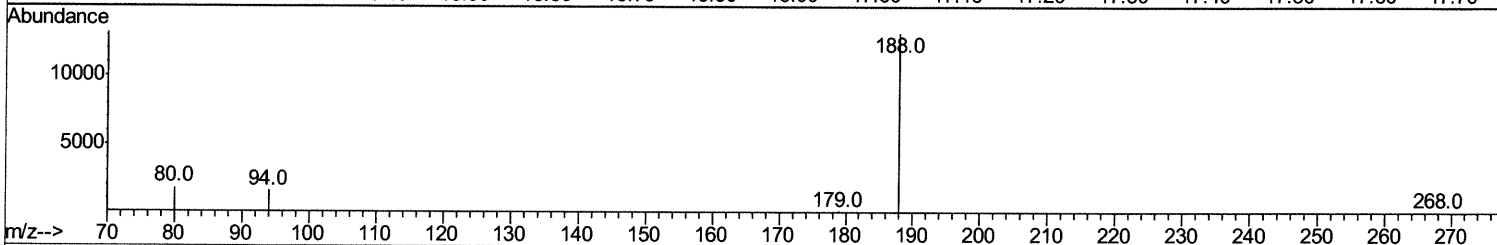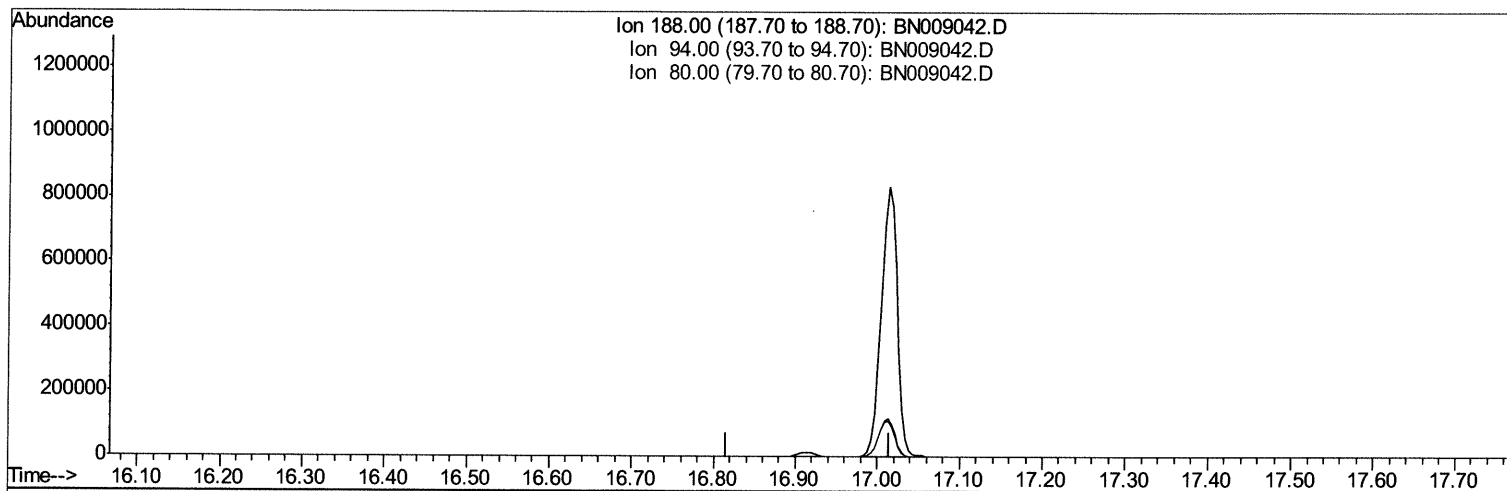

TIC: BN009042.D

(10) Phenanthrene-d10 (I)

16.916min (-16.916) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.60	0.00#
80.00	13.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009042.D
 Acq On : 19 Dec 2019 22:27
 Operator : JU
 Sample : K6170-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BW6

Manual Integrations
 APPROVED

Sohil
 12/20/2019 4:29:34 PM

Quant Time: Dec 20 05:06:35 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

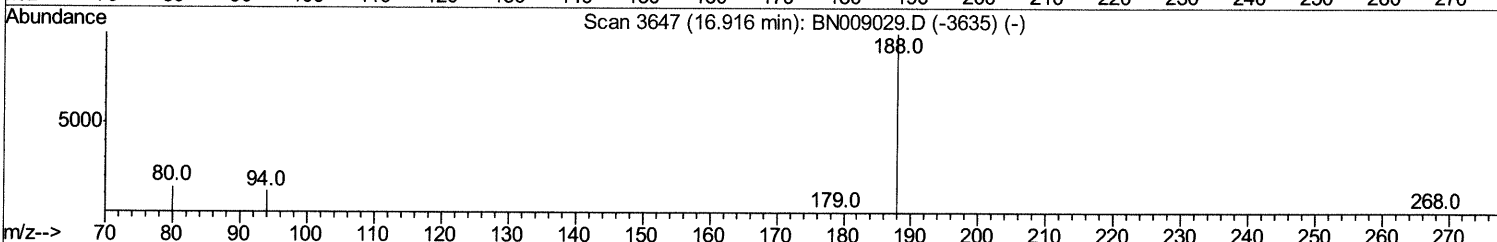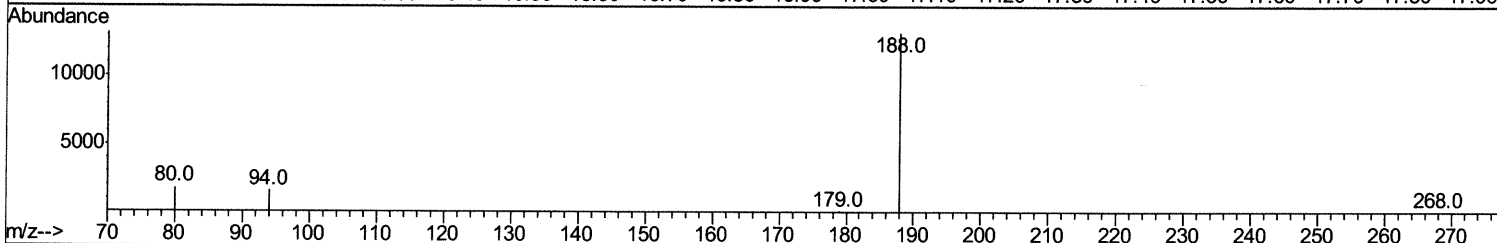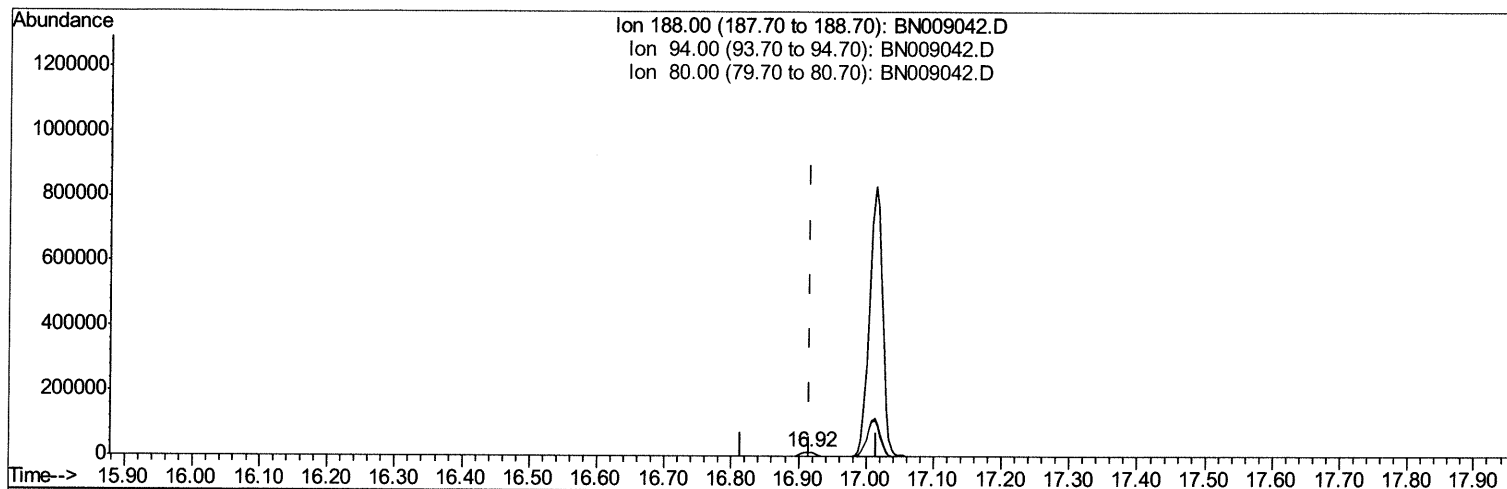

TIC: BN009042.D

(10) Phenanthrene-d10 (I)

16.916min (+0.000) 0.40ng/ul m JU 12/23/19

response 17846

Ion	Exp%	Act%
188.00	100	100
94.00	11.60	11.71
80.00	13.70	13.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121919\
 Data File : BN009042.D
 Acq On : 19 Dec 2019 22:27
 Operator : JU
 Sample : K6170-16
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0BW6

Manual Integrations
 APPROVED

Sohil
 12/20/2019 4:29:34 PM

Quant Time: Dec 20 06:11:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN121619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 19 15:54:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.54	152	3255	0.40	ng/ul	0.00
2) Naphthalene-d8	10.30	136	12948	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.17	164	8059	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.92	188	17846m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.12	240	12426	0.40	ng/ul	0.00
20) Perylene-d12	23.26	264	10533	0.40	ng/ul	0.00

24/12/19

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.89	152	5553	0.24	ng/ul	0.00
14) Fluoranthene-d10	18.95	212	14996	0.29	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed