
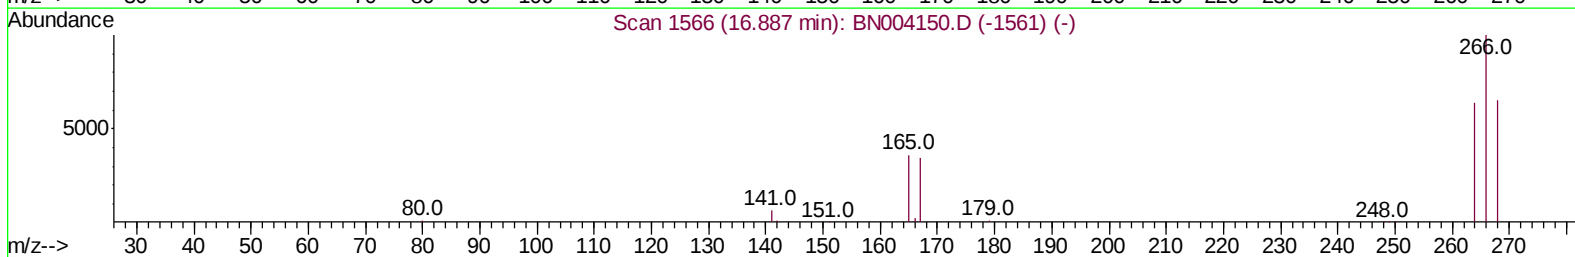
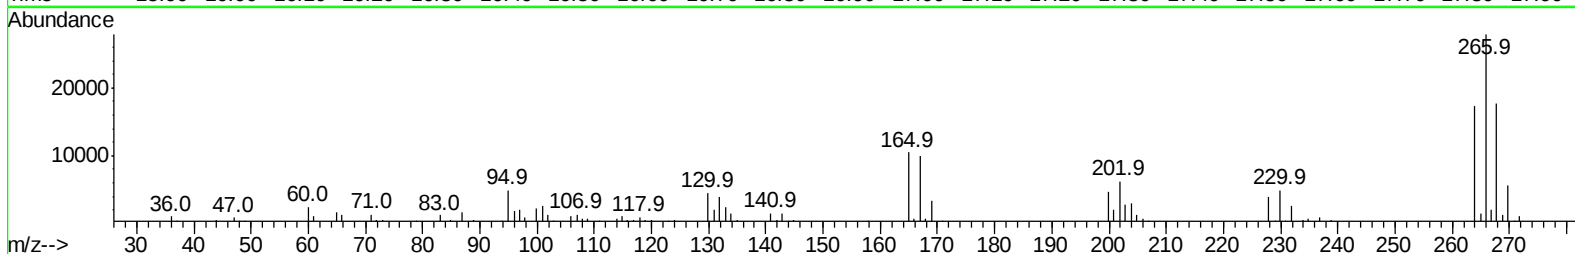


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122018\
Data File : BN004147.D
Acq On : 20 Dec 2018 12:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 17:57:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 17:31:49 2018
Response via : Initial Calibration

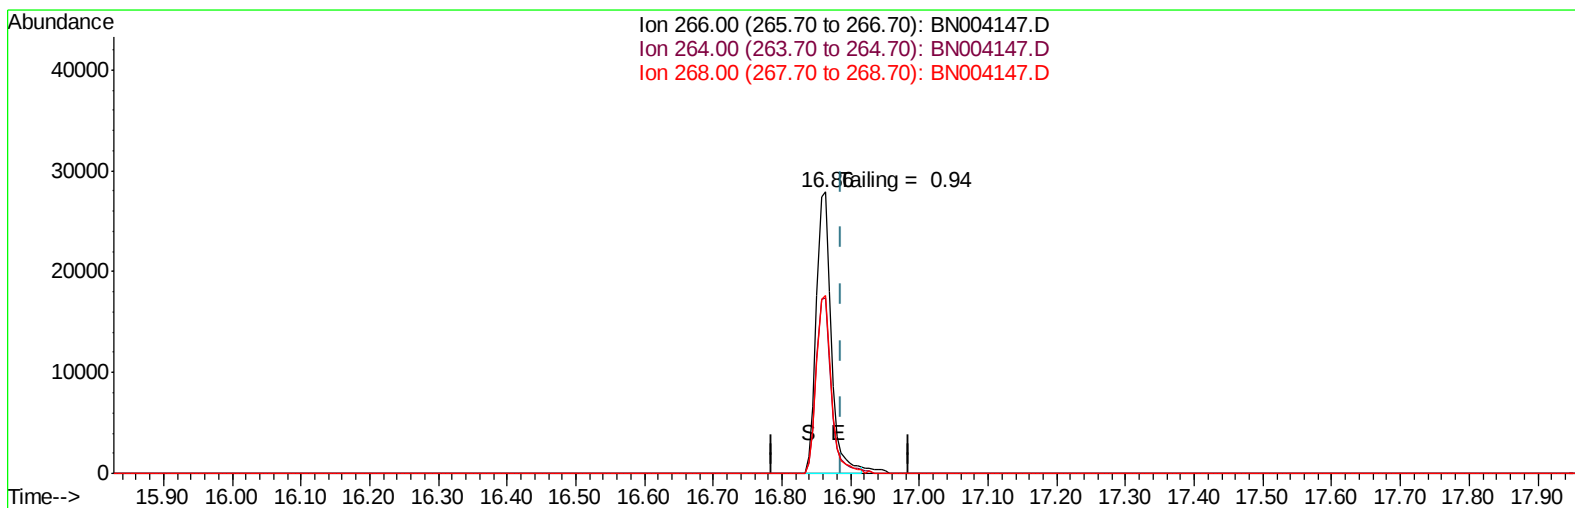

TIC: BN004147.D

(22) Pentachlorophenol

16.863min (-0.023) 0.00ng

response 42610

Ion	Exp%	Act%
266.00	100	100
264.00	65.10	62.11
268.00	64.70	63.14
0.00	0.00	0.00