

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122018\
 Data File : BN004153.D
 Acq On : 20 Dec 2018 16:48
 Operator : JU/SJ
 Sample : SSTDICC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Quant Time: Dec 20 17:29:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 20 16:25:43 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	1926	0.40	ng	0.00
7) Naphthalene-d8	10.62	136	10046	0.40	ng	-0.01
13) Acenaphthene-d10	14.47	164	6446	0.40	ng	0.00
19) Phenanthrene-d10	17.21	188	15653	0.40	ng	-0.01
27) Chrysene-d12	21.41	240	16680	0.40	ng	0.00
34) Perylene-d12	23.73	264	14842	0.40	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.41	112	17021	3.57	ng	0.00
5) Phenol-d6	6.99	99	24829	4.12	ng	0.00
8) Nitrobenzene-d5	9.00	82	22674	5.15	ng	0.00
11) 2-Methylnaphthalene-d10	12.21	152	55076	3.37	ng	0.00
14) 2,4,6-Tribromophenol	15.96	330	13342	5.20	ng	-0.01
15) 2-Fluorobiphenyl	13.08	172	77734	2.80	ng	0.00
25) Fluoranthene-d10	19.24	212	154203	3.39	ng	0.00
29) Terphenyl-d14	19.83	244	130388	3.36	ng	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) 1,4-Dioxane	3.32	88	5714	2.291	ng	95
6) bis(2-Chloroethyl)ether	7.26	93	19128	3.559	ng	99
9) Naphthalene	10.67	128	80603	3.279	ng	99
10) Hexachlorobutadiene	10.93	225	13540	3.016	ng	# 100
12) 2-Methylnaphthalene	12.28	142	59109	3.441	ng	99
16) Acenaphthylene	14.19	152	104377	3.632	ng	100
17) Acenaphthene	14.52	154	64626	3.245	ng	98
18) Fluorene	15.51	166	83167	3.337	ng	100
20) 4-Bromophenyl-phenylether	16.40	248	29840	3.291	ng	# 93
21) Hexachlorobenzene	16.52	284	31932	3.340	ng	95
23) Phenanthrene	17.25	178	141775	3.302	ng	100
24) Anthracene	17.34	178	136214	3.698	ng	100
26) Fluoranthene	19.27	202	168179	3.410	ng	98
28) Pyrene	19.64	202	171265	3.714	ng	100
30) Benzo(a)anthracene	21.39	228	152029	3.478	ng	99
31) Chrysene	21.44	228	152940	3.244	ng	99
32) Bis(2-ethylhexyl)phthalate	21.28	149	94722	7.323	ng	100
33) Indeno(1,2,3-cd)pyrene	26.09	276	159172	3.261	ng	99
35) Benzo(b)fluoranthene	23.02	252	144624	3.123	ng	# 93
36) Benzo(k)fluoranthene	23.07	252	145531	3.173	ng	98
37) Benzo(a)pyrene	23.62	252	133683	3.172	ng	# 89
38) Dibenzo(a,h)anthracene	26.10	278	133454	3.398	ng	98
39) Benzo(g,h,i)perylene	26.82	276	129842	3.306	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122018\
Data File : BN004153.D
Acq On : 20 Dec 2018 16:48
Operator : JU/SJ
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Dec 20 17:29:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 20 16:25:43 2018
Response via : Initial Calibration

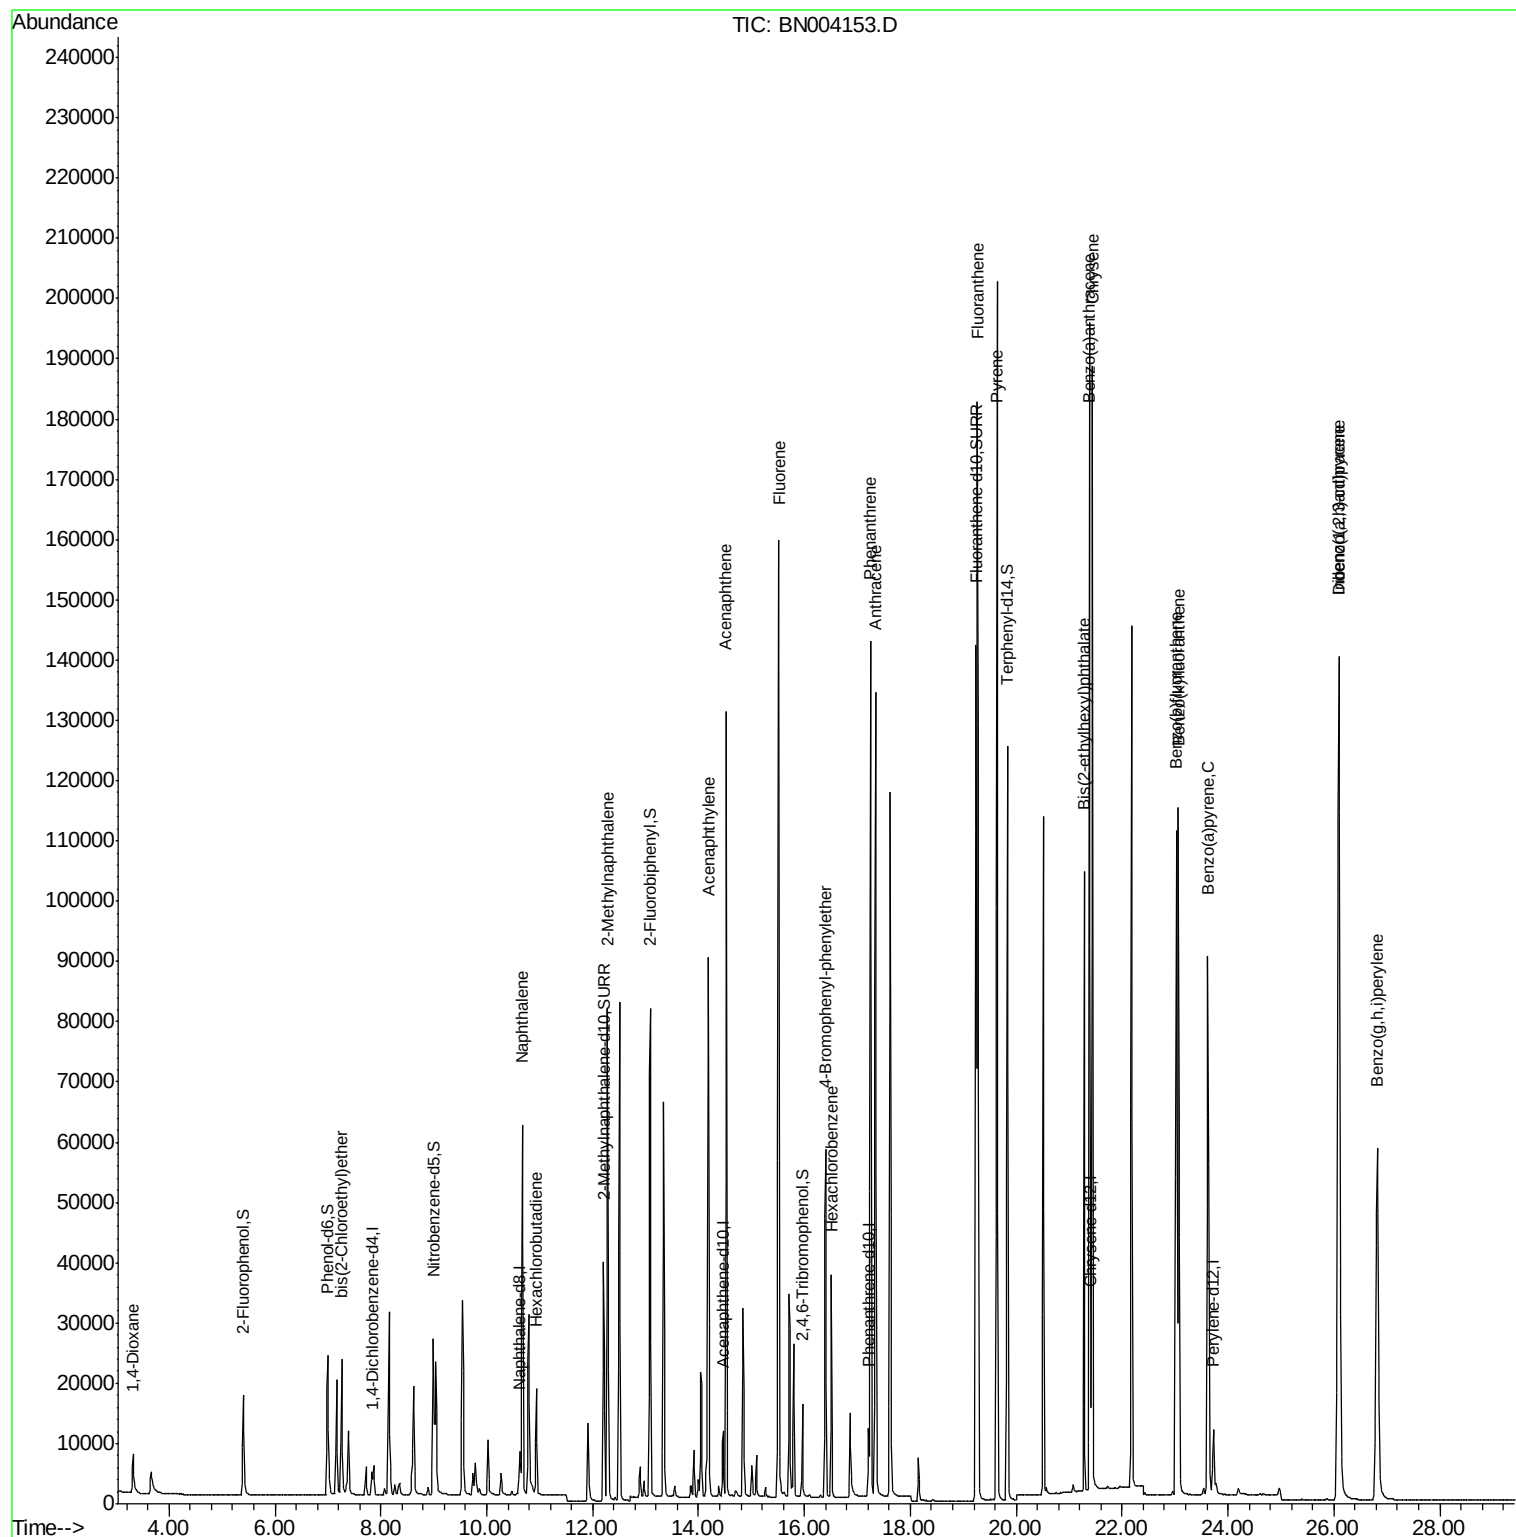



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.83 min Scan# 596

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:152 Resp: 1926

Ion Ratio Lower Upper

152 100

150 154.2 124.6 187.0




115 63.1 46.4 69.6

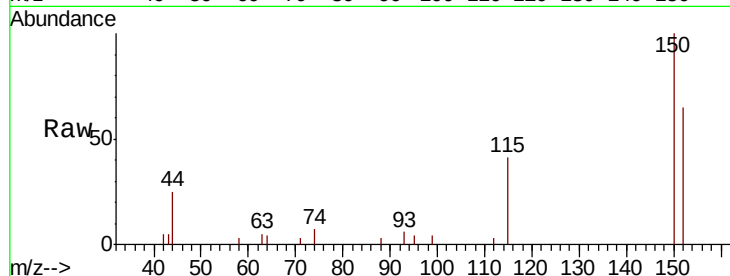

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

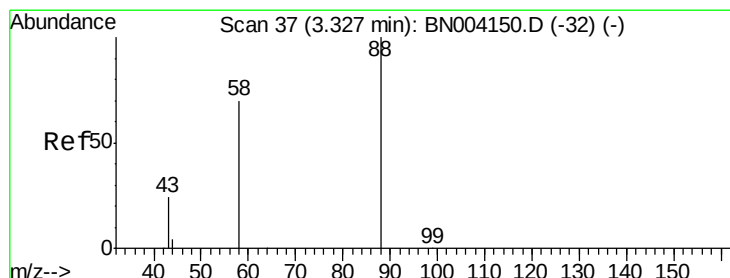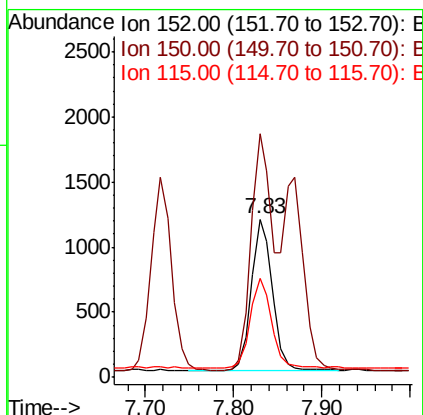

#2

1,4-Dioxane

Concen: 2.291 ng

RT: 3.32 min Scan# 36

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion: 88 Resp: 5714

Ion Ratio Lower Upper

88 100

58 72.9 60.9 91.3



43 26.2 23.9 35.9

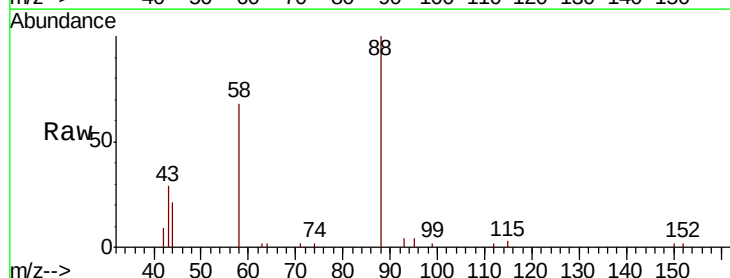


Abundance Ion 88.00 (87.70 to 88.70): BNC

Ion 58.00 (57.70 to 58.70): BNC

Ion 43.00 (42.70 to 43.70): BNC

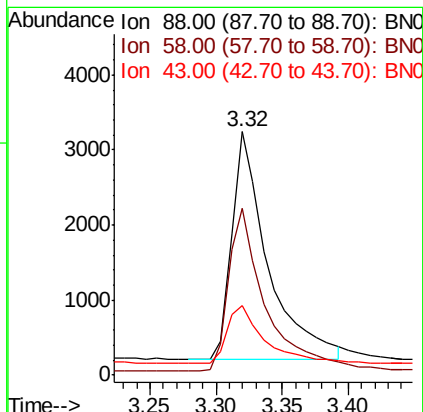



#4

2-Fluorophenol

Concen: 3.569 ng

RT: 5.41 min Scan# 295

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion: 112 Resp: 17021

Ion Ratio Lower Upper




112 100

64 55.4 44.3 66.5

63 27.3 22.4 33.6

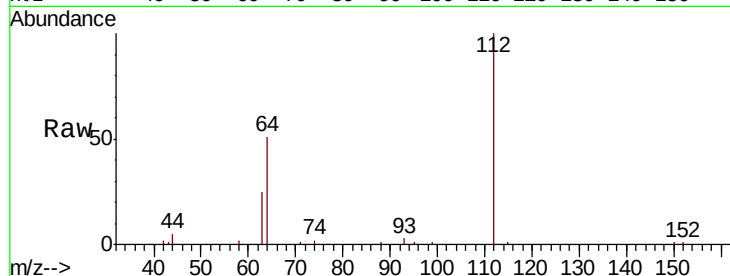

Abundance Ion 112.00 (111.70 to 112.70): BNC
Ion 64.00 (63.70 to 64.70): BNC
Ion 63.00 (62.70 to 63.70): BNC

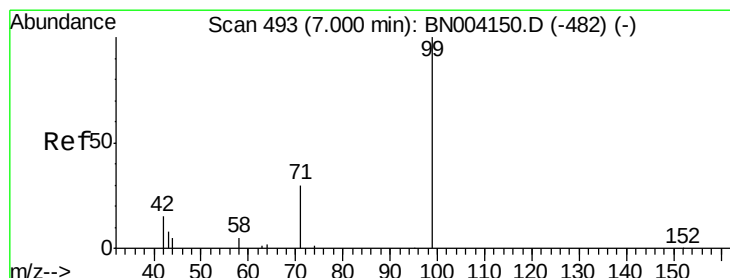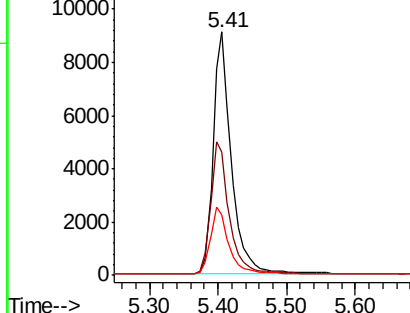

#5

Phenol-d6

Concen: 4.123 ng

RT: 6.99 min Scan# 492

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion: 99 Resp: 24829

Ion Ratio Lower Upper



99 100


42 16.9 14.8 22.2

71 30.3 24.8 37.2

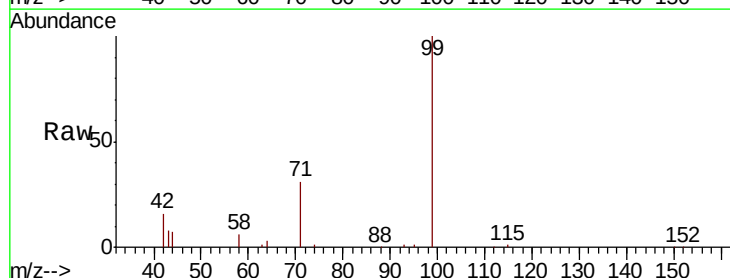

Abundance Ion 99.00 (98.70 to 99.70): BNC
Ion 42.00 (41.70 to 42.70): BNC
Ion 71.00 (70.70 to 71.70): BNC

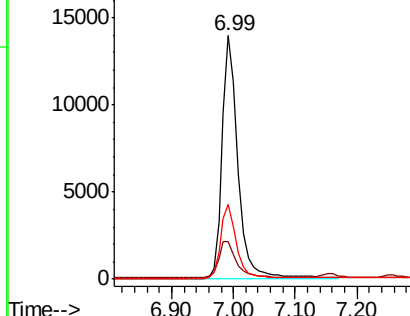



#6

bis(2-Chloroethyl)ether

Concen: 3.559 ng

RT: 7.26 min Scan# 525

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion: 93 Resp: 19128

Ion Ratio Lower Upper




93 100

63 70.5 55.8 83.6

95 31.4 25.4 38.2

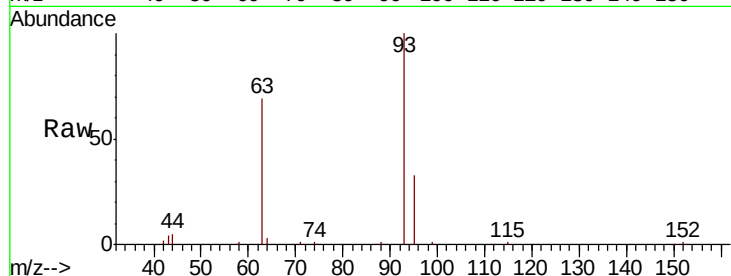

Abundance Ion 93.00 (92.70 to 93.70): BN004153.D (-500) (-)

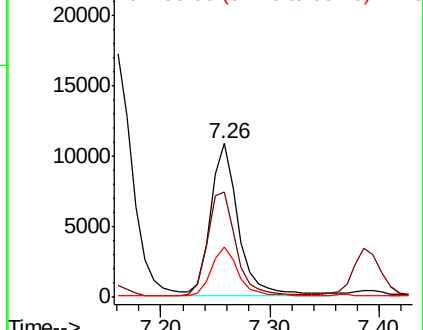

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.62 min Scan# 847

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Tgt Ion: 136 Resp: 10046


Ion Ratio Lower Upper

136 100



137 11.6 9.0 13.4


54 9.6 4.1 6.1#

68 8.3 3.5 5.3#



Abundance Ion 136.00 (135.70 to 136.70): BN004153.D (-832) (-)

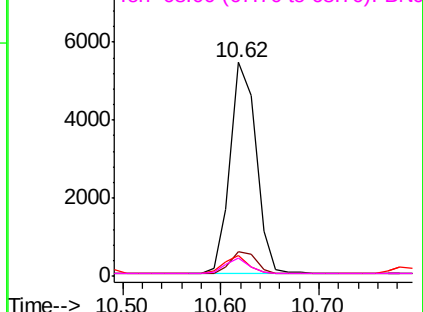



#8

Nitrobenzene-d5

Concen: 5.153 ng

RT: 9.00 min Scan# 719

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion: 82 Resp: 22674

Ion Ratio Lower Upper

82 100

128 48.8 28.9 43.3#

54 44.0 46.1 69.1#



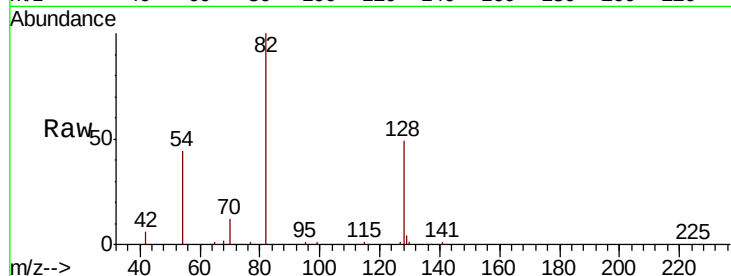


Abundance

Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): BNC

Ion 54.00 (53.70 to 54.70): BNC

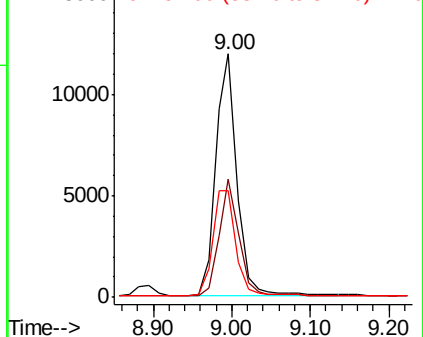

#9

Naphthalene

Concen: 3.279 ng

RT: 10.67 min Scan# 851

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion: 128 Resp: 80603

Ion Ratio Lower Upper

128 100

129 11.0 9.1 13.7

127 13.4 10.2 15.4






Abundance

Ion 128.00 (127.70 to 128.70): BNC

Ion 129.00 (128.70 to 129.70): BNC

Ion 127.00 (126.70 to 127.70): BNC

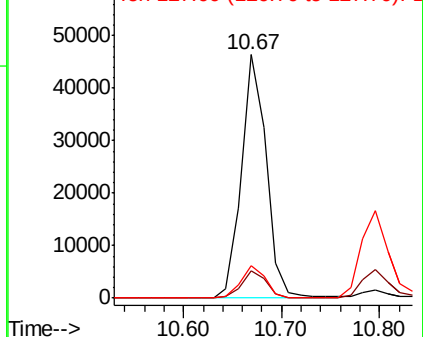


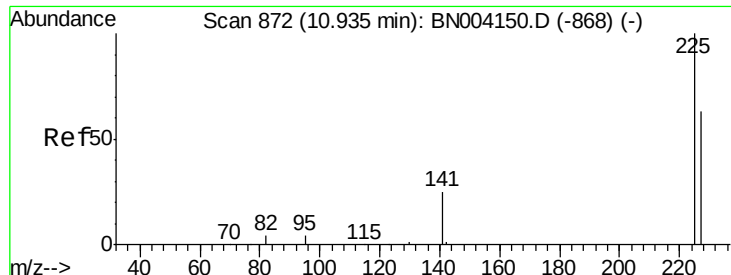




#10
Hexachlorobutadiene
Concen: 3.016 ng
RT: 10.93 min Scan# 872
Delta R.T. 0.00 min
Lab File: BN004153.D
Acq: 20 Dec 2018 16:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tot Ion:225 Resp: 13540
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.4 51.3 76.9

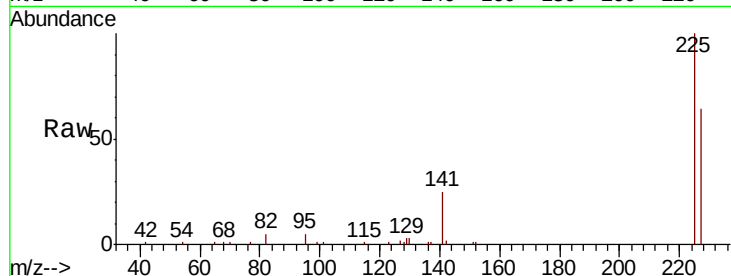


Abundance Ion 225.00 (224.70 to 225.70): E
Ion 223.00 (222.70 to 223.70): E
Ion 227.00 (226.70 to 227.70): E

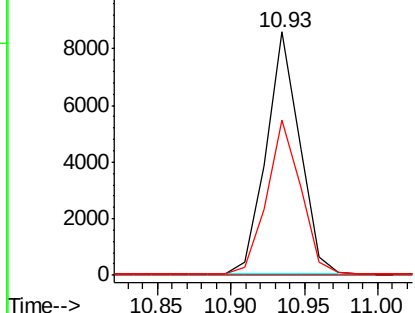




#11
2-Methylnaphthalene-d10
Concen: 3.368 ng
RT: 12.21 min Scan# 1075
Delta R.T. -0.01 min
Lab File: BN004153.D
Acq: 20 Dec 2018 16:48

Tgt Ion:152 Resp: 55076
Ion Ratio Lower Upper
152 100
151 19.2 15.1 22.7

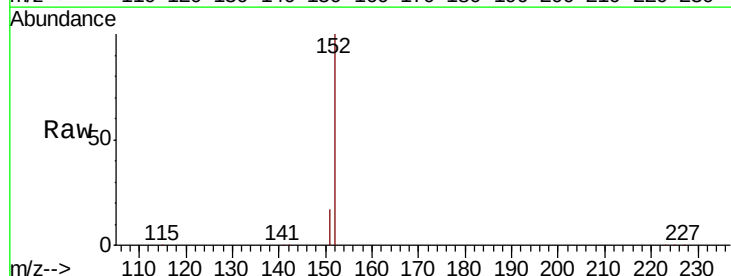

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E

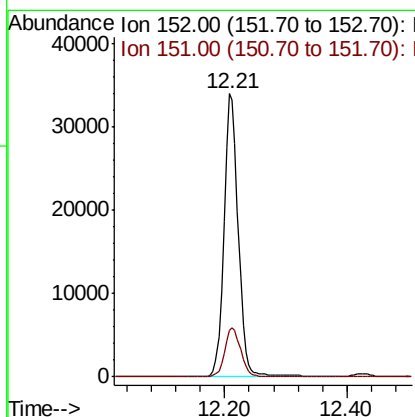

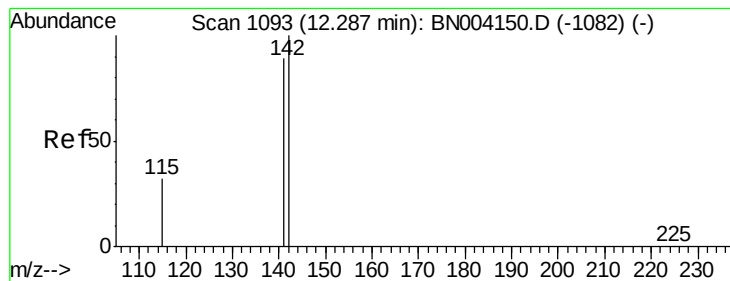

#12

2-Methylnaphthalene

Concen: 3.441 ng

RT: 12.28 min Scan# 1092

Delta R.T. -0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:142 Resp: 59109

Ion Ratio Lower Upper

142 100

141 89.3 71.9 107.9

115 32.2 27.0 40.6



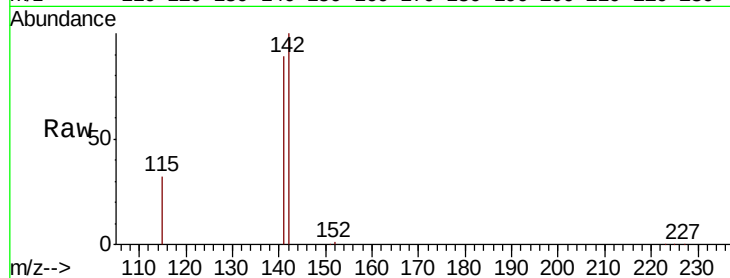


Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

Ion 115.00 (114.70 to 115.70): E

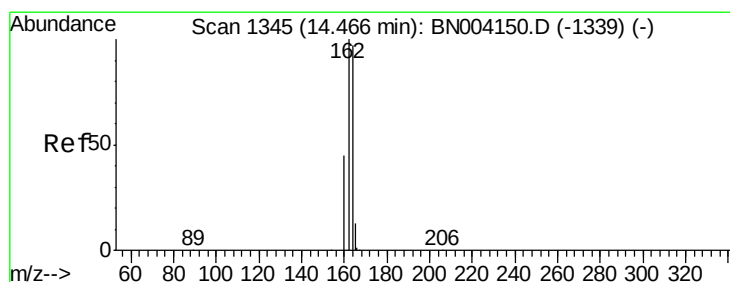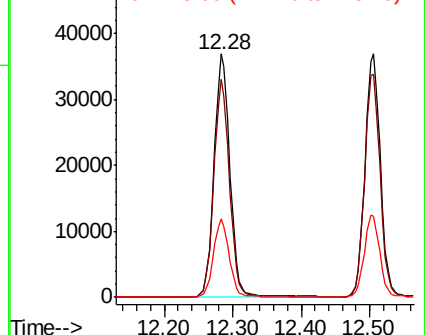

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.47 min Scan# 1345

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:164 Resp: 6446

Ion Ratio Lower Upper

164 100

162 103.3 81.8 122.6

160 46.2 37.2 55.8


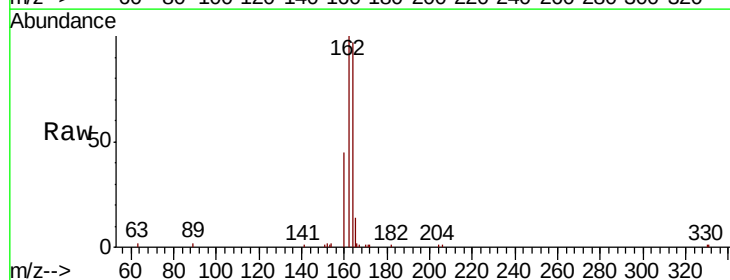



Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

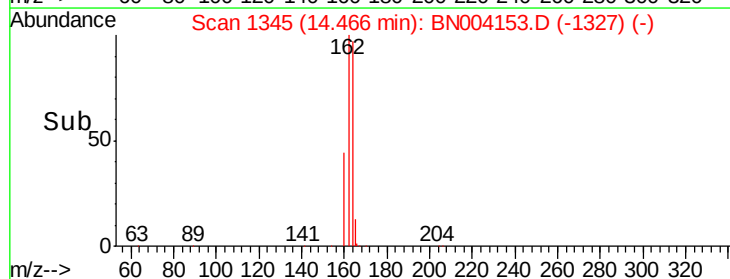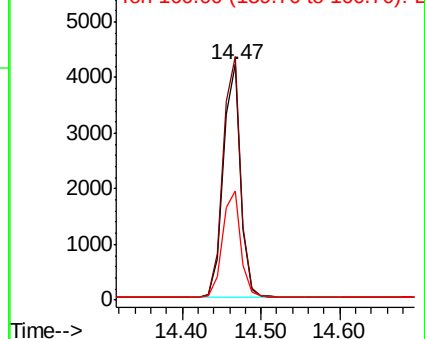

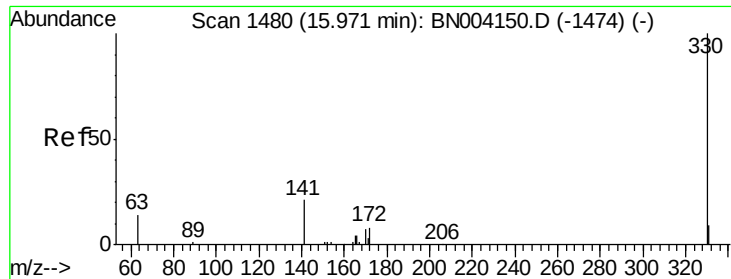

#14

2,4,6-Tribromophenol

Concen: 5.200 ng

RT: 15.96 min Scan# 1479

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:330 Resp: 13342

Ion Ratio Lower Upper




330 100

332 0.0 0.0 0.0

141 28.9 28.3 42.5



Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

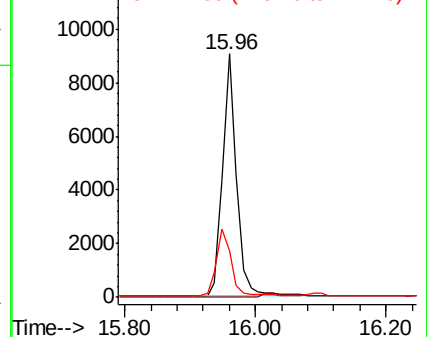

#15

2-Fluorobiphenyl

Concen: 2.802 ng

RT: 13.08 min Scan# 1221

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:172 Resp: 77734

Ion Ratio Lower Upper



172 100


171 34.4 27.1 40.7

170 22.1 17.4 26.0



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

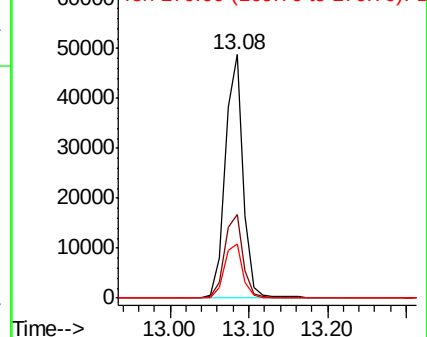

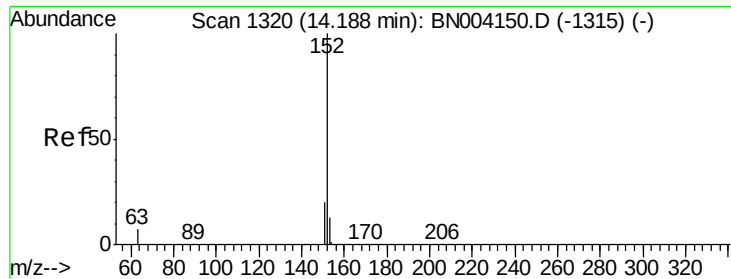

#16

Acenaphthylene

Concen: 3.632 ng

RT: 14.19 min Scan# 1320

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2





Tot Ion:152 Resp: 104377

Ion Ratio Lower Upper

152 100

151 19.7 15.7 23.5

153 13.0 10.6 15.8

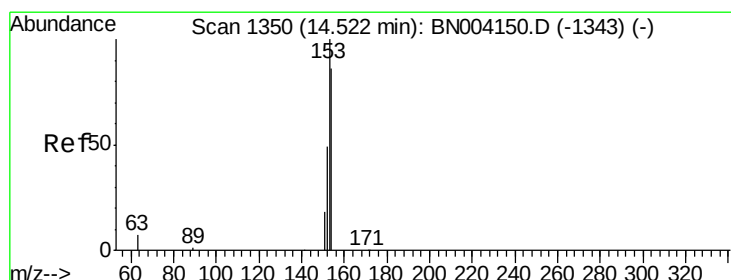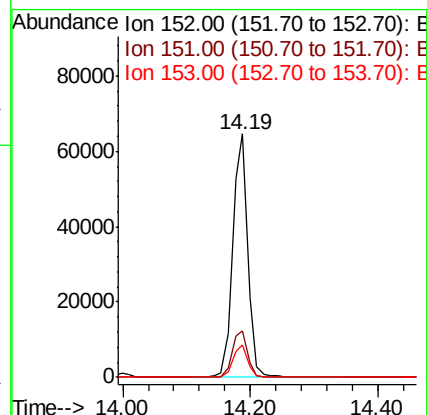

#17

Acenaphthene

Concen: 3.245 ng

RT: 14.52 min Scan# 1350

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48




Tgt Ion:154 Resp: 64626


Ion Ratio Lower Upper

154 100

153 113.4 88.9 133.3

152 53.9 43.5 65.3

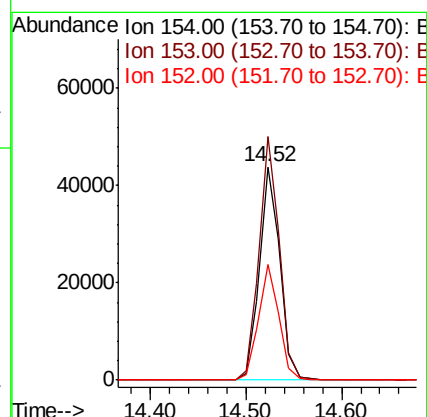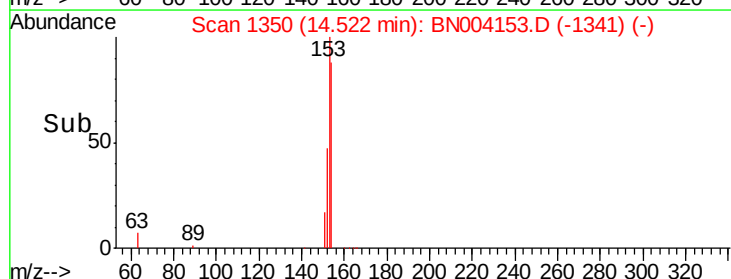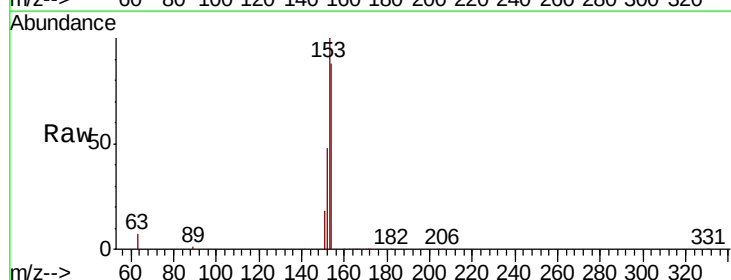

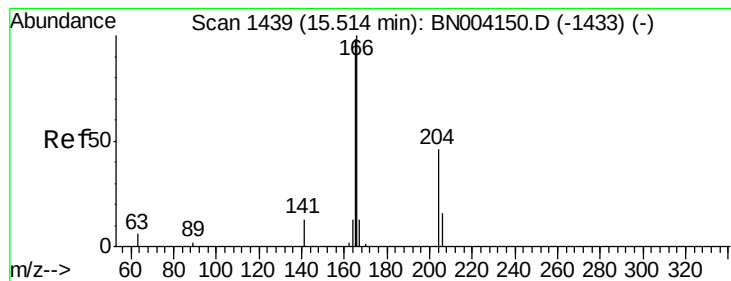

#18

Fluorene

Concen: 3.337 ng

RT: 15.51 min Scan# 1439

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:166 Resp: 83167

Ion Ratio Lower Upper




166 100

165 97.5 77.8 116.8

167 13.5 10.9 16.3



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

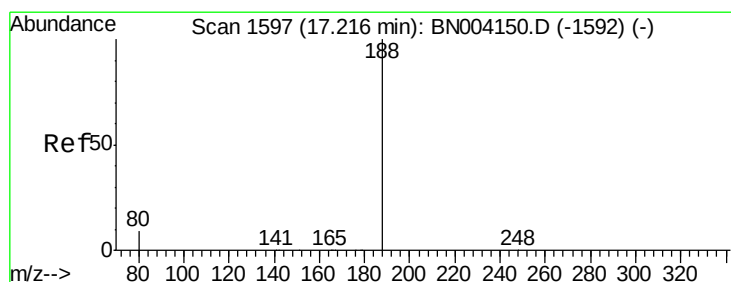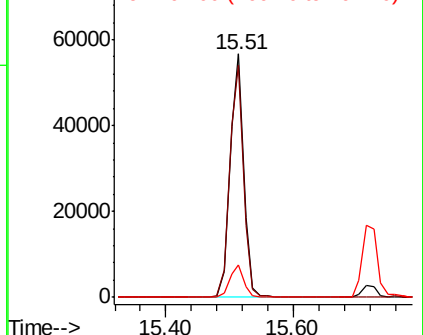

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.21 min Scan# 1596

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:188 Resp: 15653

Ion Ratio Lower Upper



188 100


94 0.0 0.0 0.0

80 13.4 8.6 12.8#

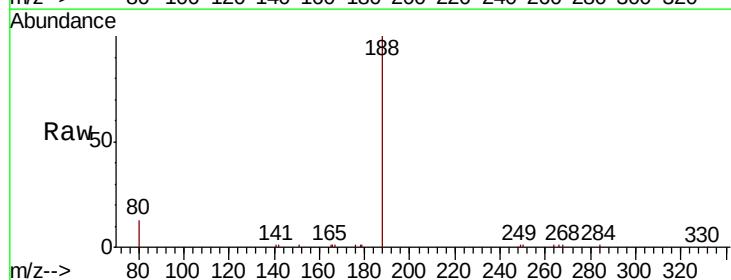

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BNC
Ion 80.00 (79.70 to 80.70): BNC

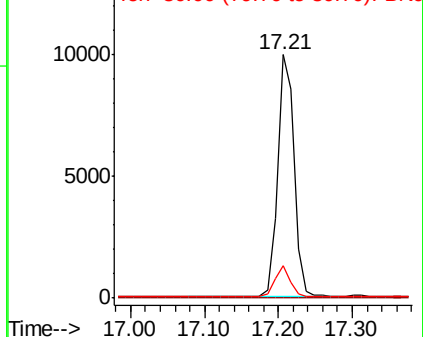


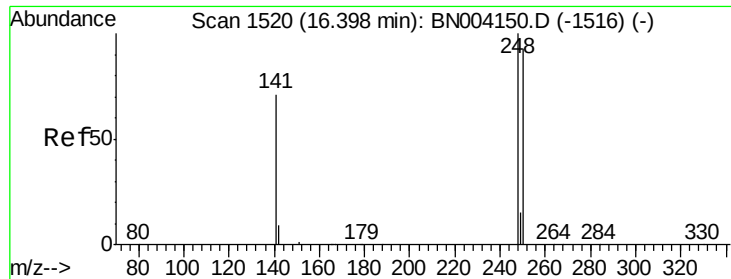




#20
4-Bromophenyl-phenylether
Concen: 3.291 ng
RT: 16.40 min Scan# 1520
Delta R.T. 0.00 min
Lab File: BN004153.D
Acq: 20 Dec 2018 16:48

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tot Ion:248 Resp: 29840
Ion Ratio Lower Upper
248 100
250 101.3 83.7 125.5
141 48.7 31.4 47.0#

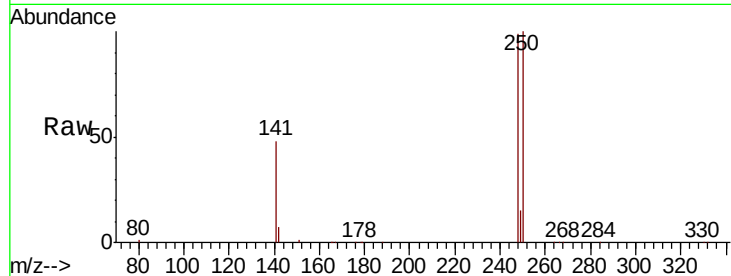


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

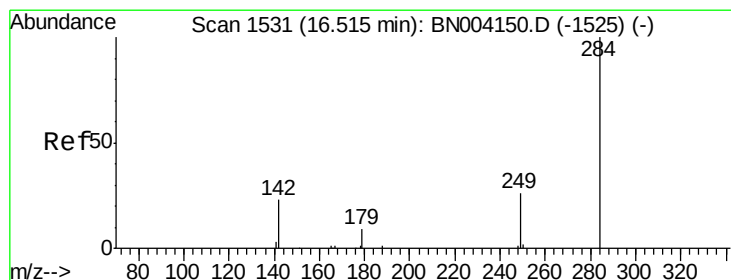
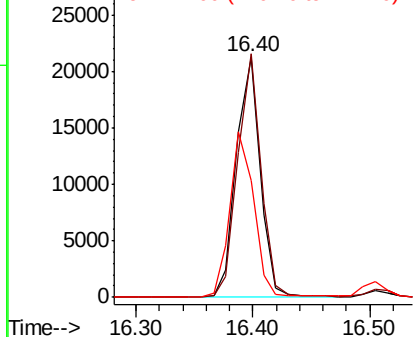



#21
Hexachlorobenzene
Concen: 3.340 ng
RT: 16.52 min Scan# 1531
Delta R.T. 0.00 min
Lab File: BN004153.D
Acq: 20 Dec 2018 16:48

Tgt Ion:284 Resp: 31932
Ion Ratio Lower Upper
284 100
142 32.8 29.7 44.5
249 28.7 24.0 36.0



Abundance Ion 283.80 (283.50 to 284.50): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E

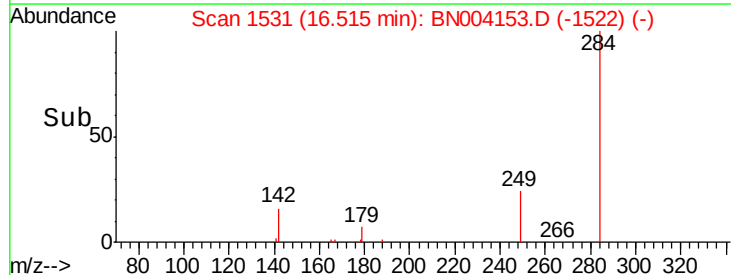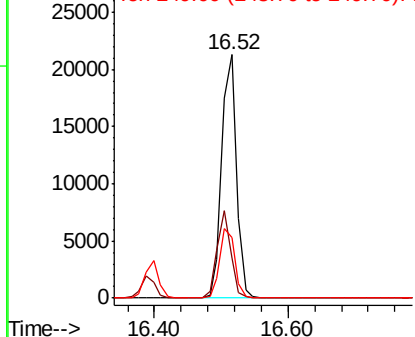

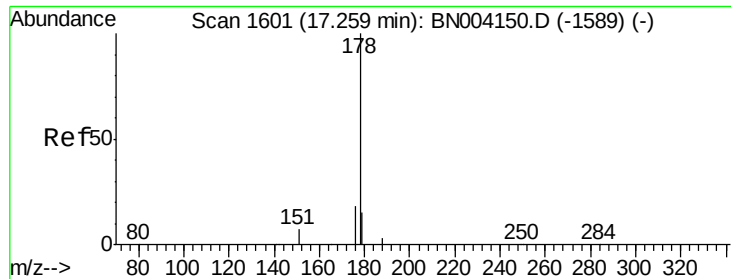

#23

Phenanthrene

Concen: 3.302 ng

RT: 17.25 min Scan# 1600

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:178 Resp: 141775

Ion Ratio Lower Upper

178 100

176 18.7 15.1 22.7




179 15.3 12.4 18.6

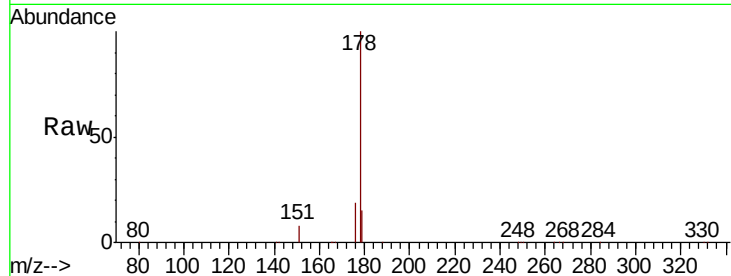

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

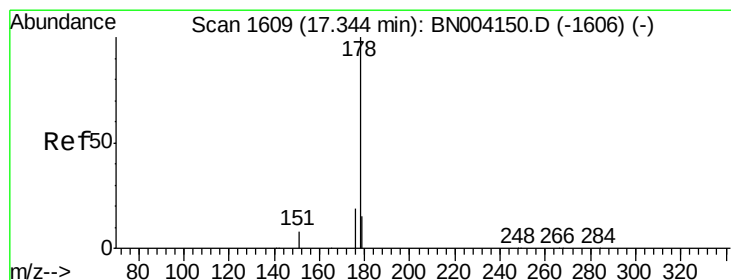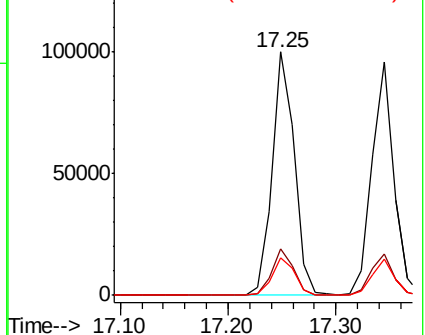

#24

Anthracene

Concen: 3.698 ng

RT: 17.34 min Scan# 1609

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:178 Resp: 136214

Ion Ratio Lower Upper

178 100

176 18.1 14.5 21.7



179 15.3 12.2 18.4




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E




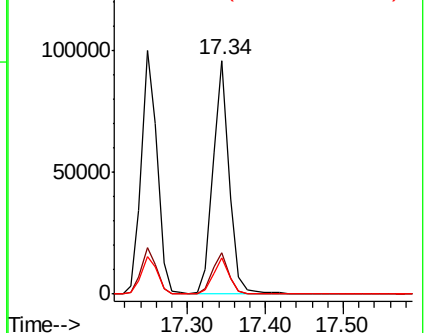


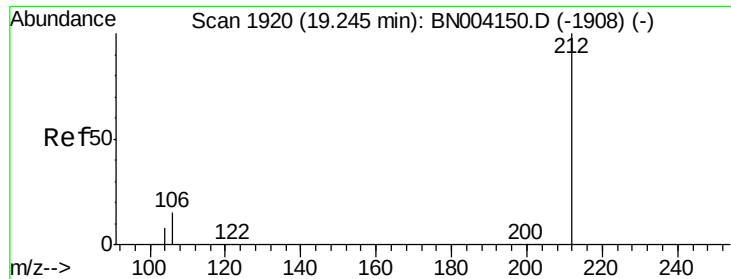

#25
 Fluoranthene-d10
 Concen: 3.388 ng
 RT: 19.24 min Scan# 1919
 Delta R.T. -0.00 min
 Lab File: BN004153.D
 Acq: 20 Dec 2018 16:48




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tot Ion:212 Resp: 154203
 Ion Ratio Lower Upper
 212 100
 106 14.7 10.3 15.5
 104 8.1 5.6 8.4

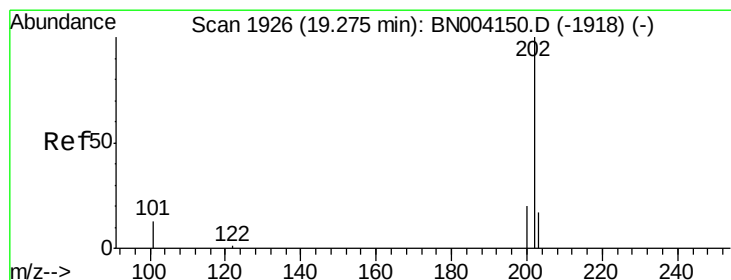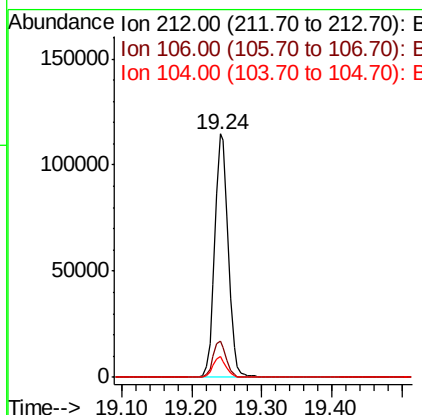

#26
 Fluoranthene
 Concen: 3.410 ng
 RT: 19.27 min Scan# 1925
 Delta R.T. -0.00 min
 Lab File: BN004153.D
 Acq: 20 Dec 2018 16:48

Tgt Ion:202 Resp: 168179
 Ion Ratio Lower Upper
 202 100
 101 12.6 9.0 13.4
 203 17.4 13.8 20.6

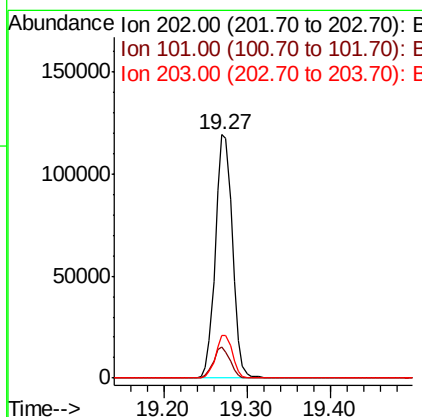



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.41 min Scan# 2205

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:240 Resp: 16680

Ion Ratio Lower Upper

240 100

120 6.3 9.3 13.9#




236 25.1 21.0 31.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

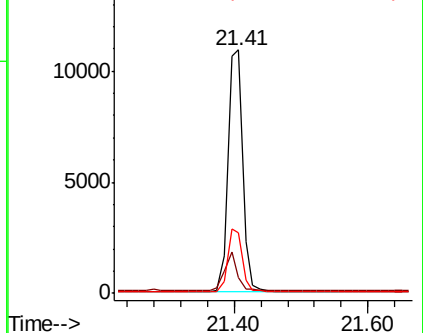

#28

Pyrene

Concen: 3.714 ng

RT: 19.64 min Scan# 1999

Delta R.T. -0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:202 Resp: 171265

Ion Ratio Lower Upper

202 100

200 20.5 16.5 24.7



203 17.5 13.9 20.9




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

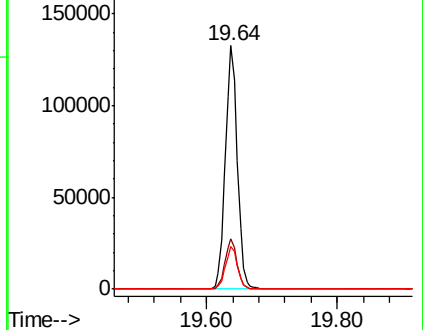



#29

Terphenyl-d14

Concen: 3.361 ng

RT: 19.83 min Scan# 2038

Delta R.T. -0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:244 Resp: 130388

Ion Ratio Lower Upper

244 100

212 6.8 5.6 8.4




122 12.3 8.5 12.7

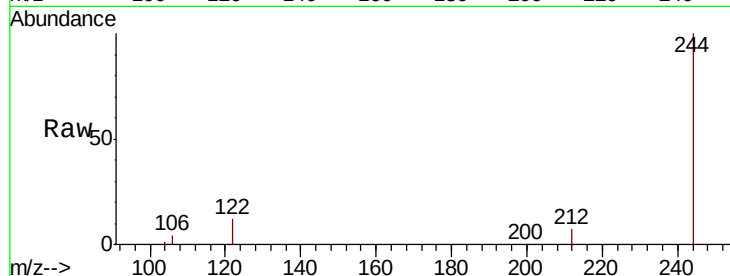

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

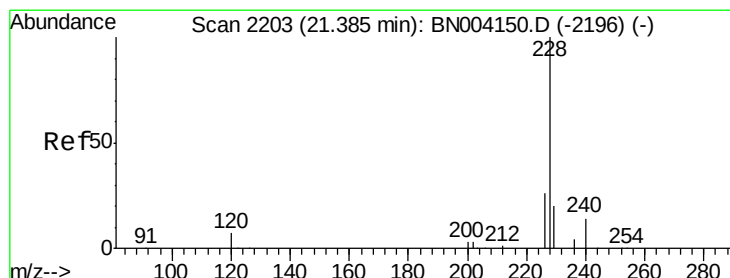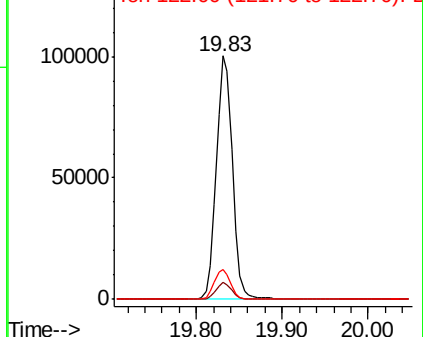

#30

Benzo(a)anthracene

Concen: 3.478 ng

RT: 21.39 min Scan# 2203

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:228 Resp: 152029

Ion Ratio Lower Upper

228 100

226 26.5 20.8 31.2



229 19.6 16.1 24.1

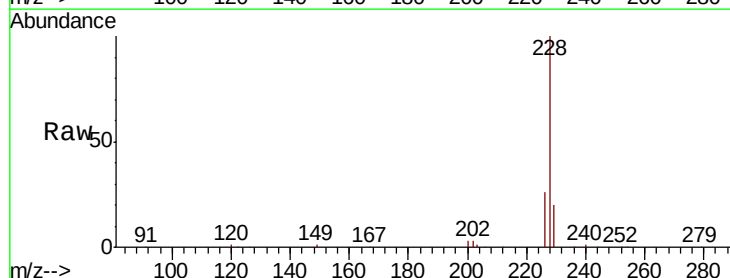


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

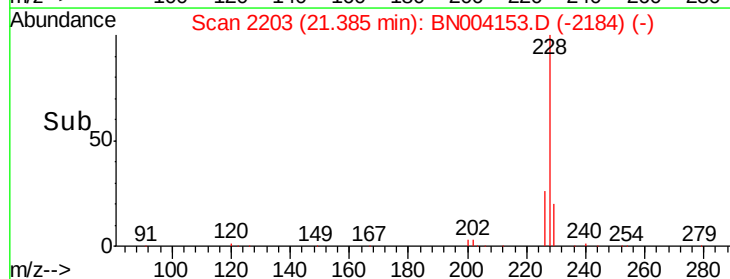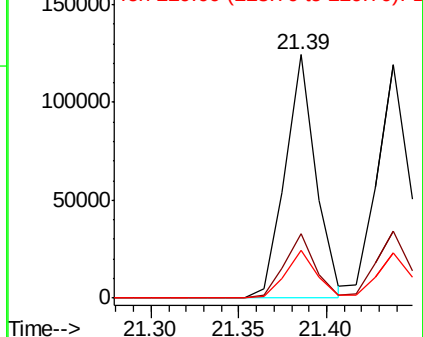

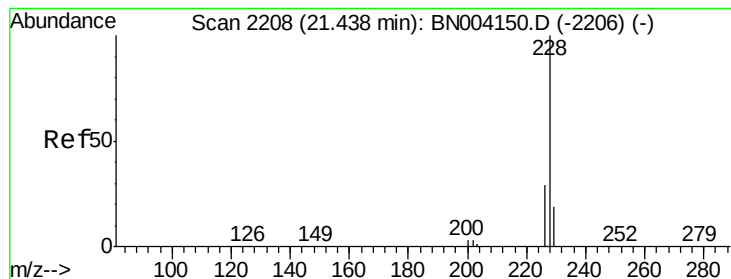

#31

Chrysene

Concen: 3.244 ng

RT: 21.44 min Scan# 2208

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :


BNA_N

ClientSampleId :

SSTDICC3.2

Tot Ion:228 Resp: 152940

Ion	Ratio	Lower	Upper
228	100		
226	29.0	22.7	34.1
229	19.5	16.0	24.0






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

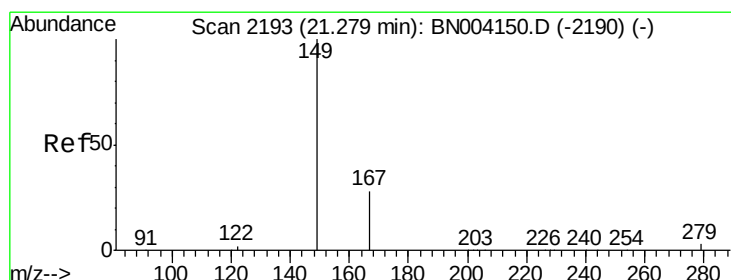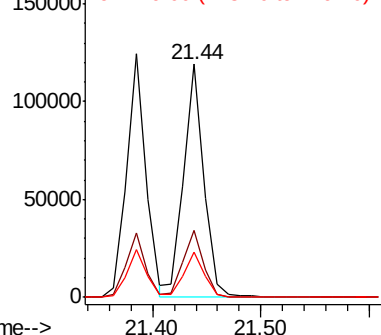

#32

Bis(2-ethylhexyl)phthalate

Concen: 7.323 ng

RT: 21.28 min Scan# 2193


Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Tgt Ion:149 Resp: 94722

Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.4	33.6
279	5.0	3.9	5.9






Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

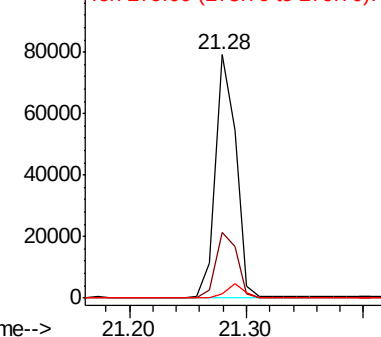



#33

Indeno(1,2,3-cd)pyrene

Concen: 3.261 ng

RT: 26.09 min Scan# 3375

Delta R.T. -0.01 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:276 Resp: 159172

Ion Ratio Lower Upper

276 100

138 26.0 20.6 30.8




277 25.2 20.0 30.0

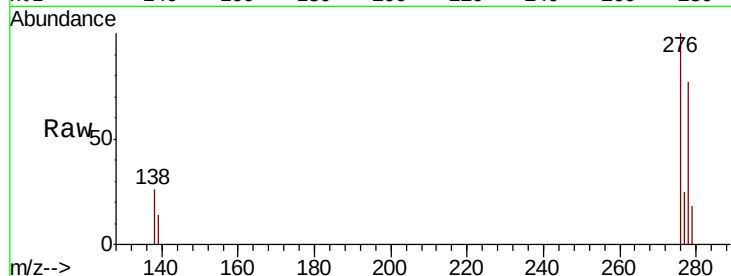

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

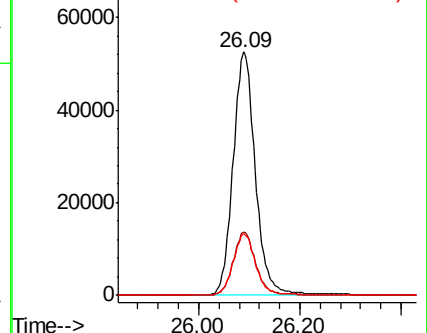

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.73 min Scan# 2685

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:264 Resp: 14842

Ion Ratio Lower Upper

264 100

260 24.7 19.1 28.7



265 30.6 26.4 39.6




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

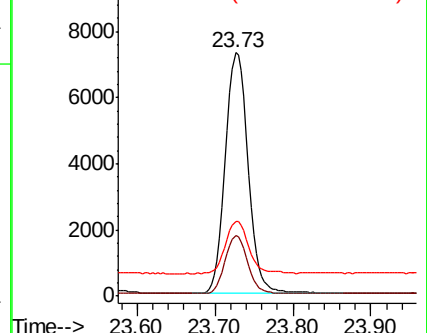

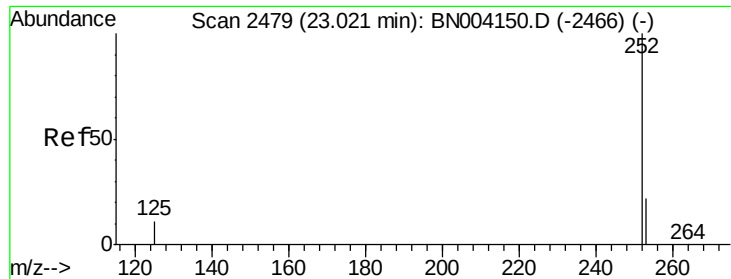

#35

Benzo(b)fluoranthene

Concen: 3.123 ng

RT: 23.02 min Scan# 2479

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:252 Resp: 144624

Ion Ratio Lower Upper

252 100

253 22.3 19.3 28.9

125 10.9 12.7 19.1#






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

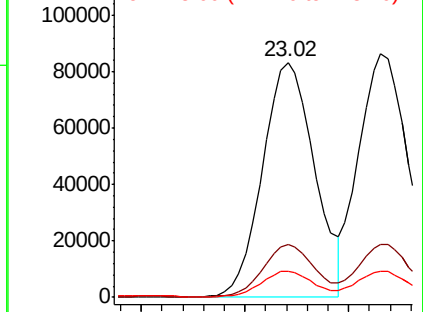

#36

Benzo(k)fluoranthene

Concen: 3.173 ng

RT: 23.07 min Scan# 2492

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:252 Resp: 145531

Ion Ratio Lower Upper

252 100

253 21.9 18.5 27.7

125 10.9 9.1 13.7






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

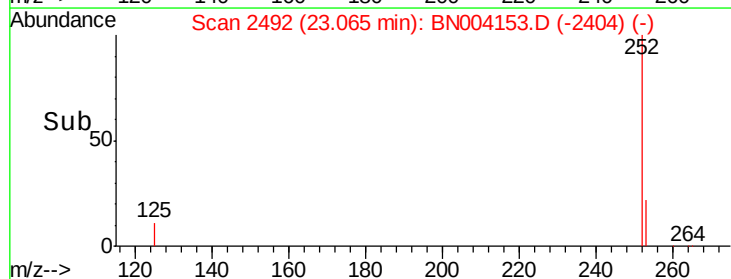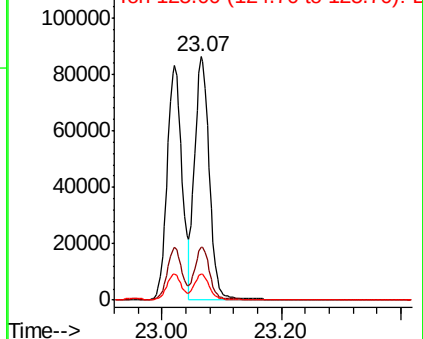

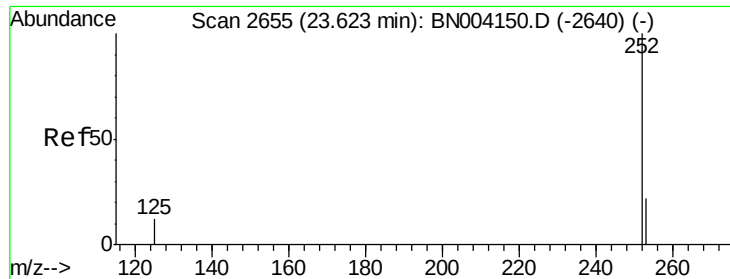

#37

Benzo(a)pyrene

Concen: 3.172 ng

RT: 23.62 min Scan# 2655

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion:252 Resp: 133683

Ion Ratio Lower Upper




252 100

253 21.9 20.1 30.1

125 12.2 16.0 24.0#

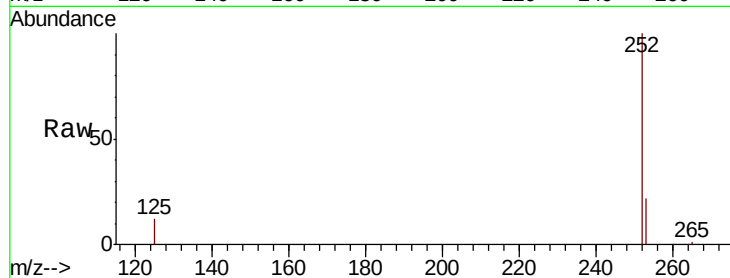

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

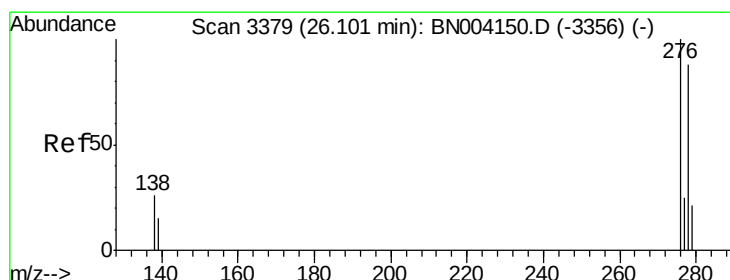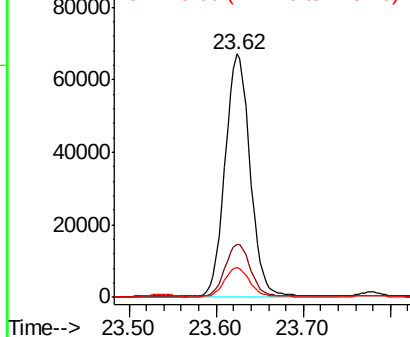

#38

Dibenzo(a,h)anthracene

Concen: 3.398 ng

RT: 26.10 min Scan# 3378

Delta R.T. -0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48


Tgt Ion:278 Resp: 133454

Ion Ratio Lower Upper



278 100


139 17.3 13.5 20.3

279 23.6 19.8 29.6

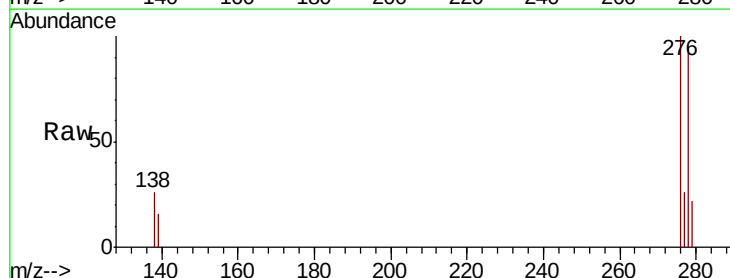

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

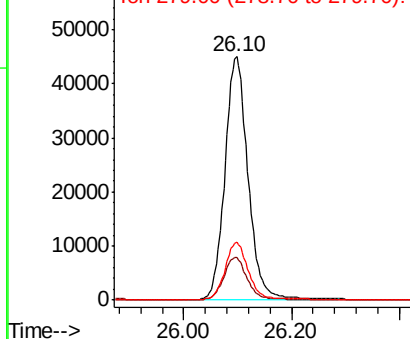

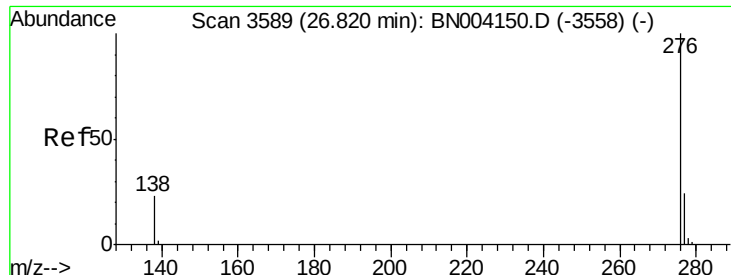

#39

Benzo(a,h,i)perylene

Concen: 3.306 ng

RT: 26.82 min Scan# 3589

Delta R.T. 0.00 min

Lab File: BN004153.D

Acq: 20 Dec 2018 16:48

Instrument :

BNA_N

ClientSampleId :

SSTDICC3.2


Tot Ion: 276 Resp: 129842

Ion Ratio Lower Upper

276 100

277 23.8 19.5 29.3

138 22.8 17.4 26.2

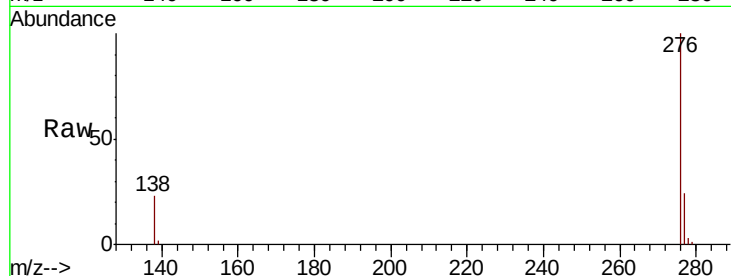

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

