


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122018\
 Data File : BN004147.D
 Acq On : 20 Dec 2018 12:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN122018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 20 17:31:49 2018

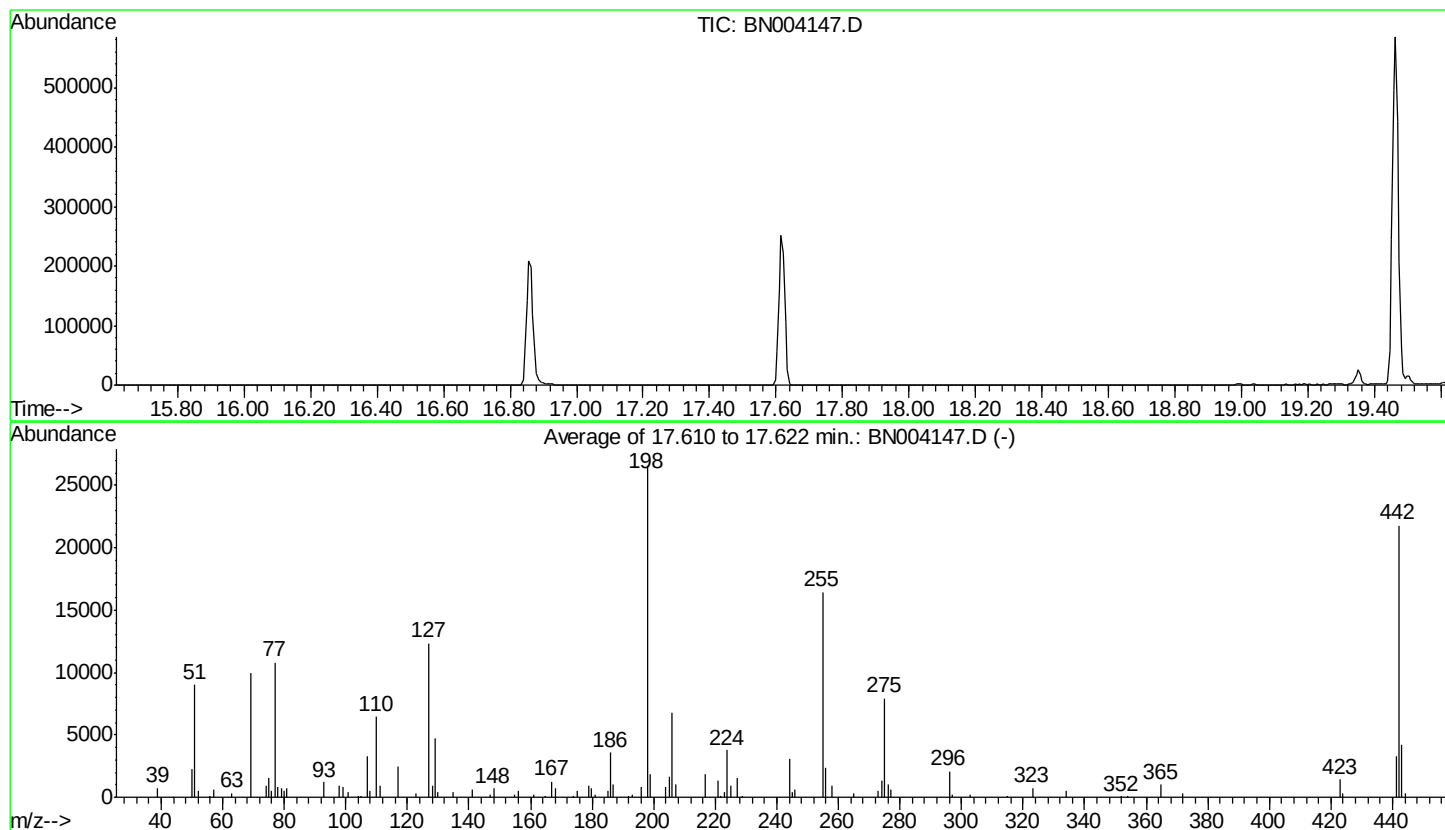

AutoFind: Scans 2486, 2487, 2488; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	9001	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	9914	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	12362	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26581	PASS
199	198	5	9	7.0	1868	PASS
275	198	10	60	29.9	7945	PASS
365	198	1	100	3.7	994	PASS
441	198	0.01	100	12.6	3337	PASS
442	198	50	100	81.9	21763	PASS
443	442	15	24	19.5	4242	PASS