

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN122118\  
 Data File : BN004181.D  
 Acq On : 22 Dec 2018 04:05  
 Operator : JU/SJ  
 Sample : AR1260-50PPM  
 Misc : GC-MS Confirmation  
 ALS Vial : 31 Sample Multiplier: 1

Instrument :  
 BNA\_N  
 ClientSampleId :  
 AR1260-50PPM

## Integration Parameters: LSCINT.P

Integrator: RTE  
 Smoothing : OFF  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 1 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN121218MA.M  
 Title : SVOA CALIBRATION

Signal : TIC

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 7.822       | 816           | 822         | 829          | rBB      | 115889         | 176038        | 25.93%          | 6.200%        |
| 2         | 10.616      | 1291          | 1297        | 1308         | rBV      | 176022         | 296132        | 43.61%          | 10.429%       |
| 3         | 14.463      | 1945          | 1951        | 1963         | rBB2     | 269561         | 424701        | 62.55%          | 14.957%       |
| 4         | 17.210      | 2412          | 2418        | 2432         | rBV2     | 352810         | 515437        | 75.91%          | 18.153%       |
| 5         | 19.116      | 2738          | 2742        | 2746         | rBV      | 8102           | 8486          | 1.25%           | 0.299%        |
| 6         | 19.398      | 2786          | 2790        | 2797         | rBV2     | 11996          | 13205         | 1.94%           | 0.465%        |
| 7         | 19.963      | 2884          | 2886        | 2890         | rBV      | 9121           | 8109          | 1.19%           | 0.286%        |
| 8         | 20.104      | 2906          | 2910        | 2917         | rBV4     | 37365          | 39297         | 5.79%           | 1.384%        |
| 9         | 20.380      | 2953          | 2957        | 2964         | rBV      | 41380          | 43847         | 6.46%           | 1.544%        |
| 10        | 20.439      | 2964          | 2967        | 2971         | rVB      | 8833           | 7928          | 1.17%           | 0.279%        |
| 11        | 20.545      | 2981          | 2985        | 2988         | rBV2     | 10439          | 12306         | 1.81%           | 0.433%        |
| 12        | 20.704      | 3005          | 3012        | 3016         | rBV      | 24743          | 38437         | 5.66%           | 1.354%        |
| 13        | 20.845      | 3033          | 3036        | 3039         | rBV      | 16712          | 16457         | 2.42%           | 0.580%        |
| 14        | 21.116      | 3079          | 3082        | 3086         | rBV      | 14714          | 13483         | 1.99%           | 0.475%        |
| 15        | 21.398      | 3124          | 3130        | 3137         | rBV      | 521830         | 678978        | 100.00%         | 23.912%       |
| 16        | 21.721      | 3182          | 3185        | 3191         | rVB3     | 11272          | 13715         | 2.02%           | 0.483%        |
| 17        | 21.851      | 3204          | 3207        | 3211         | rVB2     | 7694           | 7924          | 1.17%           | 0.279%        |
| 18        | 23.721      | 3517          | 3525        | 3537         | rVB2     | 264233         | 524992        | 77.32%          | 18.489%       |


Sum of corrected areas: 2839472

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_N\DATA\BN122118\  
Data File : BN004181.D  
Acq On : 22 Dec 2018 04:05  
Operator : JU/SJ  
Sample : AR1260-50PPM  
Misc : GC-MS Confirmation  
ALS Vial : 31 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
AR1260-50PPM

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN121218MA.M  
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

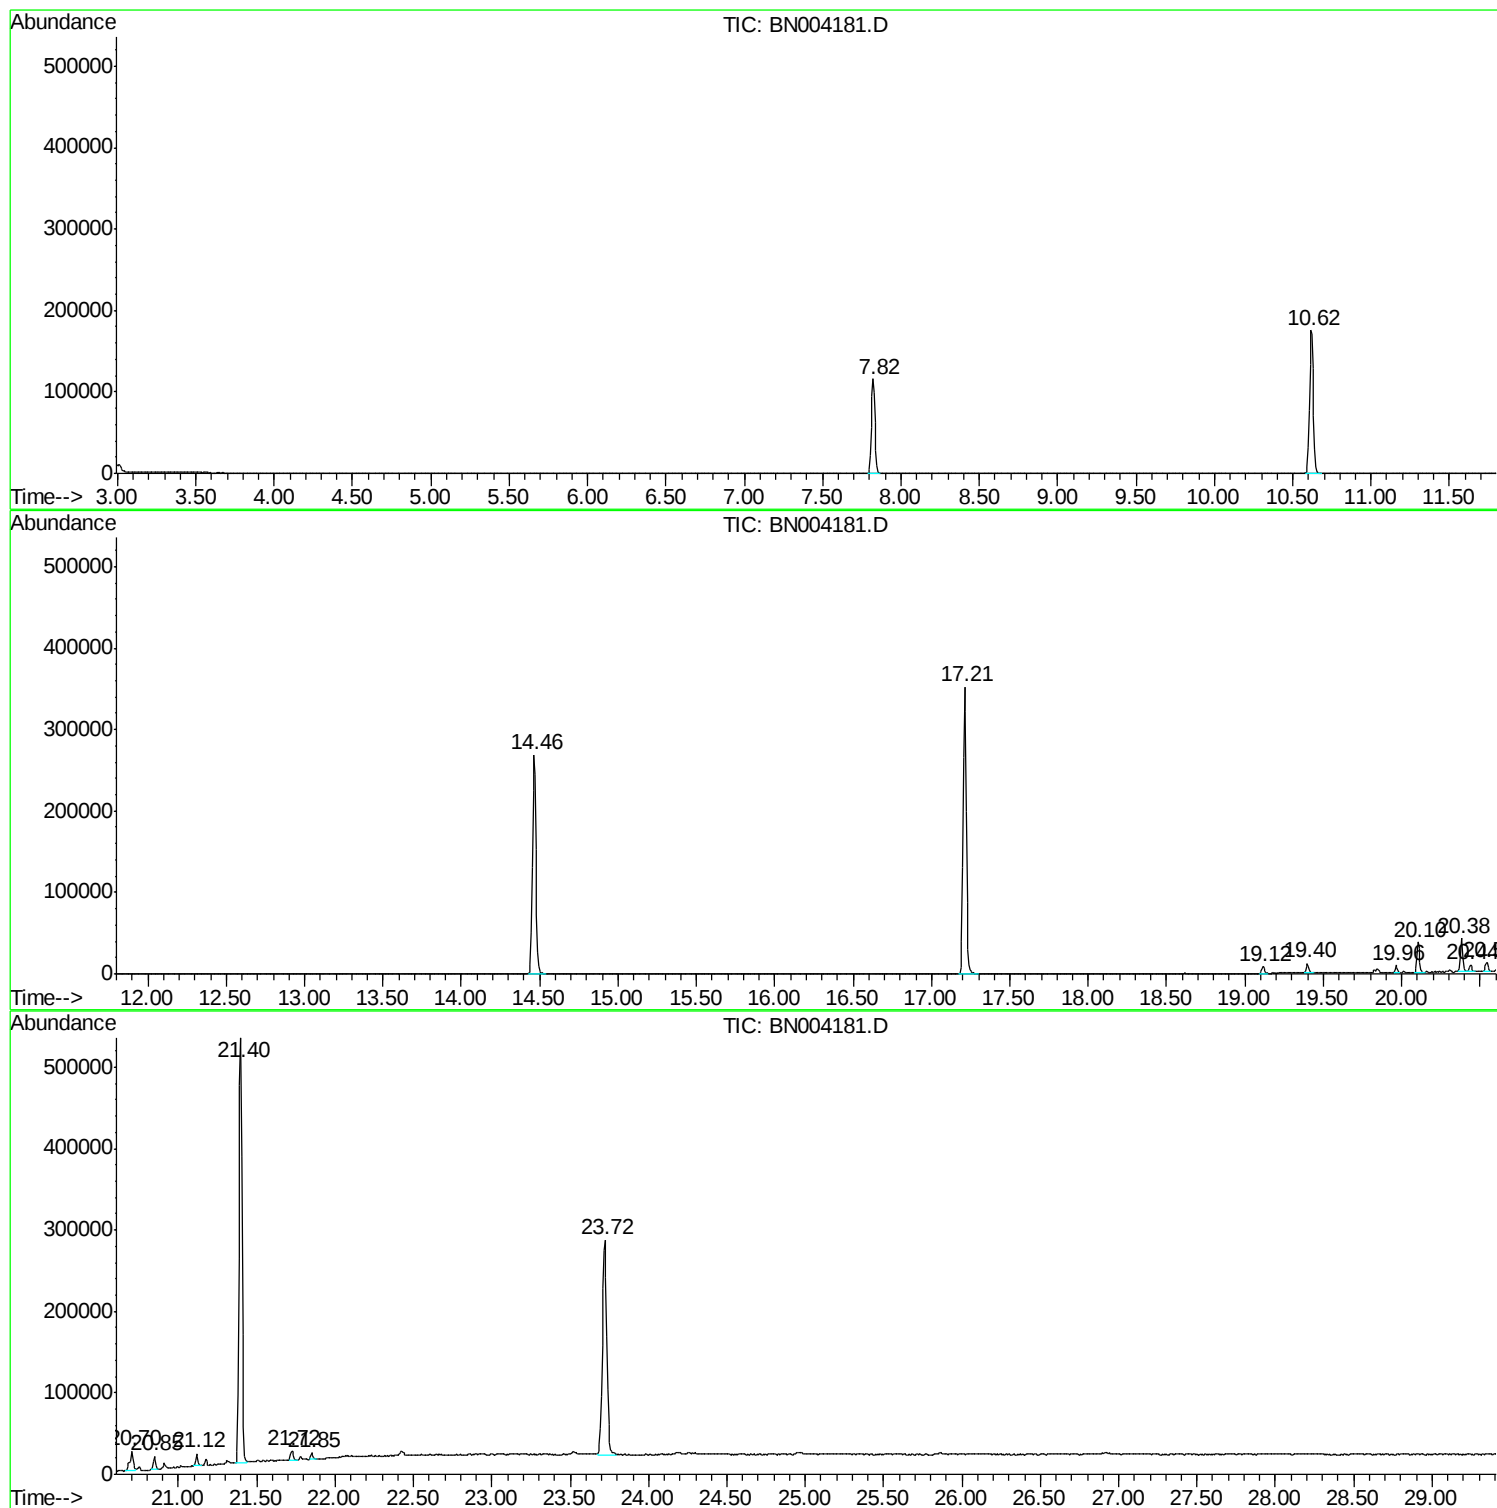

DbaaaPath::ZZ\SS0088RVNPE00001BBN\ANNDATA\ABBN222188\  
 DbaaaFile::BBN001881DD  
 AcqQ00n::222Dec2008 004005  
 Operator::JUSJ  
 Sample::ARR2000500PPM  
 Misc::GCMSC00ffimaaion  
 AASSVal::331 SampleMultiplier:11

Instrument :  
 BNA\_N  
 ClientSampleId :  
 AR1260-50PPM

QqantMebdd::ZZ\SS0088RVNPE00001BBN\ANNDATA\ABBN222188\AMM  
 QqantTitle::SS00ACALIBRATION

TICLibrary::CC\DaabbaaeN0\$T11LL  
 TICIntegrat00onParameters:LS6CNTTP

| TIC Top Hit name | RT | EstConc | Units | Response | Internal Standard |
|------------------|----|---------|-------|----------|-------------------|
|                  |    |         |       | #        | RT Resp Conc      |

No Library Search Compounds Detected

\*\*\*\*\*