

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122221\
 Data File : BN018158.D
 Acq On : 22 Dec 2021 19:35
 Operator : CG/JU
 Sample : M5091-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3C6

Quant Time: Dec 23 00:08:35 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 14:08:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	3908	0.400	ng/ul	0.00
4) Naphthalene-d8	10.388	136	12900	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.249	164	8986	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.995	188	20273	0.400	ng/ul	0.00
17) Chrysene-d12	21.192	240	17953	0.400	ng/ul	0.00
23) Perylene-d12	23.416	264	21759	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.076	96	18370	4.548	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	6175	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.027	212	20930	0.430	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.438	128	3187	0.087	ng/ul#	94
7) 2-Methylnaphthalene	12.066	142	685	0.029	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122221\
Data File : BN018158.D
Acq On : 22 Dec 2021 19:35
Operator : CG/JU
Sample : M5091-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3C6

Quant Time: Dec 23 00:08:35 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 14:08:04 2021
Response via : Initial Calibration




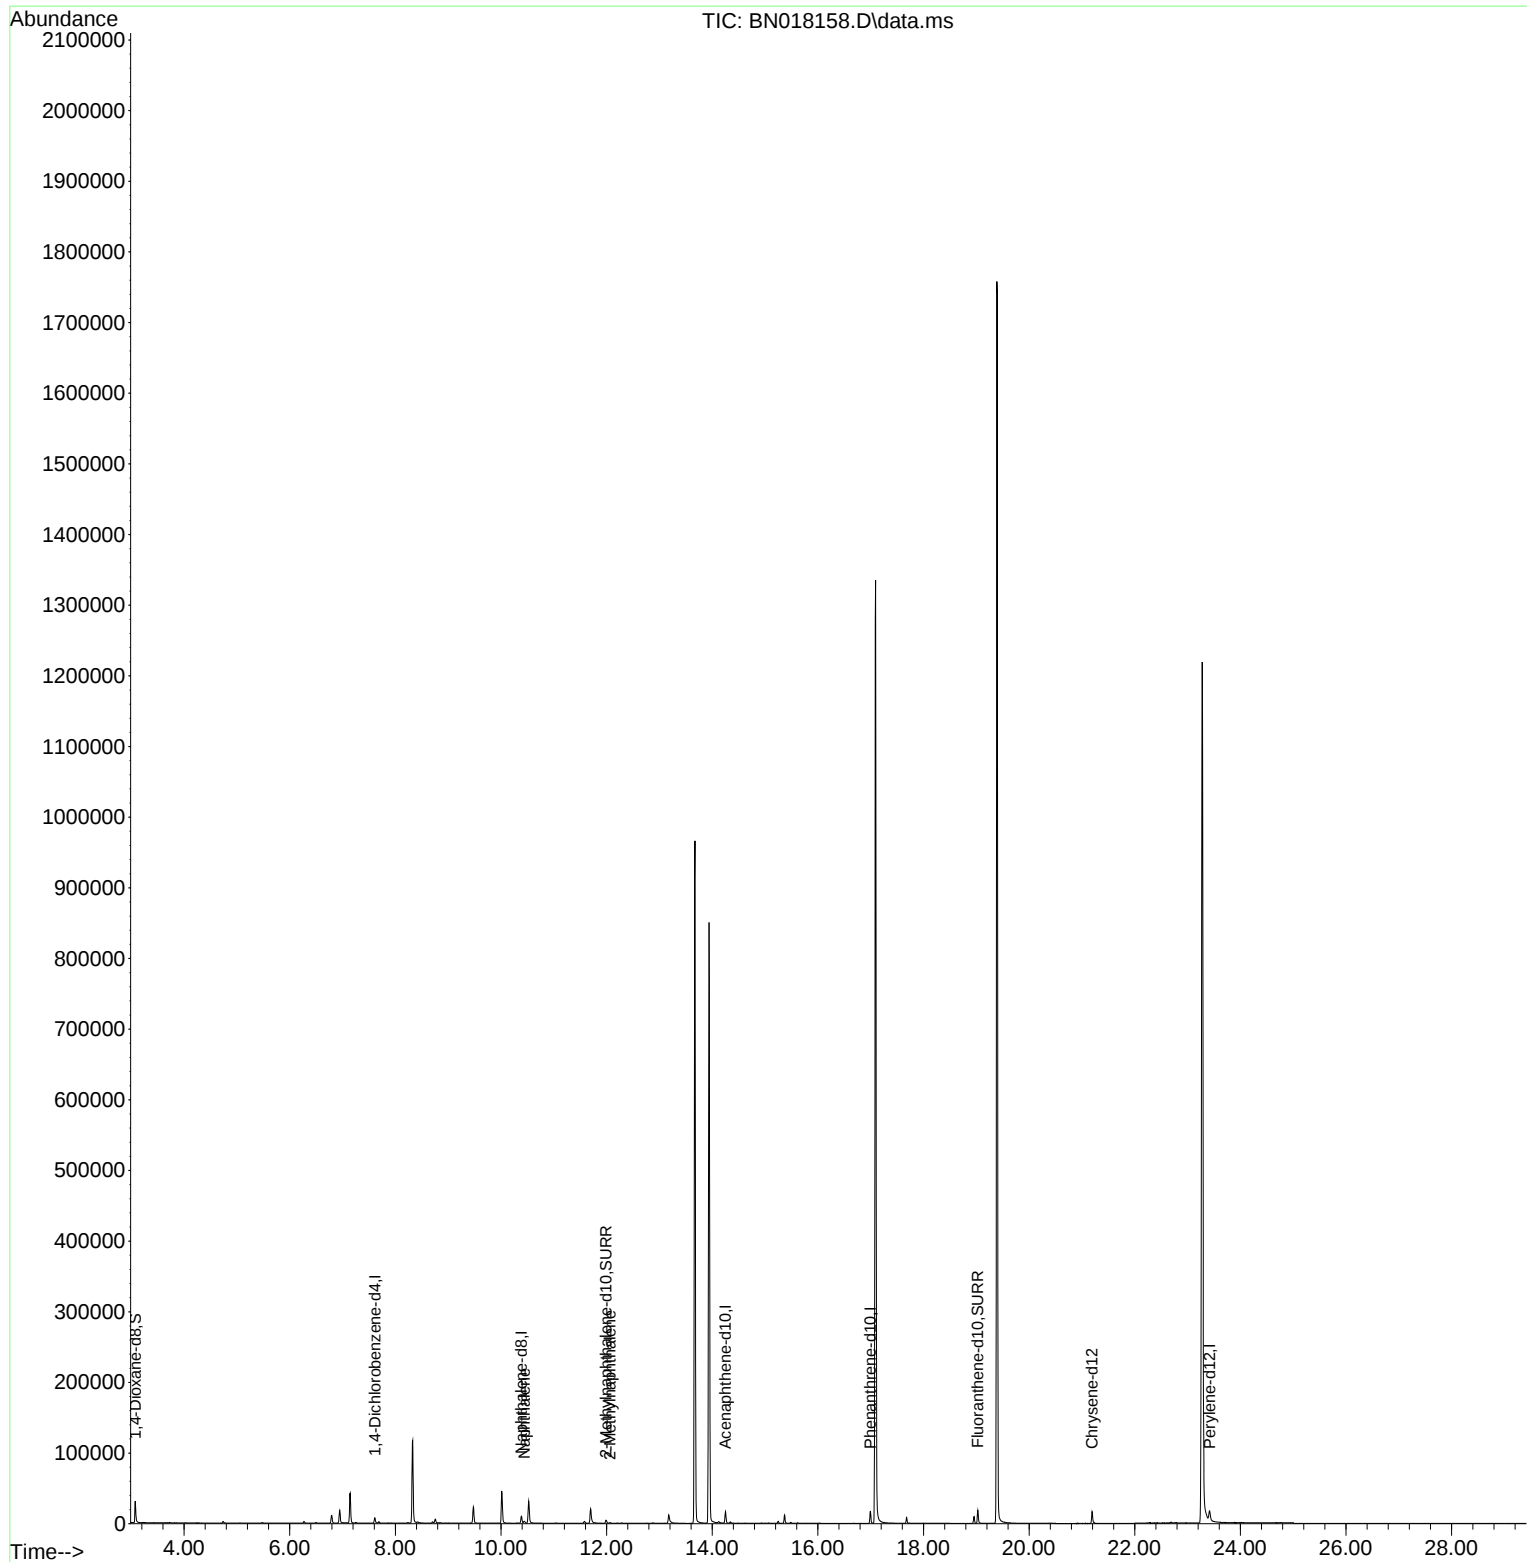


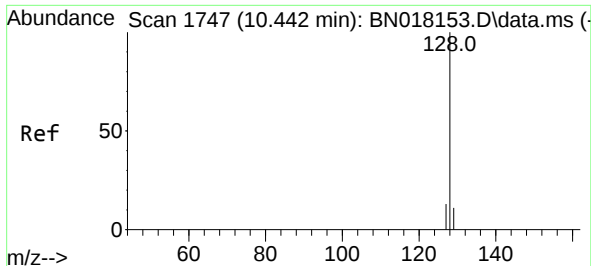

#5
Naphthalene
Concen: 0.087 ng/ul
RT: 10.438 min Scan# 1746
Delta R.T. -0.000 min
Lab File: BN018158.D
Acq: 22 Dec 2021 19:35

Instrument :
BNA_N
ClientSampleId :
BG3C6

Tgt Ion:128 Resp: 3187
Ion Ratio Lower Upper
128 100
129 14.1 9.3 13.9#
127 15.9 11.1 16.7

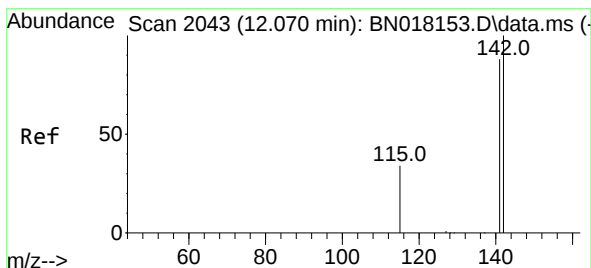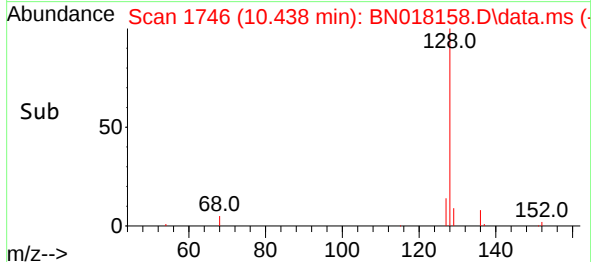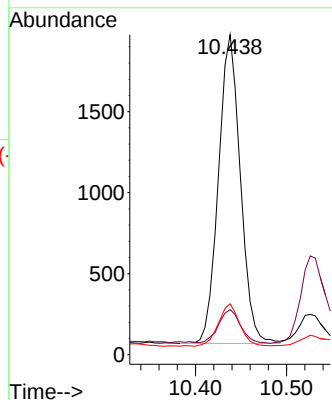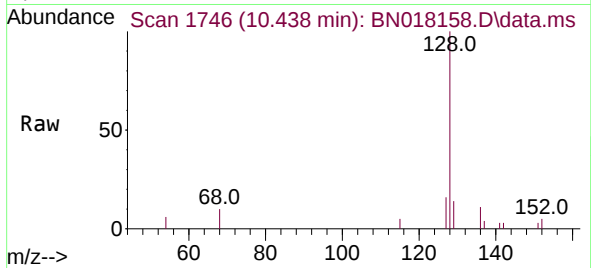

#7
2-Methylnaphthalene
Concen: 0.029 ng/ul
RT: 12.066 min Scan# 2042
Delta R.T. -0.000 min
Lab File: BN018158.D
Acq: 22 Dec 2021 19:35

Tgt Ion:142 Resp: 685
Ion Ratio Lower Upper
142 100
141 88.2 70.6 105.8

