

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122221\
 Data File : BN018159.D
 Acq On : 22 Dec 2021 20:11
 Operator : CG/JU
 Sample : M5091-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BG3C2

Quant Time: Dec 23 00:09:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 14:08:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.611	152	3695	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	12283	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.253	164	8438	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.994	188	19579	0.400	ng/ul	0.00
17) Chrysene-d12	21.190	240	18316	0.400	ng/ul	0.00
23) Perylene-d12	23.417	264	20852	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.076	96	19343	5.065	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.993	152	6136	0.363	ng/ul	0.00
18) Fluoranthene-d10	19.026	212	23620	0.475	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.109	88	509	0.110	ng/ul#	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122221\
Data File : BN018159.D
Acq On : 22 Dec 2021 20:11
Operator : CG/JU
Sample : M5091-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BG3C2


Quant Time: Dec 23 00:09:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 14:08:04 2021
Response via : Initial Calibration

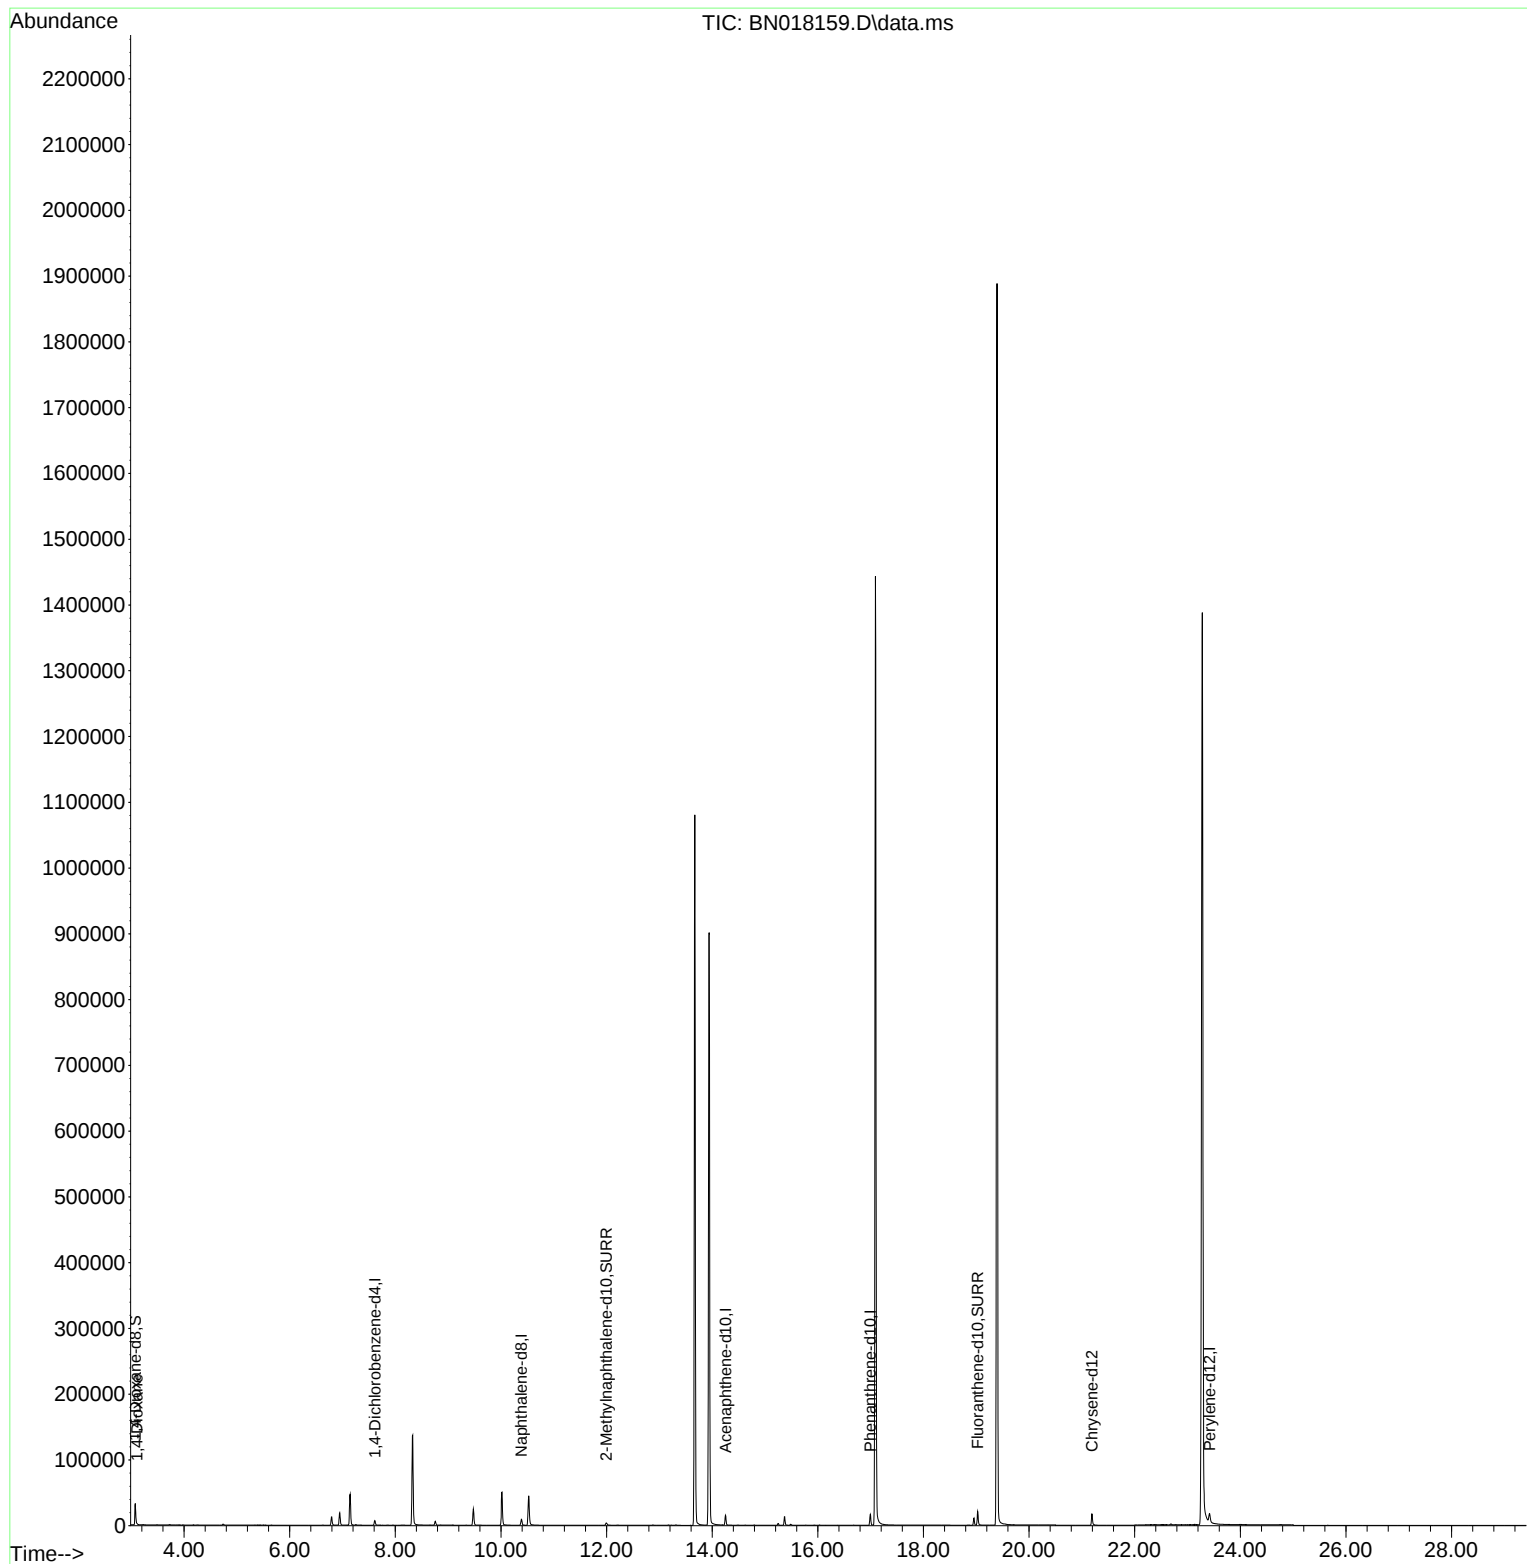

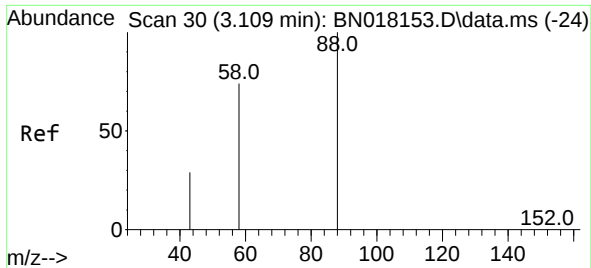

#2
 1,4-Dioxane
 Concen: 0.110 ng/ul
 RT: 3.109 min Scan# 30
 Delta R.T. -0.004 min
 Lab File: BN018159.D
 Acq: 22 Dec 2021 20:11

Instrument :
 BNA_N
 ClientSampleId :
 BG3C2

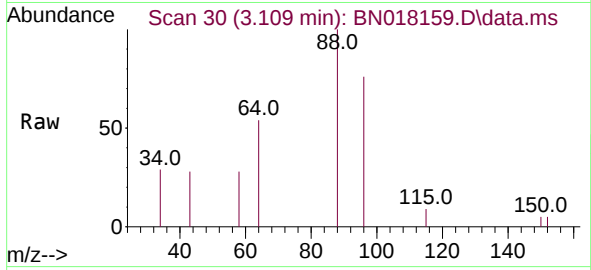

Tgt Ion: 88	Resp: 509
Ion Ratio	Lower Upper
88	100
43	28.4 24.6 36.8
58	27.5 45.2 67.8#

