


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122321\
 Data File : BN018172.D
 Acq On : 23 Dec 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN122321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 23 14:22:48 2021

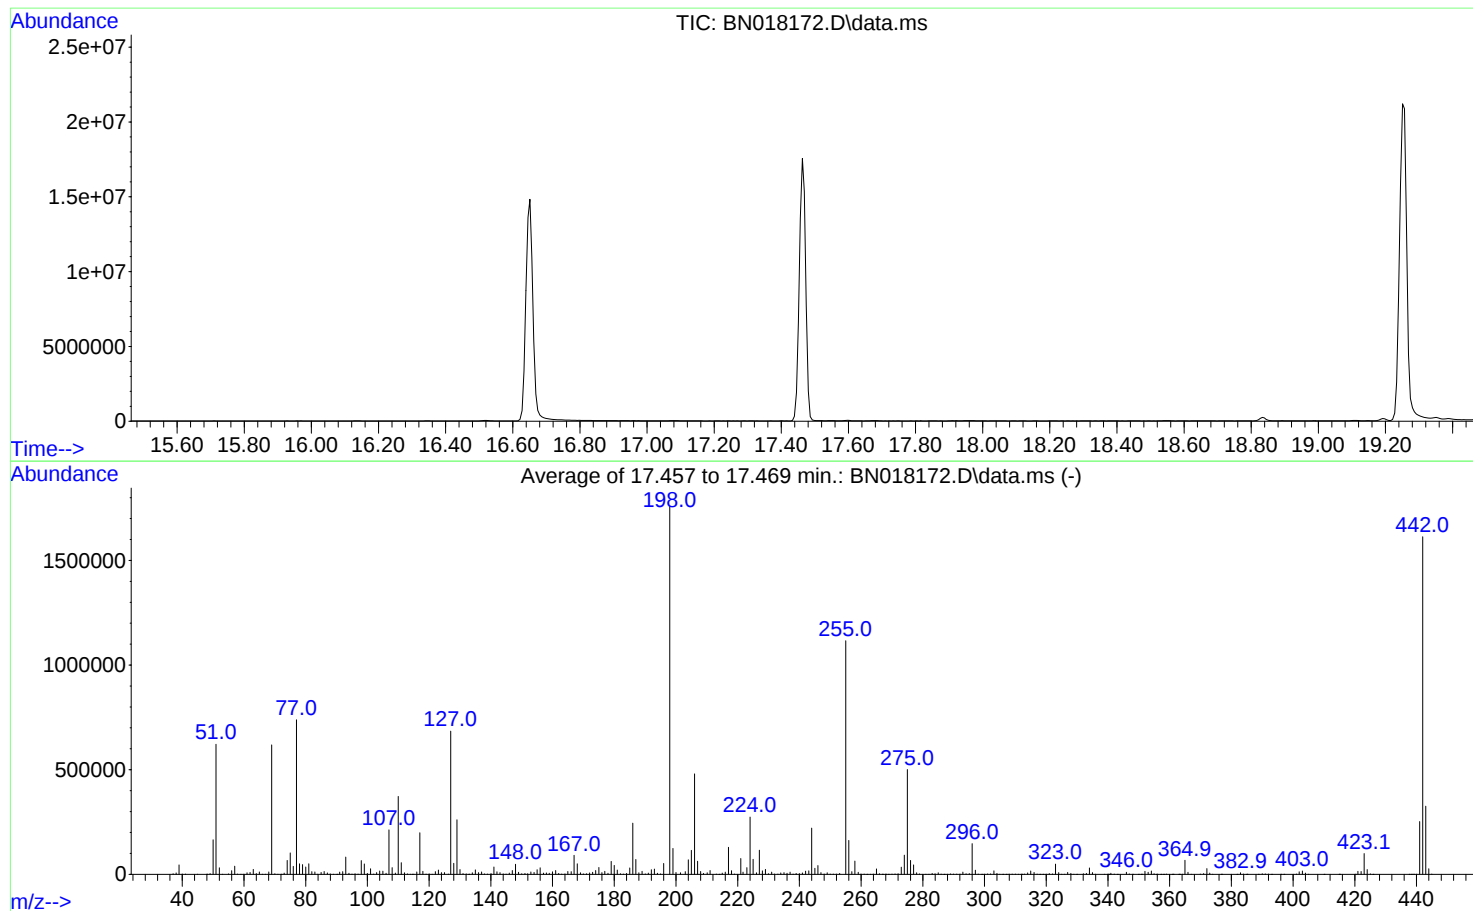

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	621577	PASS
68	69	0.00	2	1.9	11755	PASS
69	198	0.00	100	35.2	618688	PASS
70	69	0.00	2	0.5	3210	PASS
127	198	10	80	39.0	684651	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1757696	PASS
199	198	5	9	7.0	123541	PASS
275	198	10	60	28.5	500437	PASS
365	198	1	100	3.8	67192	PASS
441	198	0.01	100	14.4	252267	PASS
442	442	50	100	100.0	1613312	PASS
443	442	15	24	20.2	325653	PASS

Instrument :
BNA_N
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/23/2021	BNA_N	<u>BN018172.D</u>
Compound Name	Response	Retention Time
DDT	6735287	20.85
DDD	127523	20.49
DDE	7098	19.54
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
134621	6869908	1.96

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122321\
 Data File : BN018172.D
 Acq On : 23 Dec 2021 08:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 31 05:24:37 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 30 05:13:58 2021
 Response via : Initial Calibration

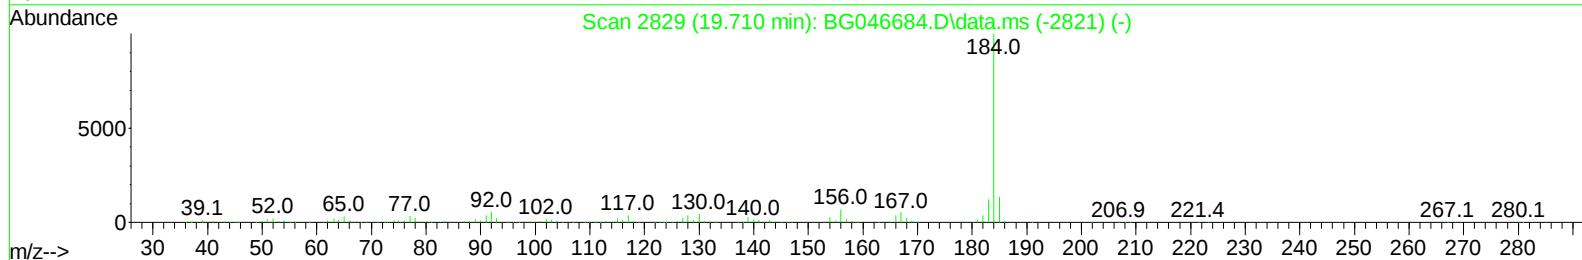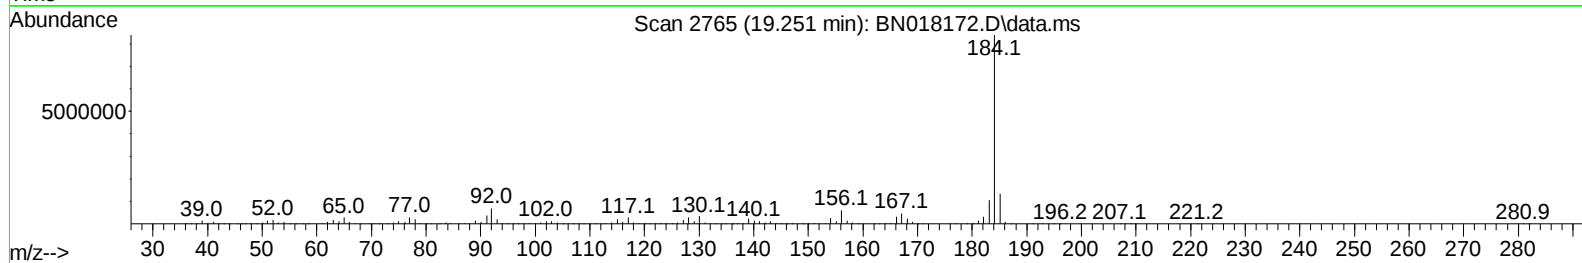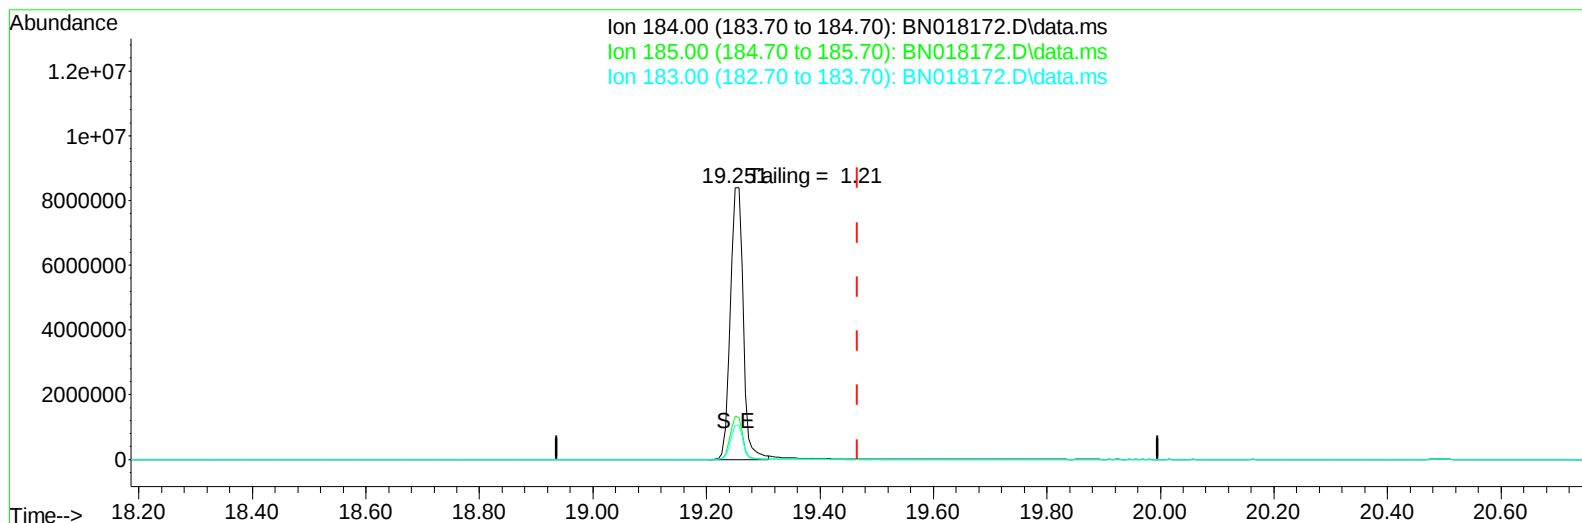

TIC: BN018172.D\data.ms




(77) Benzidine**19.251min (-0.215) 4048943.39 ng****response 13479500**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	16.03
183.00	13.20	12.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122321\
Data File : BN018172.D
Acq On : 23 Dec 2021 08:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 31 05:24:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 30 05:13:58 2021
Response via : Initial Calibration

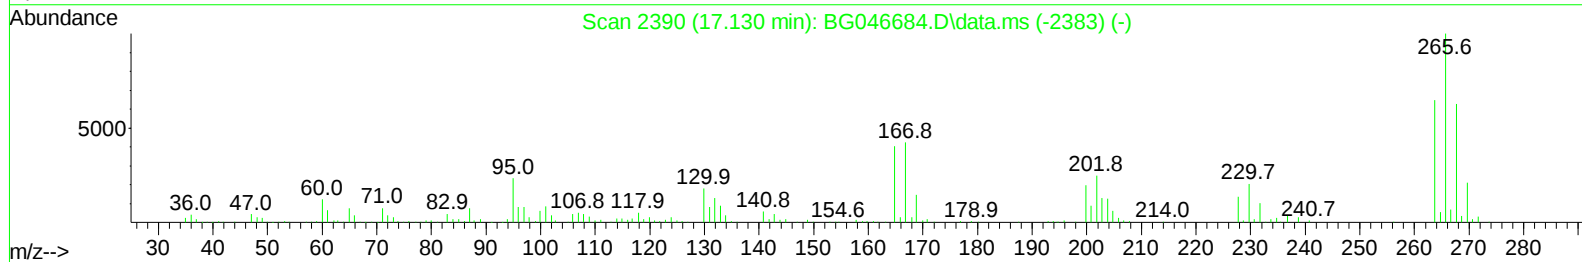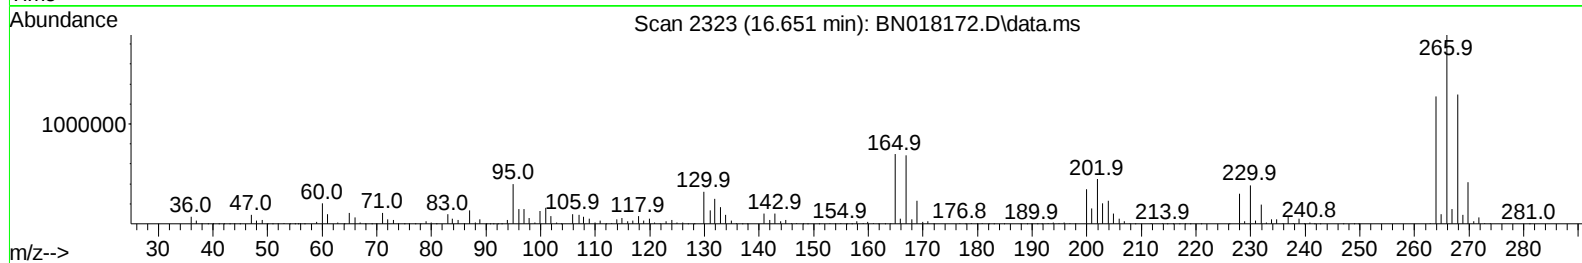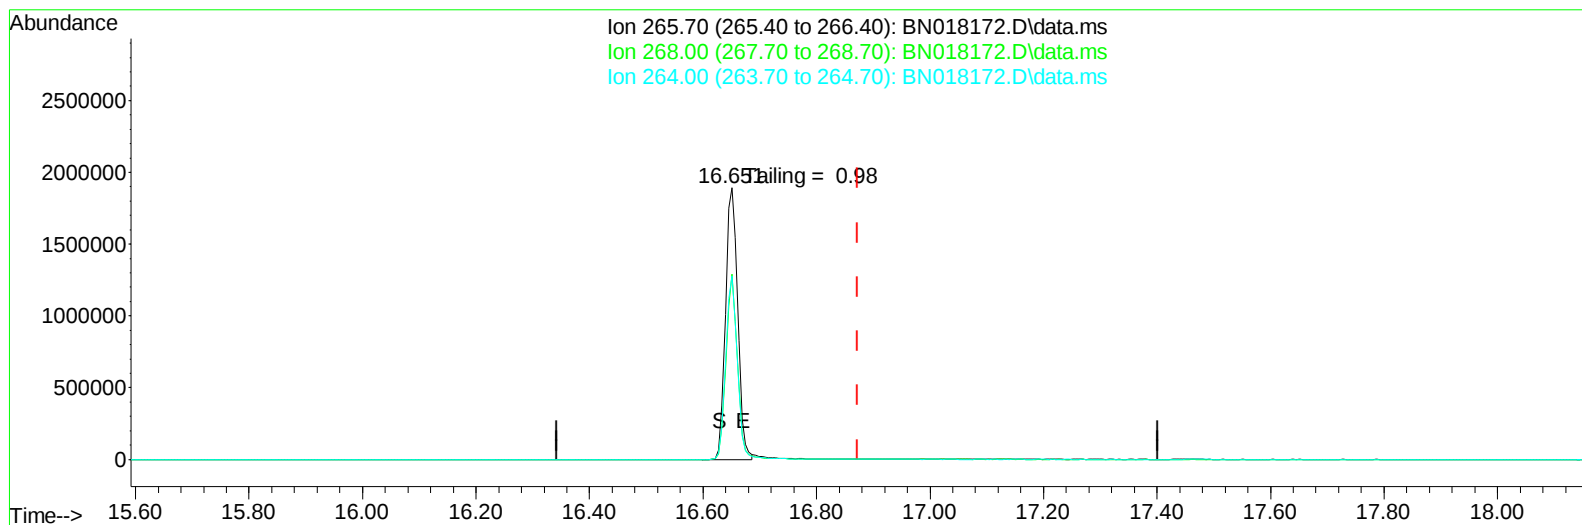

TIC: BN018172.D\data.ms

(70) Pentachlorophenol (C)

16.651min (-0.221) 32029.44 ng

response 2868509

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.38
264.00	61.60	67.49
0.00	0.00	0.00