


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122321\
 Data File : BN018188.D
 Acq On : 23 Dec 2021 19:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN122321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 23 14:22:48 2021

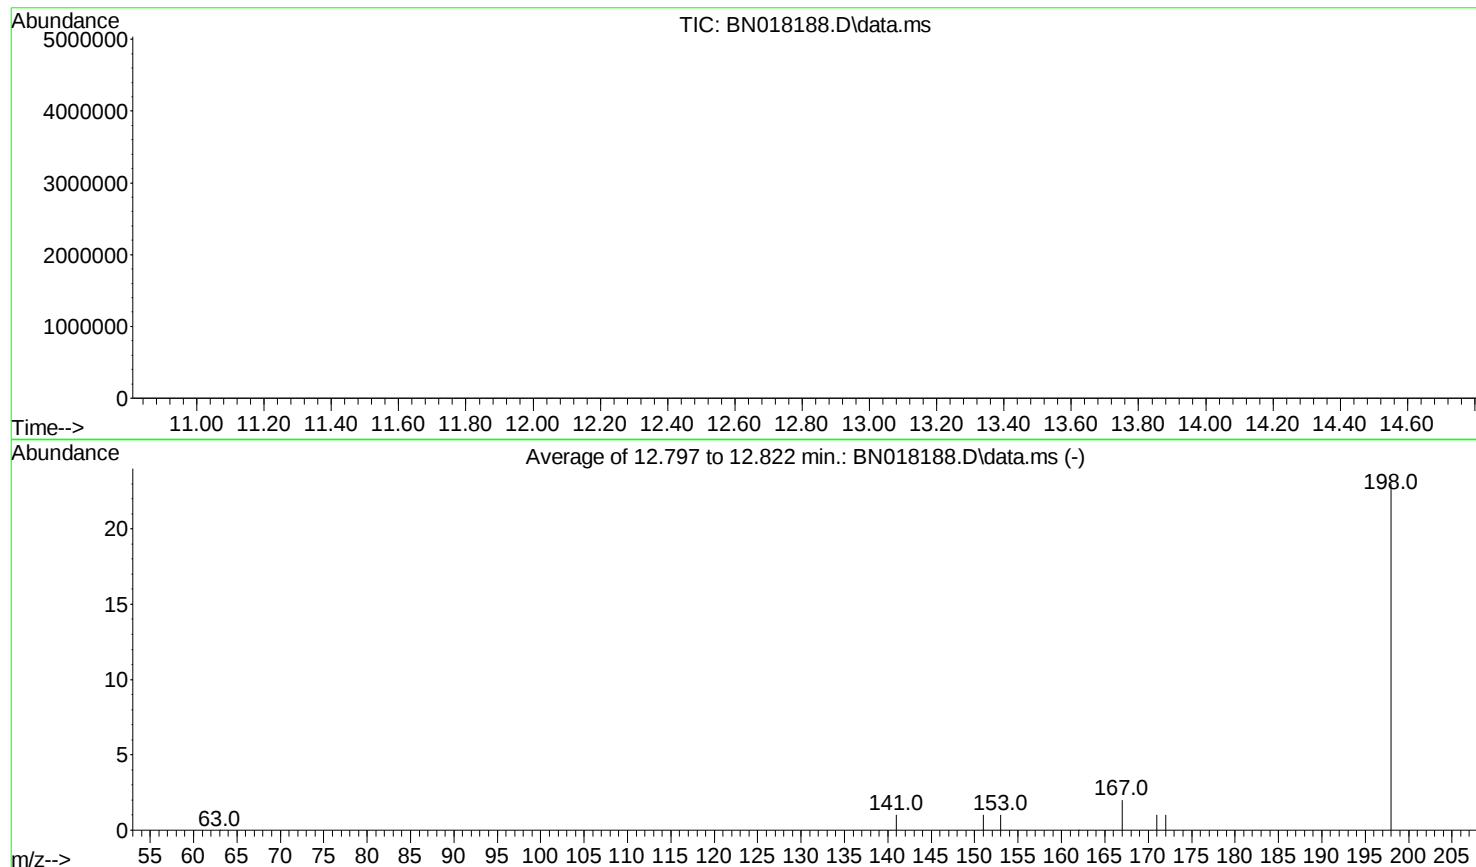

AutoFind: Scans 1067, 1068, 1069; Background Corrected with Scan 1064

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	0.0	0	FAIL*
68.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
69	198	0.00	100	0.0	0	PASS
70.00	69.00	COMPARISON MASS IS NOT PRESENT!!!				
127	198	10	80	0.0	0	FAIL*
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	23	PASS
199	198	5	9	0.0	0	FAIL*
275	198	10	60	0.0	0	FAIL*
365	198	1	100	0.0	0	FAIL*
441	198	0.01	100	0.0	0	FAIL*
442.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				
443.00	442.00	COMPARISON MASS IS NOT PRESENT!!!				