

Data File : BN009136.D
Acq On : 24 Dec 2019 21:33
Operator : JU
Sample : K6257-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFEZ8

Quant Time: Dec 25 01:09:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	159557	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	746797	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.16	164	531852	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1233746	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1271904	20.00	ng/ul	0.00
85) Perylene-d12	23.24	264	1485901	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	18838	5.39	ng/uL	0.00
5) Phenol-d5	6.72	99	463958	30.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	333133	34.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	348673	32.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	396143	32.35	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	192682	34.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	216638	34.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	377966	31.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	554454	38.82	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	1431620	35.84	ng/ul	0.00
46) Acenaphthylene-d8	13.85	160	1659789	35.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	222410	28.00	ng/ul	0.00
57) Fluorene-d10	15.16	176	1254314	36.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	185595	24.11	ng/ul	0.00
70) Anthracene-d10	17.00	188	1985000	34.59	ng/ul	0.00
78) Pyrene-d10	19.30	212	2341991	35.29	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	2651958	35.42	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.23	70	11247	1.081 ng/ul#	1
44) Dimethylphthalate	13.62	163	254729	6.235 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009136.D
Acq On : 24 Dec 2019 21:33
Operator : JU
Sample : K6257-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFEZ8

Quant Time: Dec 25 01:09:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration




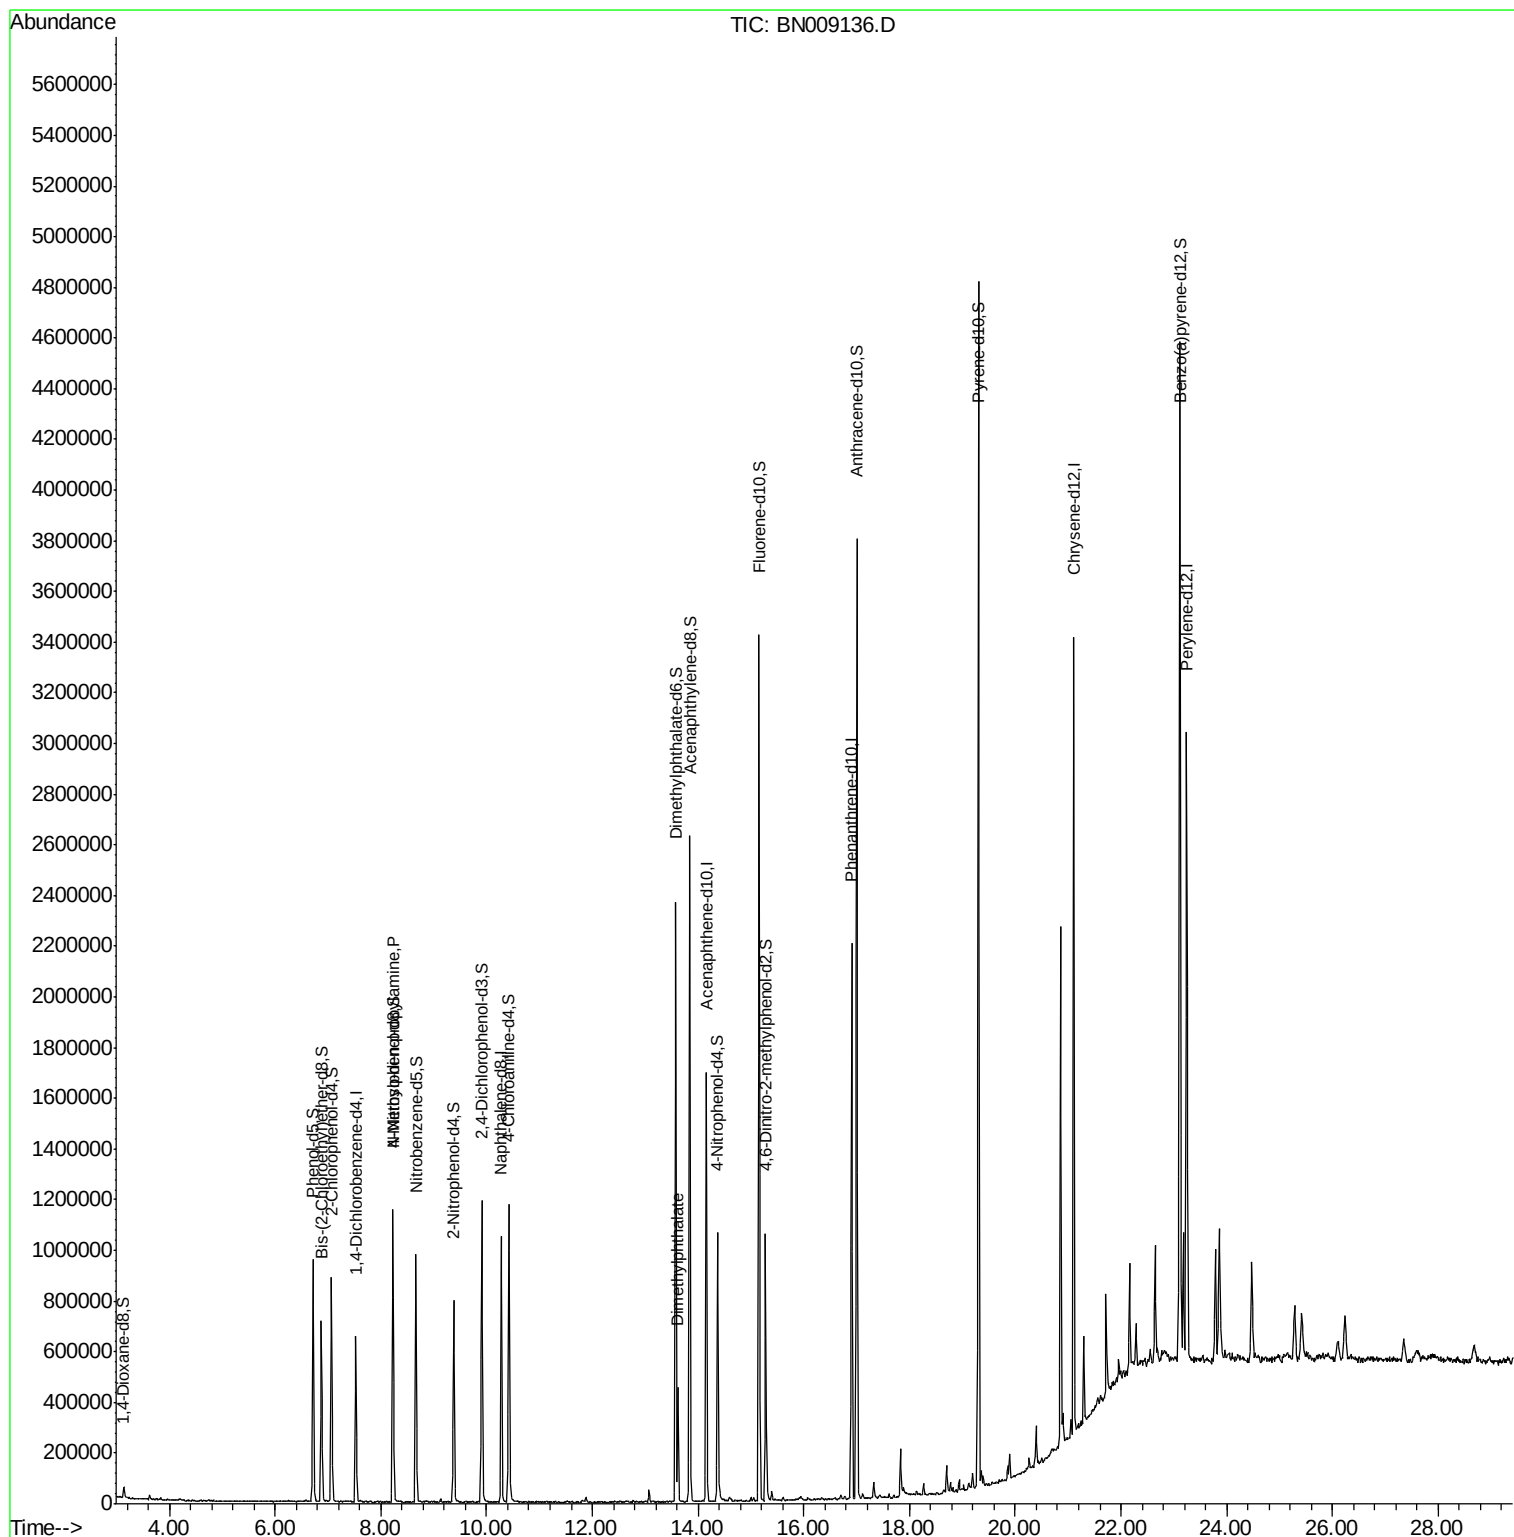


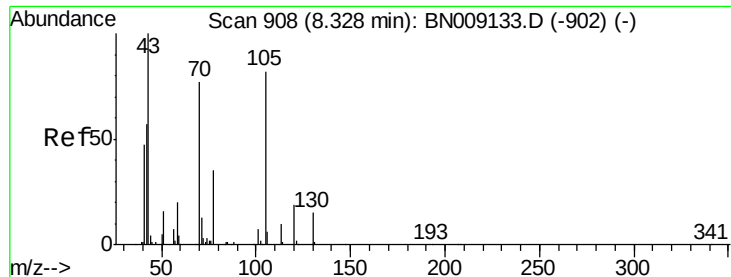

#15
N-Nitroso-di-n-propylamine
Concen: 1.081 ng/ul
RT: 8.23 min Scan# 892
Delta R.T. -0.09 min
Lab File: BN009136.D
Acq: 24 Dec 2019 21:33

Instrument :
BNA_N
ClientSampleId :
BFEZ8

Tgt Ion:	70	Resp:	11247
Ion	Ratio	Lower	Upper
70	100		
42	481.8	60.4	90.6#
101	0.0	7.4	11.0#
130	0.0	15.8	23.8#

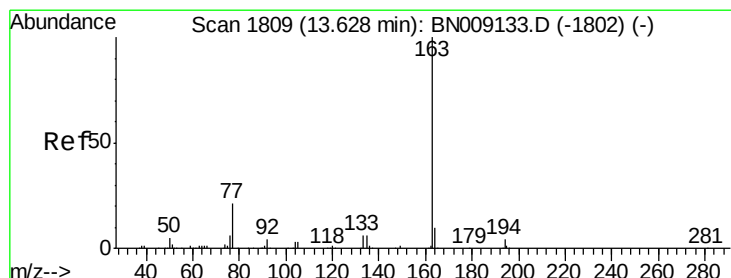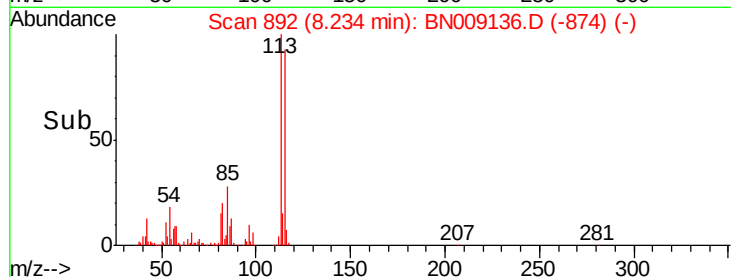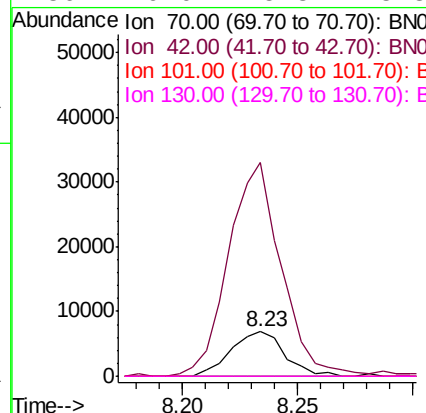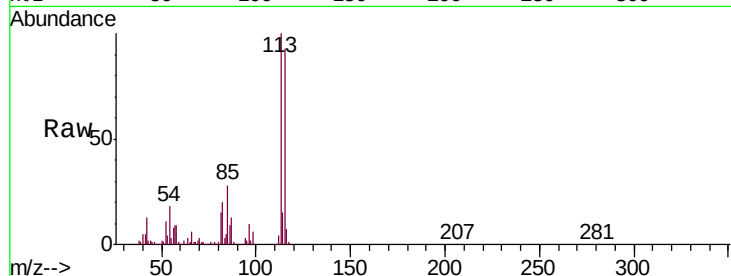

#44
Dimethylphthalate
Concen: 6.235 ng/ul
RT: 13.62 min Scan# 1808
Delta R.T. -0.01 min
Lab File: BN009136.D
Acq: 24 Dec 2019 21:33

Tgt Ion:	163	Resp:	254729
Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.5	5.3
164	9.8	8.3	12.5

