

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122419\
 Data File : BN009154.D
 Acq On : 25 Dec 2019 08:53
 Operator : JU
 Sample : PB125531 BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 25 12:21:04 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	230733	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	1089553	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.16	164	745859	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1642803	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1580197	20.00	ng/ul	0.00
85) Perylene-d12	23.25	264	1711083	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	43643	8.64	ng/uL	0.00
5) Phenol-d5	6.72	99	961981	43.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	670860	47.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	731133	46.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	804811	45.45	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	400734	48.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	456293	49.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	776610	44.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	1177993	56.53	ng/ul	0.00
43) Dimethylphthalate-d6	13.58	166	2742425	48.96	ng/ul	0.00
46) Acenaphthylene-d8	13.85	160	3230646	49.19	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	515314	46.26	ng/ul	0.00
57) Fluorene-d10	15.16	176	2363753	48.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	411418	40.14	ng/ul	0.00
70) Anthracene-d10	17.00	188	3758048	49.18	ng/ul	0.00
78) Pyrene-d10	19.31	212	4137477	50.19	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	4295913	49.83	ng/ul	0.00

Target Compounds


				Ovalue		
15) N-Nitroso-di-n-propylamine	8.23	70	21587	1.435	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
Data File : BN009154.D
Acq On : 25 Dec 2019 08:53
Operator : JU
Sample : PB125531 BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 25 12:21:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

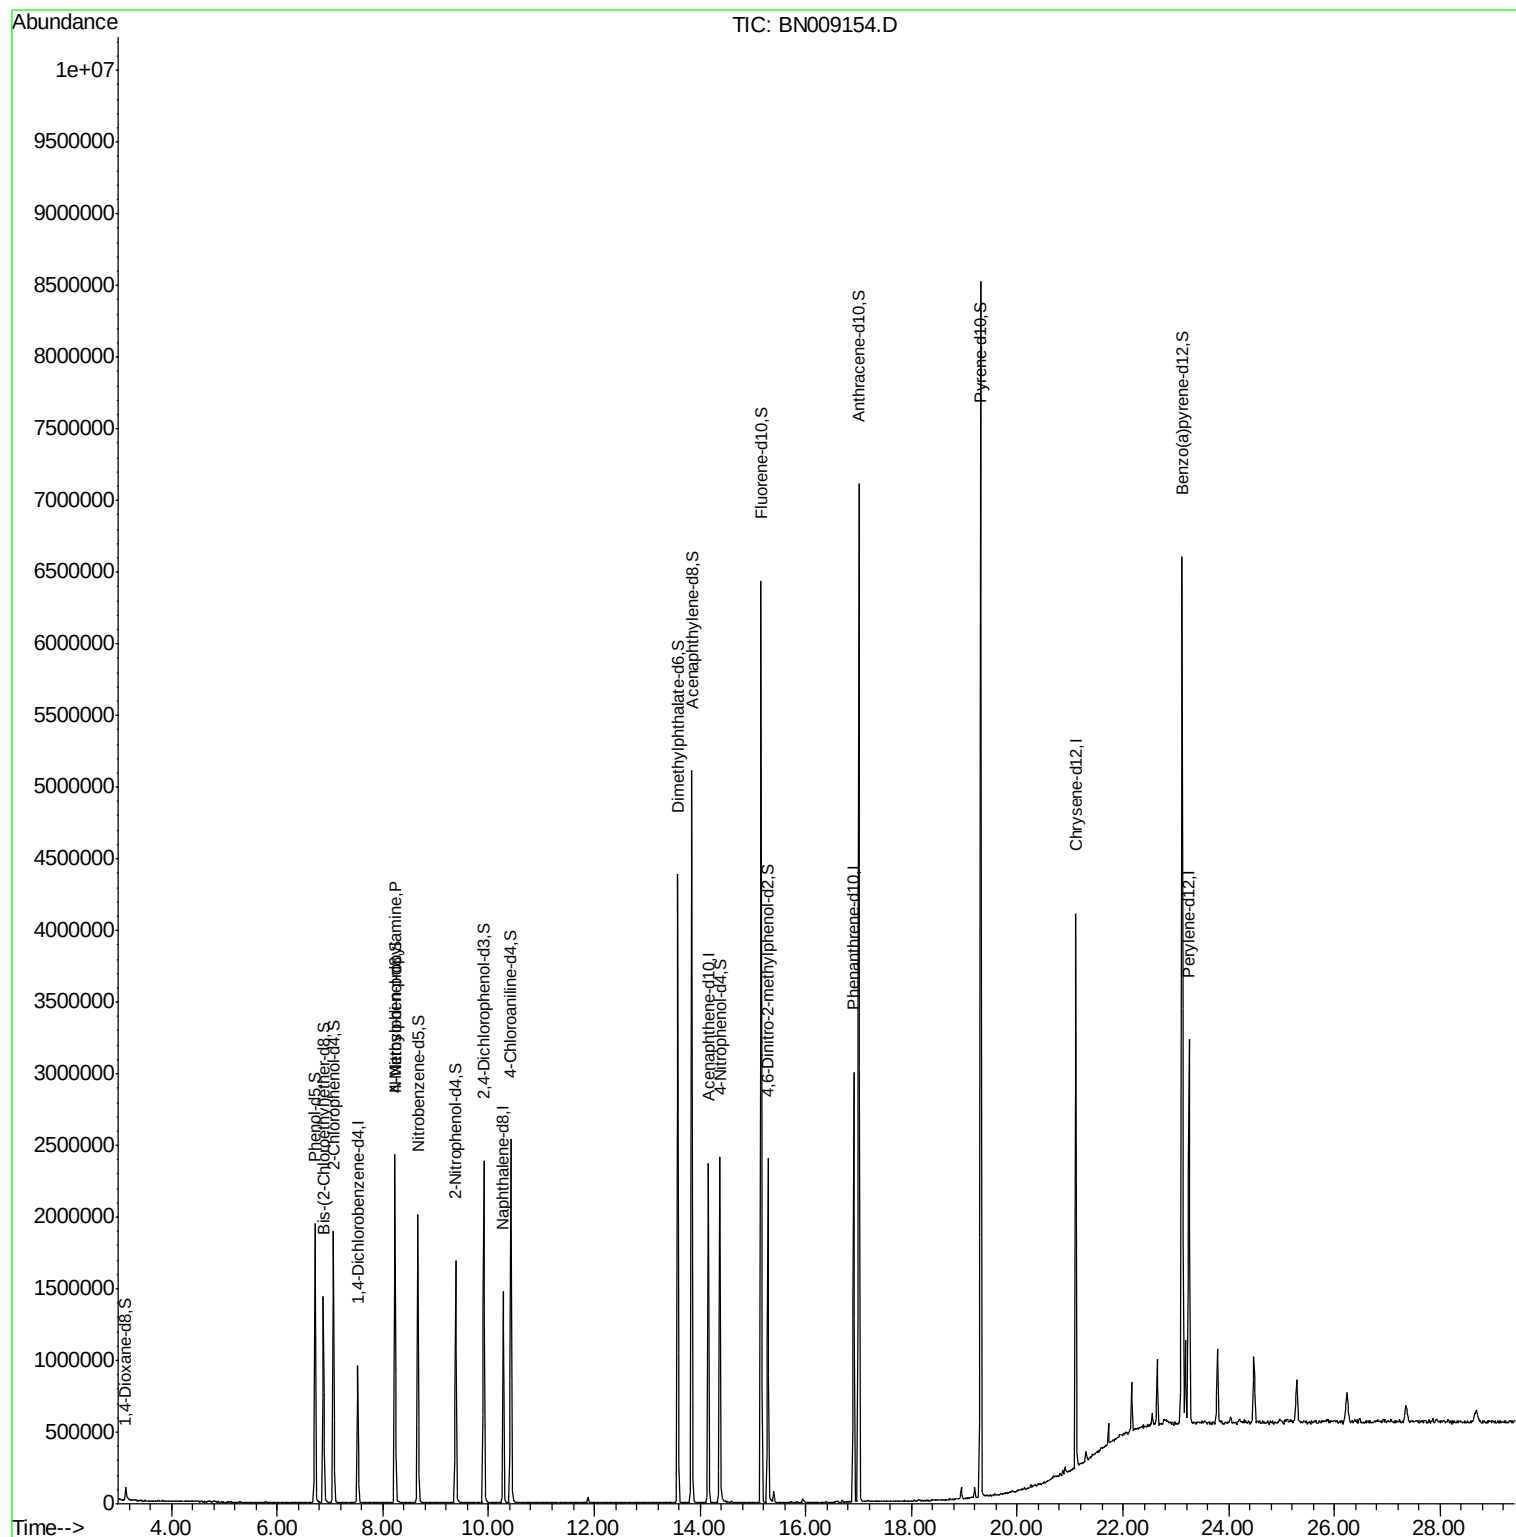

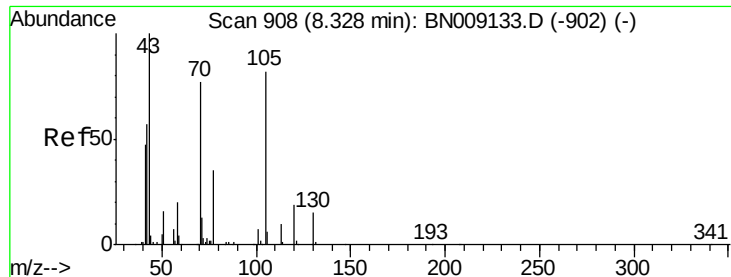

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.435 ng/ul
 RT: 8.23 min Scan# 892
 Delta R.T. -0.09 min
 Lab File: BN009154.D
 Acq: 25 Dec 2019 08:53

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion: 70 Resp: 21587
 Ion Ratio Lower Upper
 70 100
 42 420.5 60.4 90.6#
 101 0.0 7.4 11.0#
 130 0.0 15.8 23.8#

