

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
 Data File : BN009166.D
 Acq On : 25 Dec 2019 16:02
 Operator : JU
 Sample : K6276-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C73

Quant Time: Dec 25 17:30:23 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	261060	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	1238152	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.15	164	850898	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1862292	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1815195	20.00	ng/ul	0.00
85) Perylene-d12	23.25	264	1923786	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	31330	5.48	ng/uL	0.00
5) Phenol-d5	6.72	99	170125	6.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	469485	29.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	435780	24.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	338898	16.91	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	292644	31.38	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	330671	31.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	580883	29.56	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	55228	2.33	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	2224211	34.80	ng/ul	0.00
46) Acenaphthylene-d8	13.85	160	2524954	33.70	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	81168	6.39	ng/ul	0.00
57) Fluorene-d10	15.15	176	1889429	33.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	344233	29.63	ng/ul	0.00
70) Anthracene-d10	17.00	188	3085452	35.62	ng/ul	0.00
78) Pyrene-d10	19.30	212	3464159	36.58	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	3532657	36.44	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.62	163	93146	1.425	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122419\
Data File : BN009166.D
Acq On : 25 Dec 2019 16:02
Operator : JU
Sample : K6276-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C73

Quant Time: Dec 25 17:30:23 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

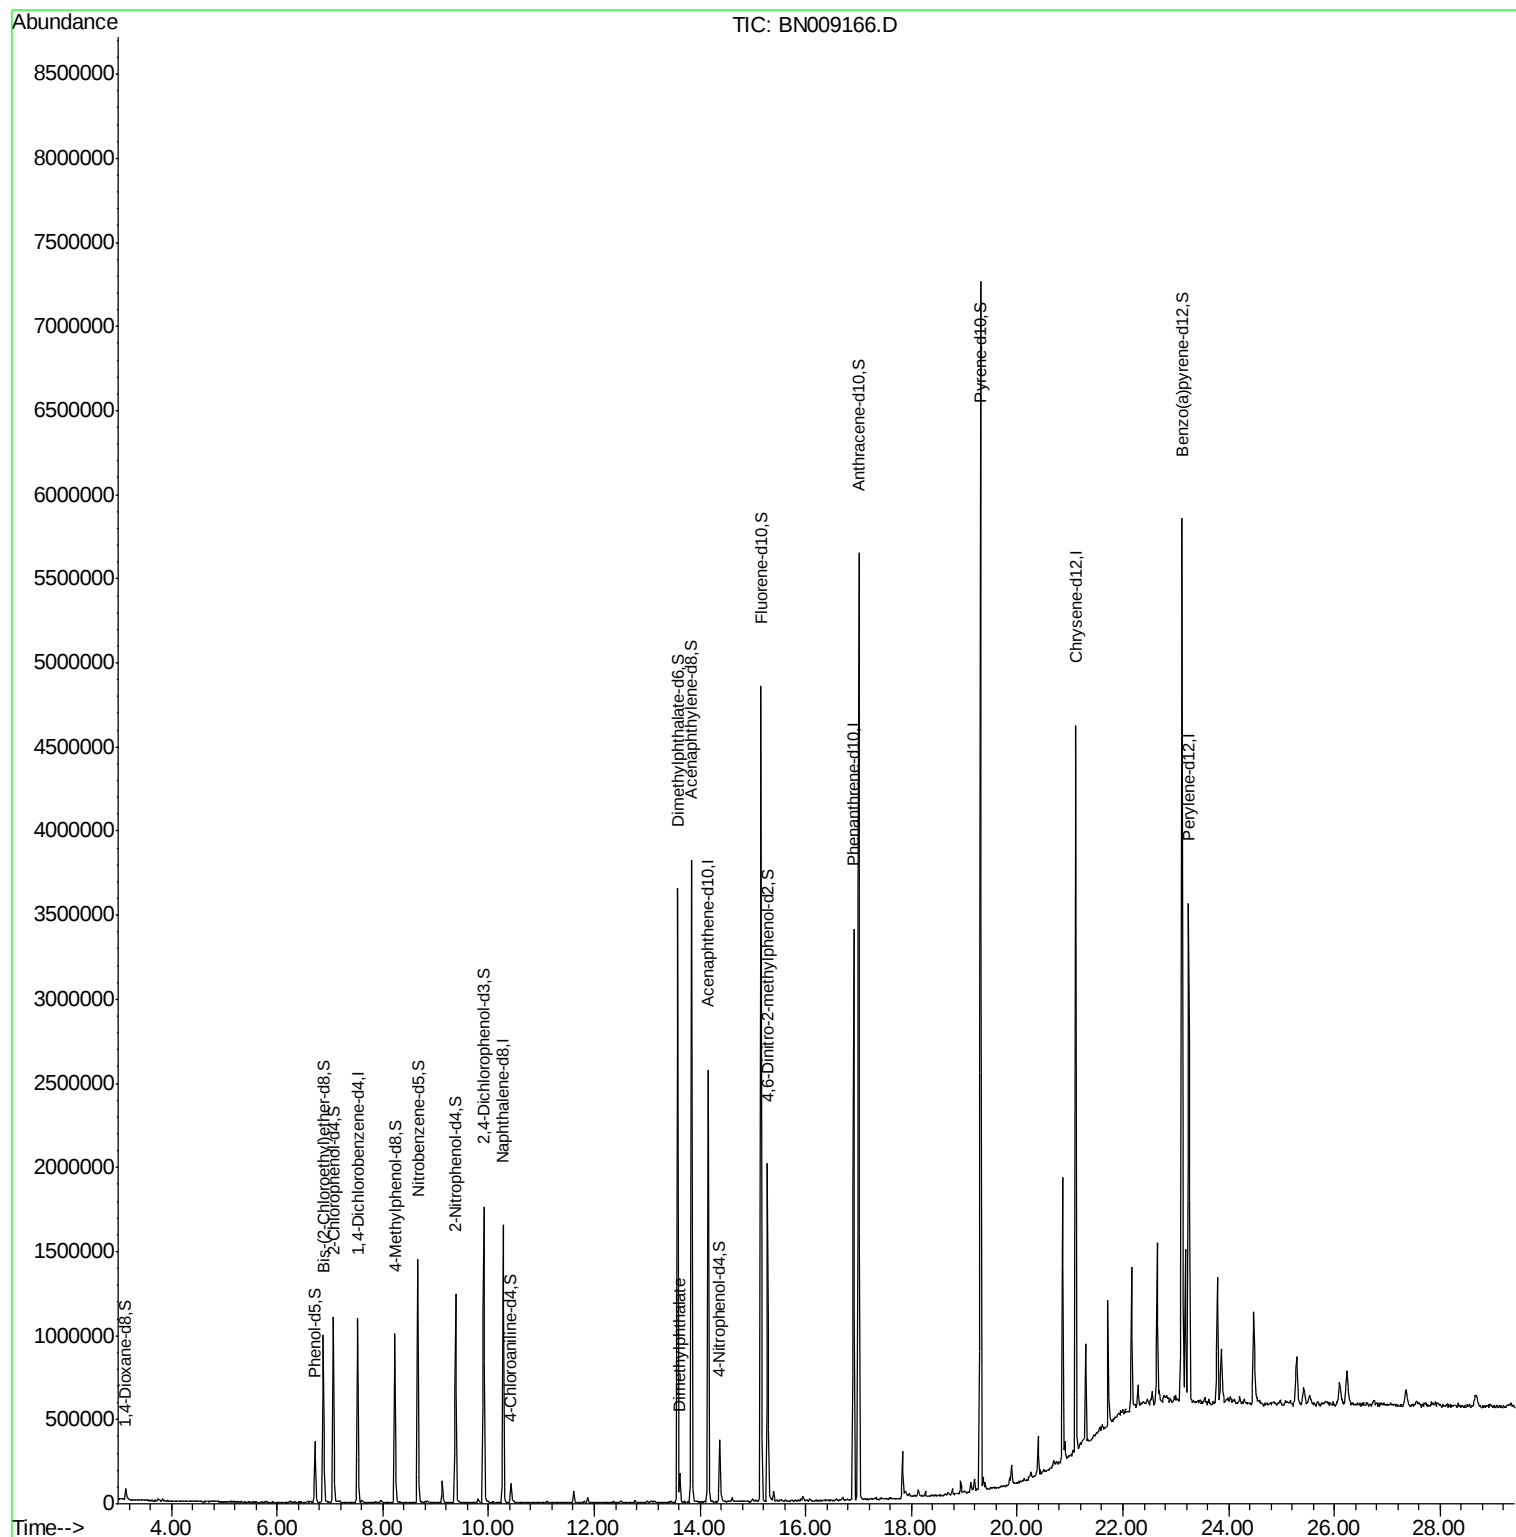

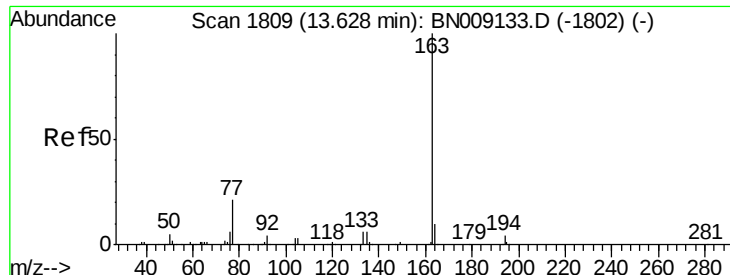

#44

Dimethylphthalate

Concen: 1.425 ng/ul

RT: 13.62 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BN009166.D

Acq: 25 Dec 2019 16:02

Instrument :

BNA_N

ClientSampleId :

C0C73


Tot Ion:163 Resp: 93146

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 9.8 8.3 12.5

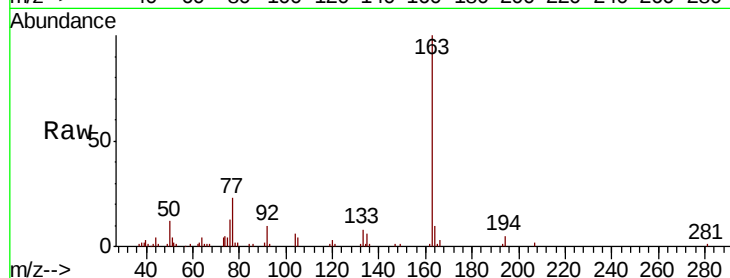

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

