

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
 Data File : BN009143.D
 Acq On : 25 Dec 2019 01:44
 Operator : JU
 Sample : K6257-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFF05

Quant Time: Dec 25 04:40:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	288565	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	1349846	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.16	164	932245	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1958524	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1867967	20.00	ng/ul	0.00
85) Perylene-d12	23.25	264	1997752	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	16283	2.58	ng/uL	0.00
5) Phenol-d5	6.72	99	423102	15.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	293486	16.70	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	319553	16.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	358748	16.20	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	172714	16.99	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	195667	17.24	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	346245	16.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.42	131	477423	18.49	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	1215753	17.36	ng/ul	0.00
46) Acenaphthylene-d8	13.85	160	1439713	17.54	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	192757	13.85	ng/ul	0.00
57) Fluorene-d10	15.16	176	1056124	17.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	155105	12.69	ng/ul	0.00
70) Anthracene-d10	17.00	188	1697389	18.63	ng/ul	0.00
78) Pyrene-d10	19.30	212	2046872	21.00	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	2019473	20.06	ng/ul	0.00


Target Compounds					Ovalue
44) Dimethylphthalate	13.62	163	252938	3.532	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
Data File : BN009143.D
Acq On : 25 Dec 2019 01:44
Operator : JU
Sample : K6257-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BFF05

Quant Time: Dec 25 04:40:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

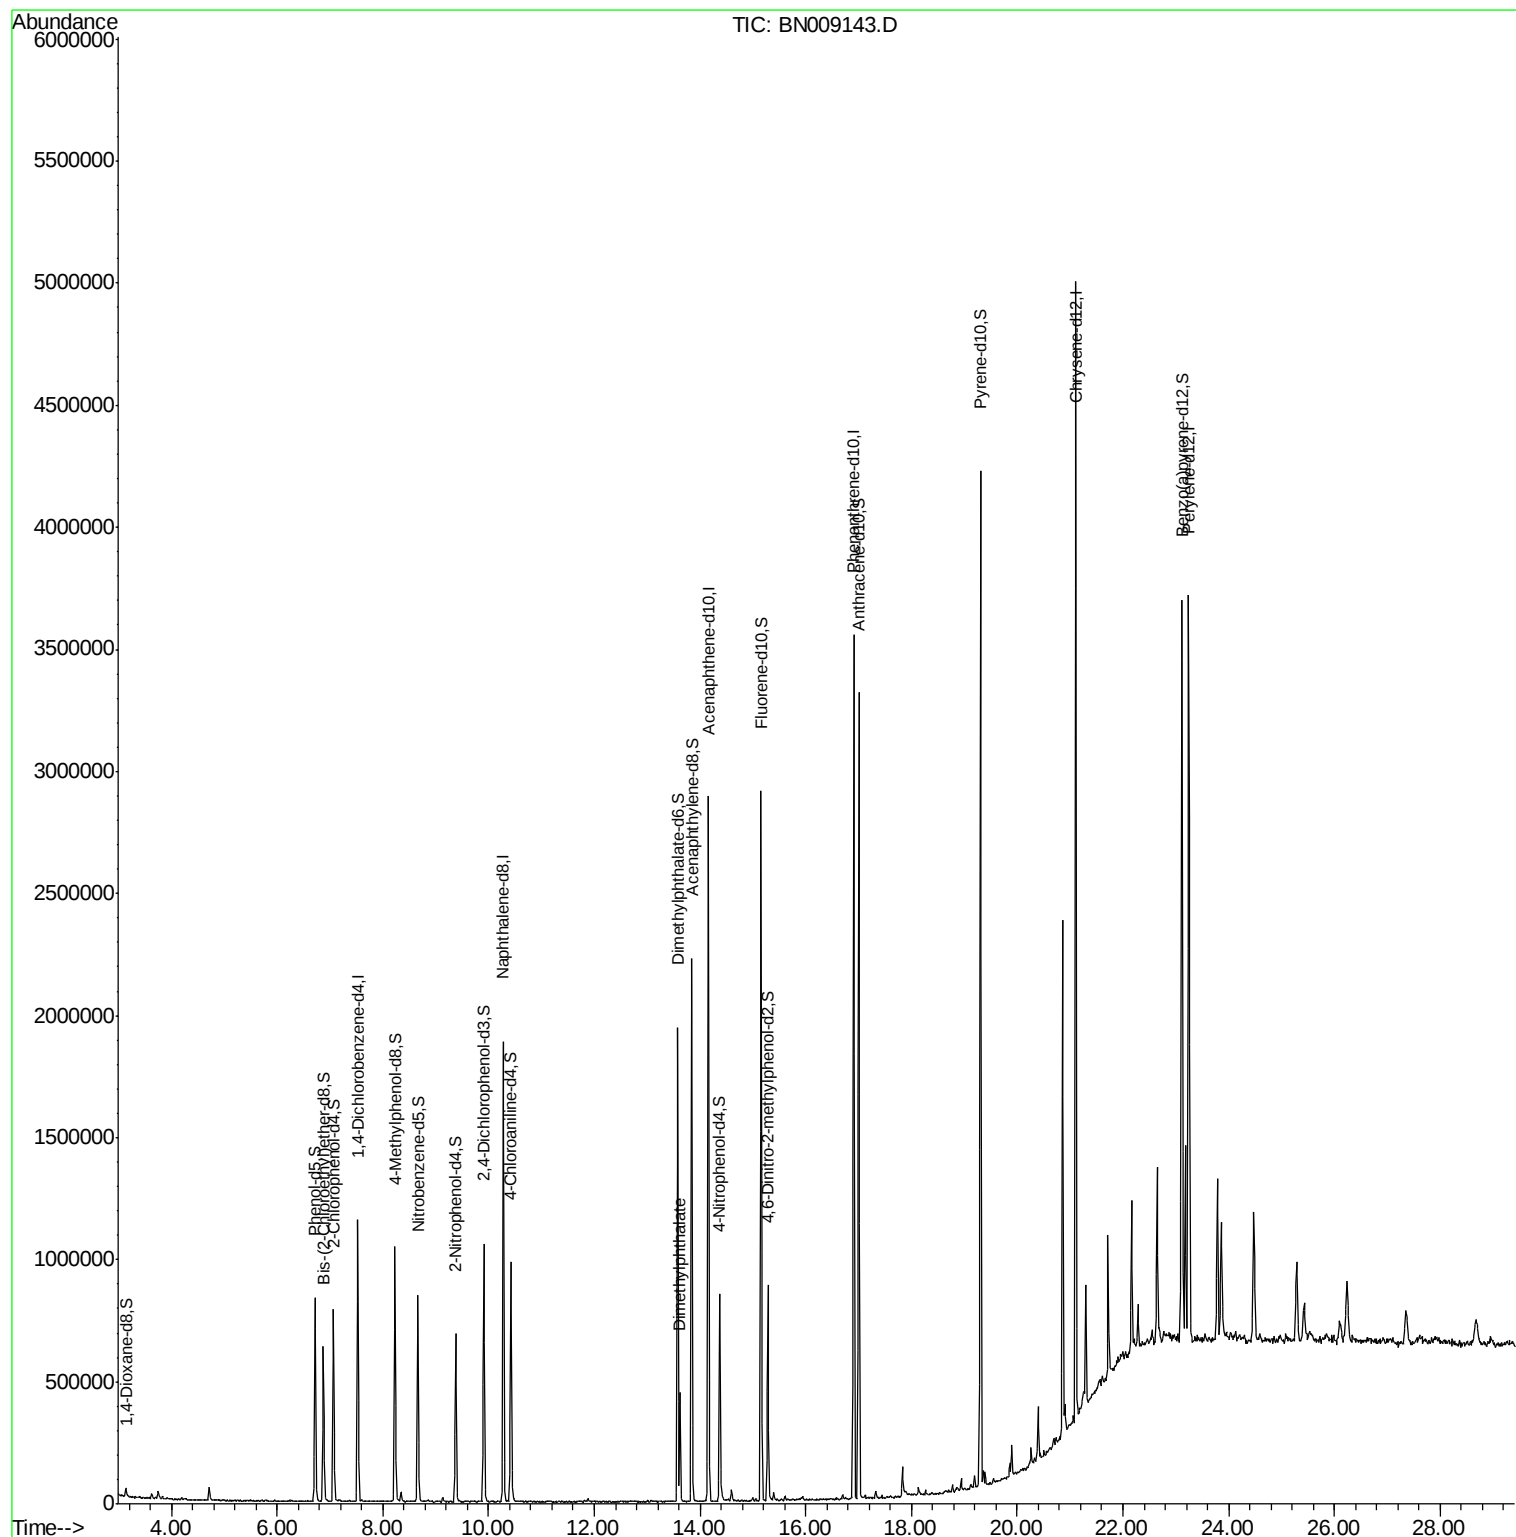

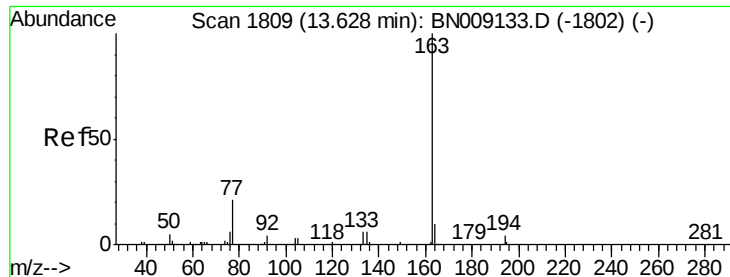

#44

Dimethylphthalate

Concen: 3.532 ng/ul

RT: 13.62 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BN009143.D

Acq: 25 Dec 2019 01:44

Instrument :

BNA_N

ClientSampleId :

BFF05



Tot Ion:163 Resp: 252938

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.4 8.3 12.5

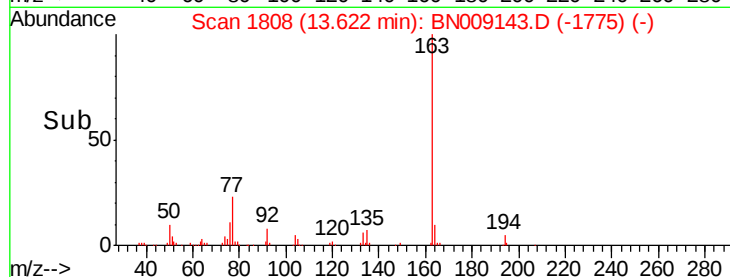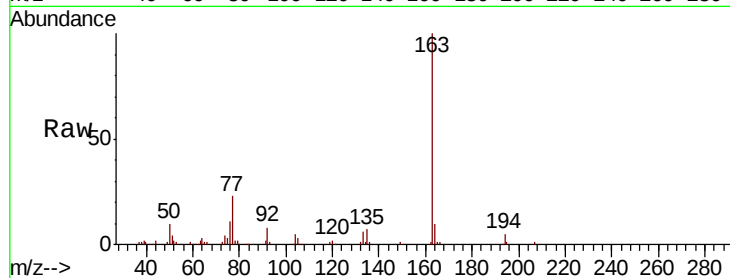

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

