

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
 Data File : BN009163.D
 Acq On : 25 Dec 2019 14:15
 Operator : JU
 Sample : K6276-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0C38

Quant Time: Dec 25 15:28:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 01:06:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	266306	20.00	ng/ul	0.00
18) Naphthalene-d8	10.28	136	1236619	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.16	164	851013	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.90	188	1890974	20.00	ng/ul	0.00
77) Chrysene-d12	21.11	240	1782759	20.00	ng/ul	0.00
85) Perylene-d12	23.25	264	1869944	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.13	96	32667	5.60	ng/uL	0.00
5) Phenol-d5	6.72	99	141037	5.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.88	67	416218	25.66	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	387289	21.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.23	113	281582	13.78	ng/ul	0.00
19) Nitrobenzene-d5	8.66	128	256959	27.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.38	143	286220	27.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.91	165	502641	25.61	ng/ul	0.00
29) 4-Chloroaniline-d4	10.43	131	40851	1.73	ng/ul	0.00
43) Dimethylphthalate-d6	13.57	166	1931625	30.22	ng/ul	0.00
46) Acenaphthylene-d8	13.84	160	2218382	29.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.37	143	72193	5.68	ng/ul	0.00
57) Fluorene-d10	15.15	176	1728579	31.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.29	200	324810	27.53	ng/ul	0.00
70) Anthracene-d10	17.00	188	2913921	33.13	ng/ul	0.00
78) Pyrene-d10	19.30	212	3382137	36.36	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.12	264	3320390	35.24	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.62	163	99195	1.518	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122419\
Data File : BN009163.D
Acq On : 25 Dec 2019 14:15
Operator : JU
Sample : K6276-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0C38

Quant Time: Dec 25 15:28:53 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN122419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 01:06:45 2019
Response via : Initial Calibration

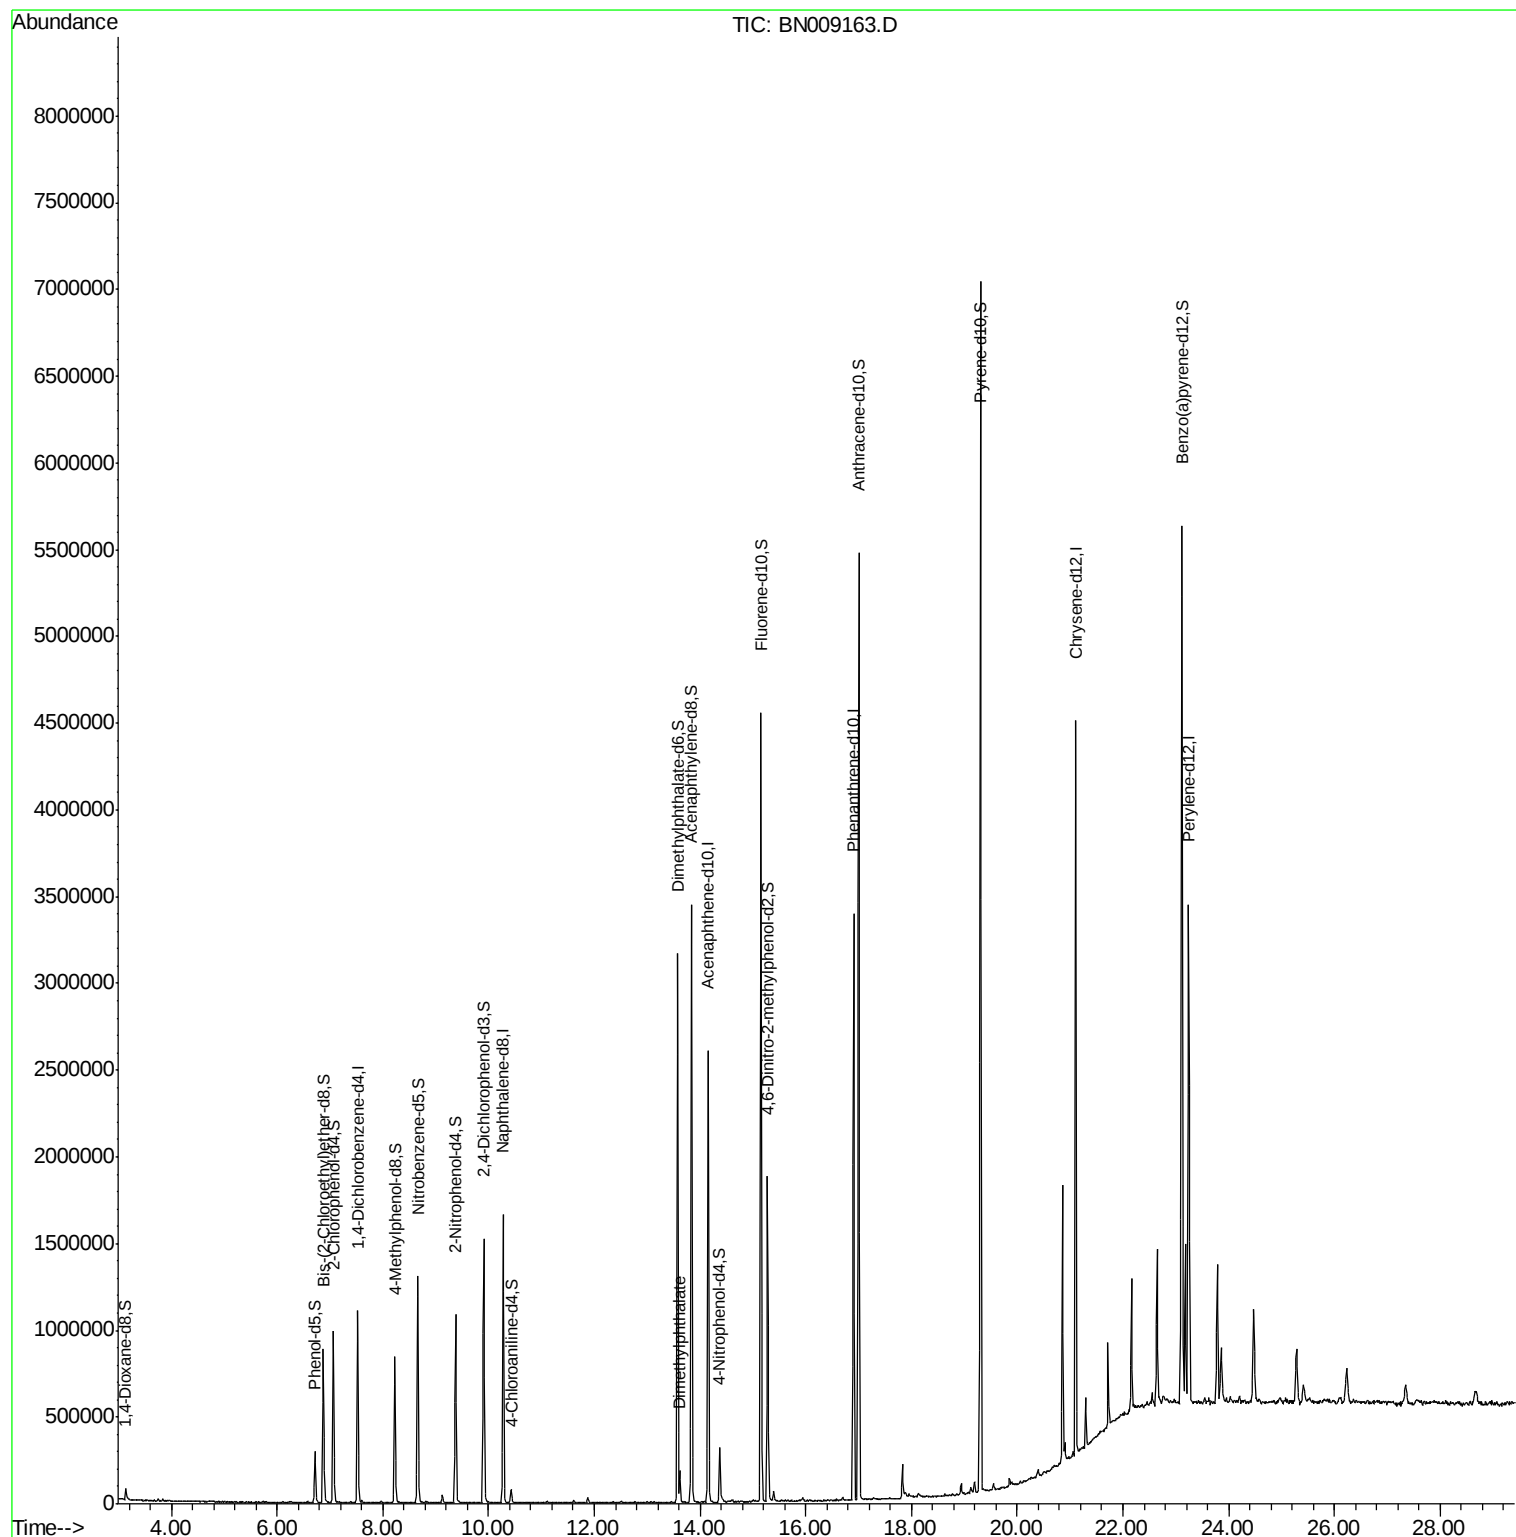

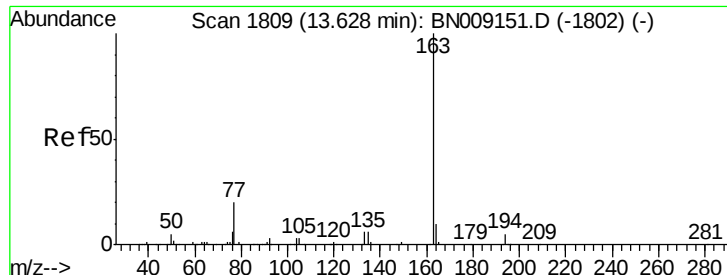

#44

Dimethylphthalate

Concen: 1.518 ng/ul

RT: 13.62 min Scan# 1808

Delta R.T. -0.01 min

Lab File: BN009163.D

Acq: 25 Dec 2019 14:15

Instrument :

BNA_N

ClientSampleId :

C0C38


Tot Ion:163 Resp: 99195

Ion Ratio Lower Upper

163 100

194 4.9 3.5 5.3

164 12.1 8.3 12.5

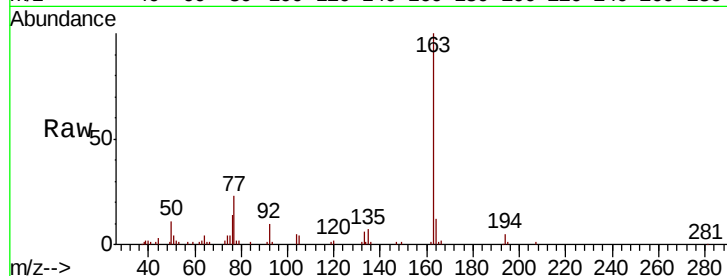

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

