

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023377.D
 Acq On : 23 Dec 2022 18:26
 Operator : CG/JU
 Sample : PB149762BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK762

Quant Time: Dec 23 22:44:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.994	152	6012	0.400	ng/ul	0.00
4) Naphthalene-d8	10.810	136	19792	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.645	164	11966	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.390	188	28068	0.400	ng/ul	0.00
17) Chrysene-d12	21.581	240	19299	0.400	ng/ul	0.00
23) Perylene-d12	24.030	264	15001	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	38612	5.911	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.399	152	9802	0.320	ng/ul	0.00
18) Fluoranthene-d10	19.420	212	23501	0.337	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.640	166	3364	0.067	ng/ul#	13
20) Pyrene	19.787	202	3199	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.875	252	5117	0.083	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023377.D
Acq On : 23 Dec 2022 18:26
Operator : CG/JU
Sample : PB149762BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK762

Quant Time: Dec 23 22:44:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration




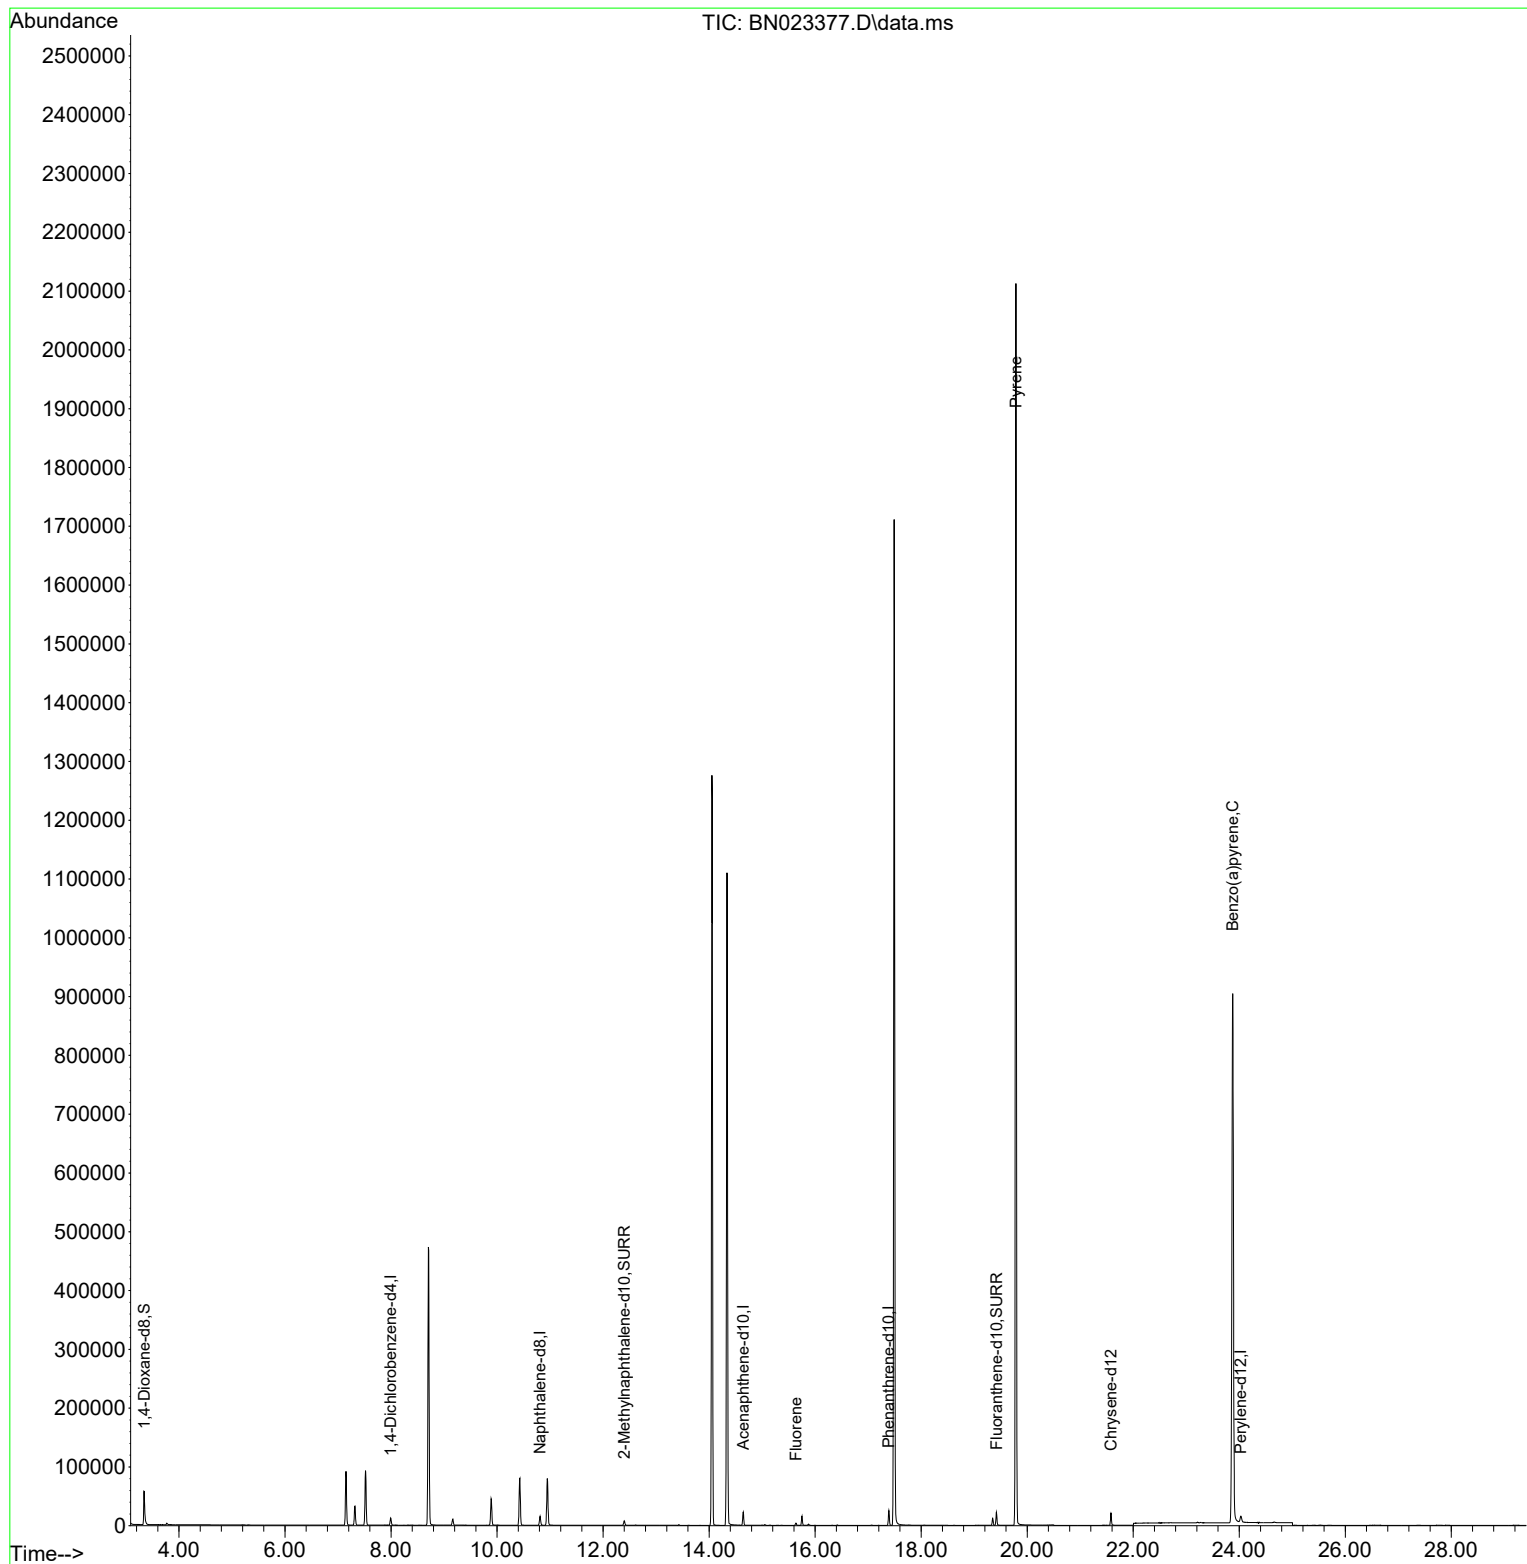


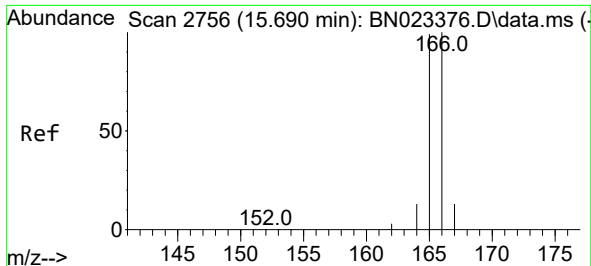

#12
Fluorene
Concen: 0.067 ng/ul
RT: 15.640 min Scan# 21
Delta R.T. -0.052 min
Lab File: BN023377.D
Acq: 23 Dec 2022 18:26




Instrument :
BNA_N
ClientSampleId :
SBLK762


Tgt Ion:166 Resp: 3364
Ion Ratio Lower Upper
166 100
165 7.7 79.1 118.7#
167 35.9 11.0 16.4#

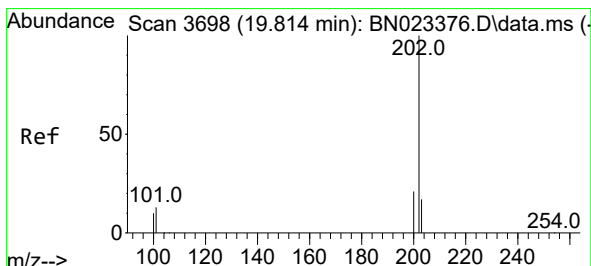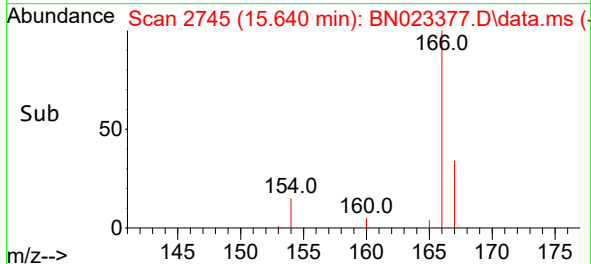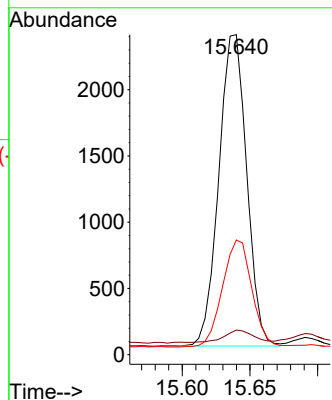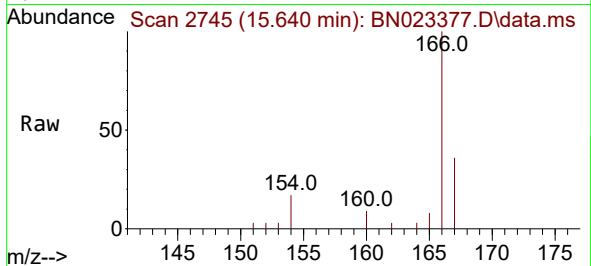

#20
Pyrene
Concen: 0.034 ng/ul
RT: 19.787 min Scan# 3692
Delta R.T. -0.024 min
Lab File: BN023377.D
Acq: 23 Dec 2022 18:26


Tgt Ion:202 Resp: 3199
Ion Ratio Lower Upper
202 100
101 161.2 11.3 16.9#
100 1187.2 9.0 13.4#

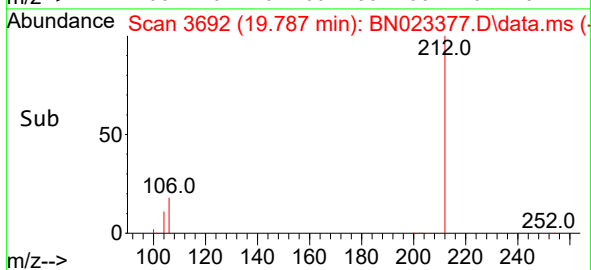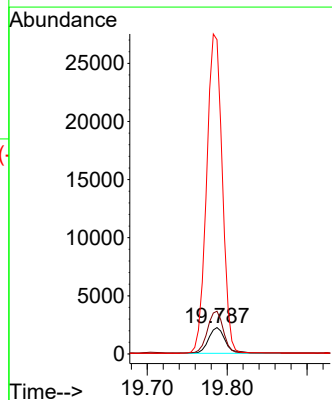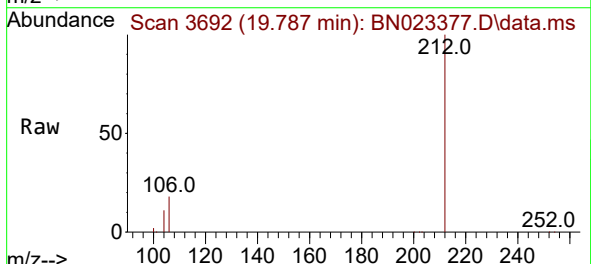

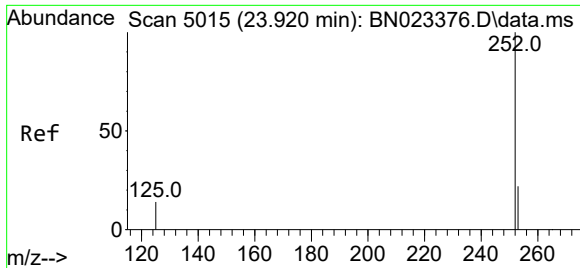

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.875 min Scan# 5015
Delta R.T. -0.039 min
Lab File: BN023377.D
Acq: 23 Dec 2022 18:26

Instrument :
BNA_N
ClientSampleId :
SBLK762

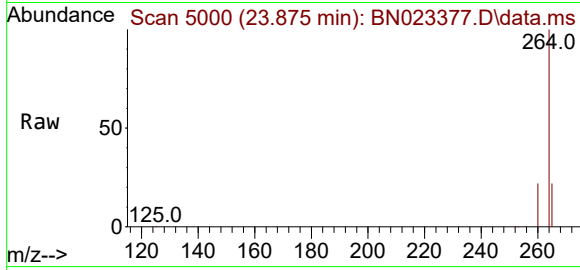

Tgt Ion:252 Resp: 5117
Ion Ratio Lower Upper
252 100
253 46.8 21.4 32.2#
125 43.2 16.2 24.4#

