

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023380.D
 Acq On : 23 Dec 2022 20:16
 Operator : CG/JU
 Sample : N6008-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBYB3

Quant Time: Dec 23 22:44:58 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 22 02:28:40 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.994	152	6394	0.400	ng/ul	0.00
4) Naphthalene-d8	10.808	136	21145	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.644	164	12507	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.389	188	30108	0.400	ng/ul	0.00
17) Chrysene-d12	21.578	240	23009	0.400	ng/ul	0.00
23) Perylene-d12	24.028	264	18205	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.344	96	34711	4.996	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.398	152	9544	0.292	ng/ul	0.00
18) Fluoranthene-d10	19.419	212	25160	0.302	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.858	128	1920	0.031	ng/ul#	88
7) 2-Methylnaphthalene	12.469	142	1152	0.029	ng/ul	99
8) 1-Methylnaphthalene	12.689	142	1022	0.025	ng/ul	98
10) Acenaphthylene	14.362	152	2084	0.038	ng/ul#	85
15) Phenanthrene	17.431	178	19507	0.199	ng/ul	98
16) Anthracene	17.524	178	3583	0.044	ng/ul#	90
19) Fluoranthene	19.447	202	51741	0.464	ng/ul	98
20) Pyrene	19.814	202	43744	0.389	ng/ul	99
21) Benzo(a)anthracene	21.561	228	24169	0.270	ng/ul	97
22) Chrysene	21.616	228	28402	0.312	ng/ul	98
24) Benzo(b)fluoranthene	23.276	252	52371	0.556	ng/ul	90
26) Benzo(a)pyrene	23.920	252	21649	0.290	ng/ul#	93
27) Indeno(1,2,3-cd)pyrene	26.584	276	16411	0.189	ng/ul#	88
28) Dibenzo(a,h)anthracene	26.594	278	4123	0.061	ng/ul#	54
29) Benzo(g,h,i)perylene	27.376	276	15710	0.221	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023380.D
Acq On : 23 Dec 2022 20:16
Operator : CG/JU
Sample : N6008-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBYB3

Quant Time: Dec 23 22:44:58 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 22 02:28:40 2022
Response via : Initial Calibration




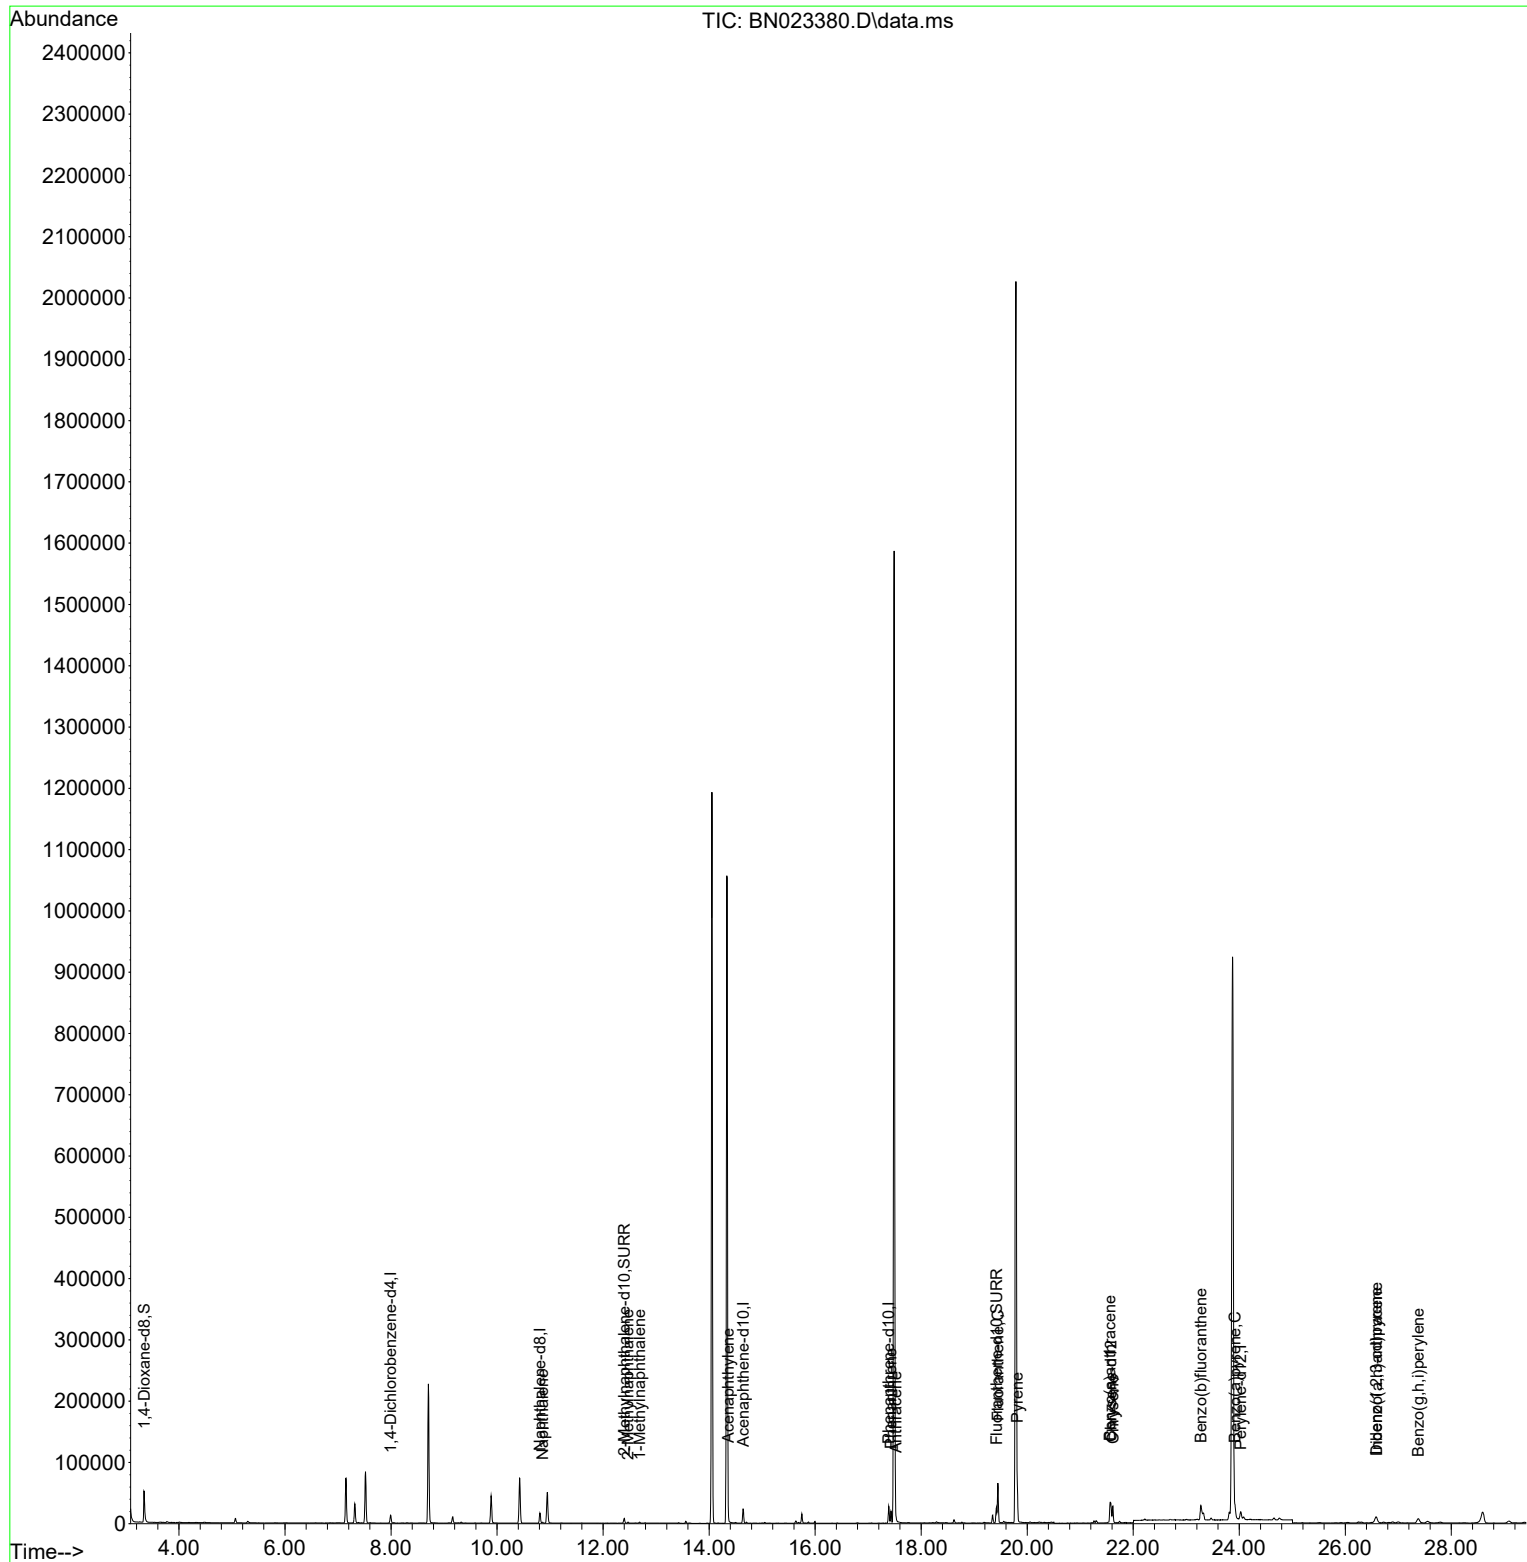


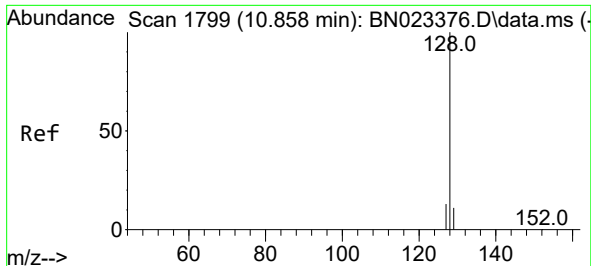

#5
Naphthalene
Concen: 0.031 ng/ul
RT: 10.858 min Scan# 1799
Delta R.T. -0.007 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16




Instrument :
BNA_N
ClientSampleId :
DBYB3


Tgt Ion:128 Resp: 1920
Ion Ratio Lower Upper
128 100
129 17.0 9.0 13.4#
127 16.8 10.7 16.1#

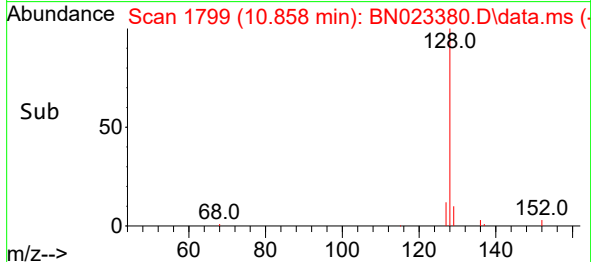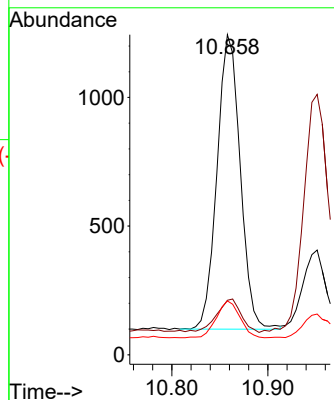

#7
2-Methylnaphthalene
Concen: 0.029 ng/ul
RT: 12.469 min Scan# 2092
Delta R.T. -0.007 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16

Tgt Ion:142 Resp: 1152
Ion Ratio Lower Upper
142 100
141 90.0 71.4 107.2


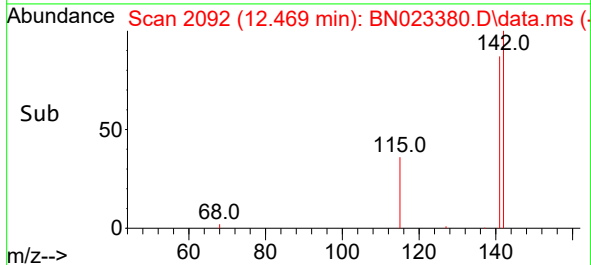
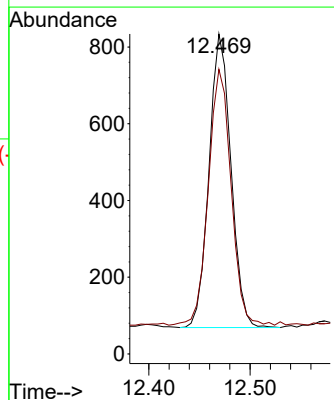
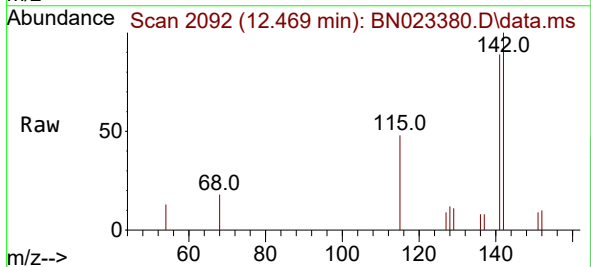


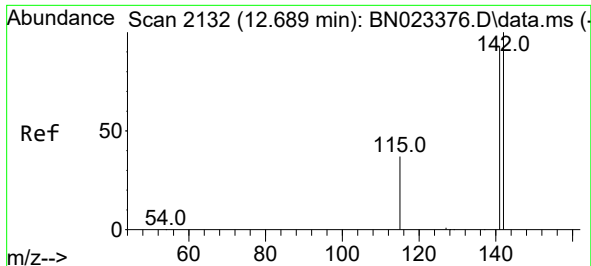

#8
1-Methylnaphthalene
Concen: 0.025 ng/ul
RT: 12.689 min Scan# 2132
Delta R.T. -0.007 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16




Instrument :
BNA_N
ClientSampleId :
DBYB3


Tgt Ion:142 Resp: 1022
Ion Ratio Lower Upper
142 100
141 94.1 74.0 111.0

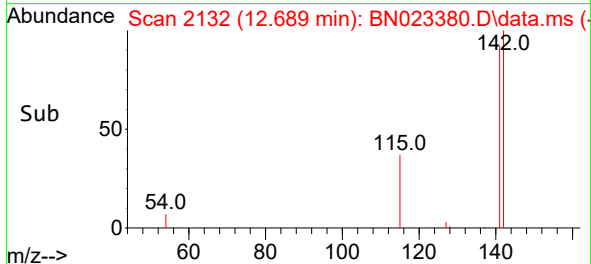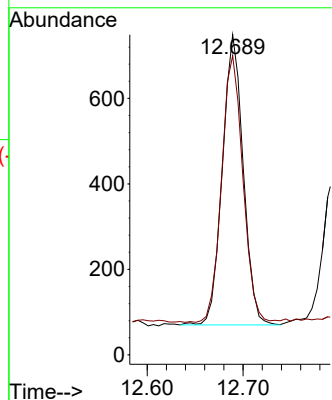

#10
Acenaphthylene
Concen: 0.038 ng/ul
RT: 14.362 min Scan# 2469
Delta R.T. -0.007 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16

Tgt Ion:152 Resp: 2084
Ion Ratio Lower Upper
152 100
151 25.3 16.1 24.1#
153 21.4 10.9 16.3#


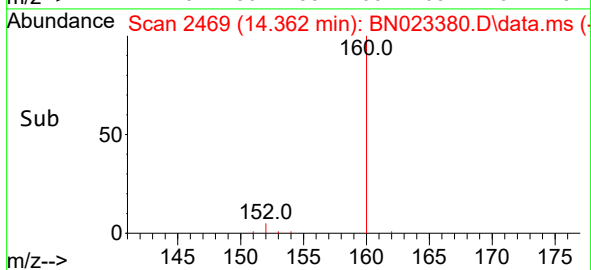
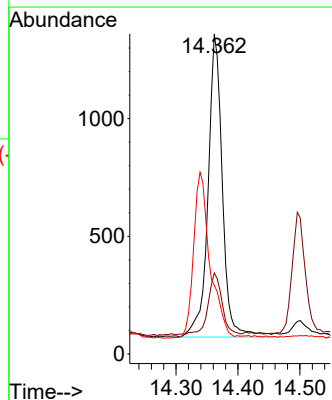
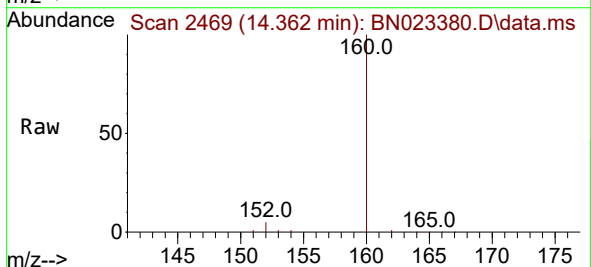


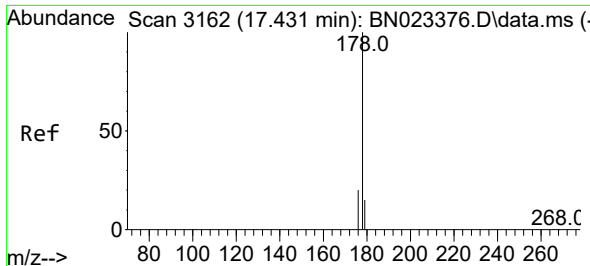

#15
Phenanthrene
Concen: 0.199 ng/ul
RT: 17.431 min Scan# 3162
Delta R.T. -0.002 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16




Instrument :
BNA_N
ClientSampleId :
DBYB3


Tgt Ion:178 Resp: 19507
Ion Ratio Lower Upper
178 100
179 16.7 12.5 18.7
176 19.9 15.7 23.5

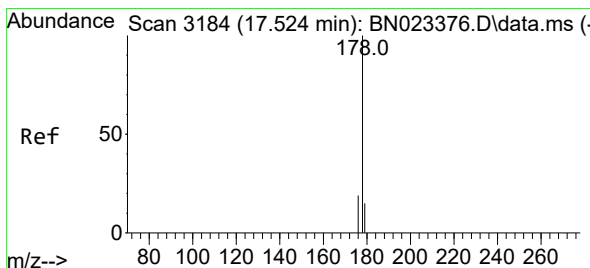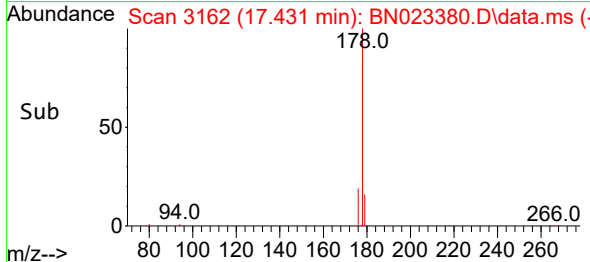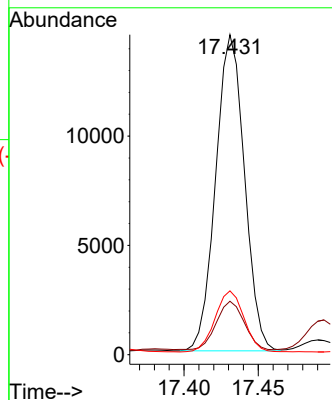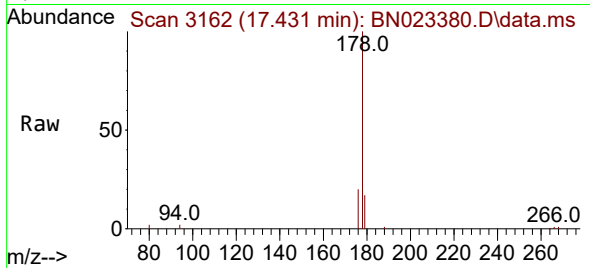

#16
Anthracene
Concen: 0.044 ng/ul
RT: 17.524 min Scan# 3184
Delta R.T. -0.002 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16

Tgt Ion:178 Resp: 3583
Ion Ratio Lower Upper
178 100
179 21.2 12.6 18.8#
176 22.2 15.4 23.0


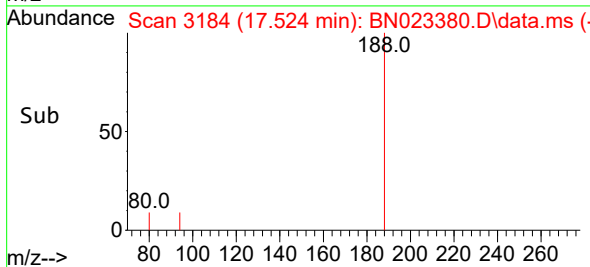
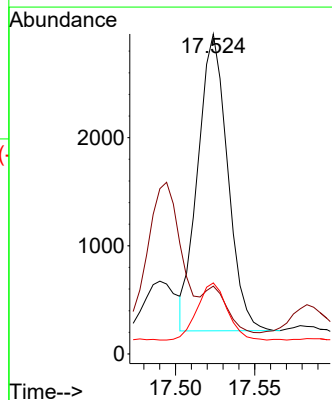
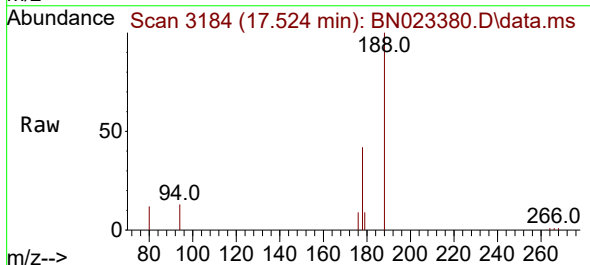


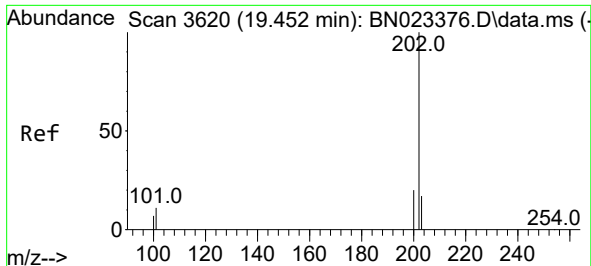

#19
Fluoranthene
Concen: 0.464 ng/ul
RT: 19.447 min Scan# 3619
Delta R.T. -0.002 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16




Instrument :
BNA_N
ClientSampleId :
DBYB3


Tgt Ion:202 Resp: 51741
Ion Ratio Lower Upper
202 100
101 12.8 9.4 14.2
100 9.5 7.0 10.6

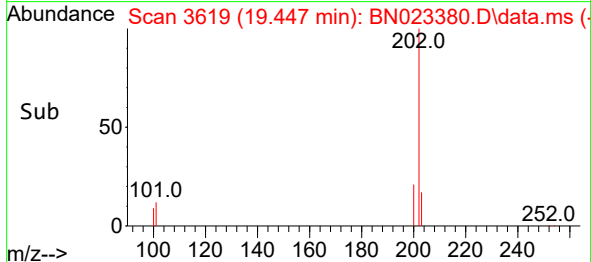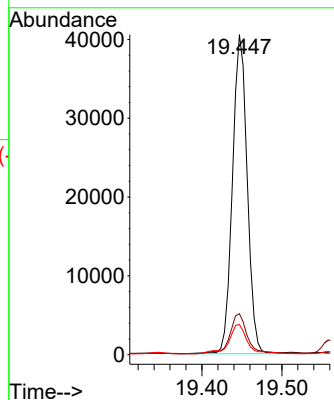

#20
Pyrene
Concen: 0.389 ng/ul
RT: 19.814 min Scan# 3698
Delta R.T. 0.003 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16

Tgt Ion:202 Resp: 43744
Ion Ratio Lower Upper
202 100
101 13.6 11.3 16.9
100 10.8 9.0 13.4


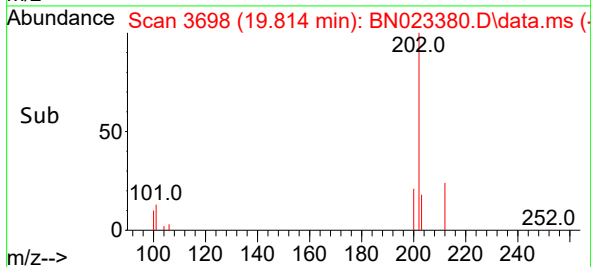
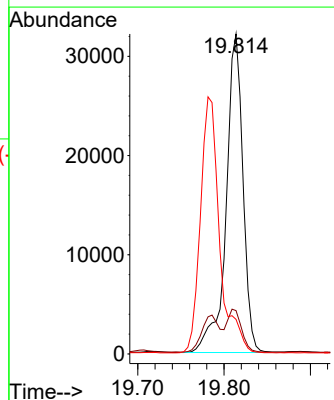
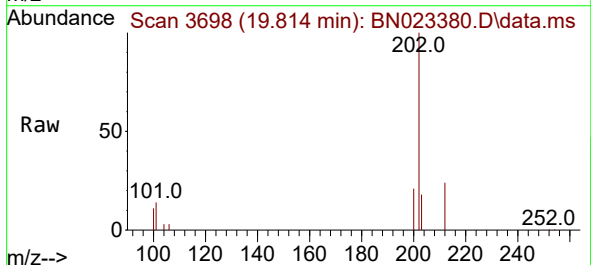


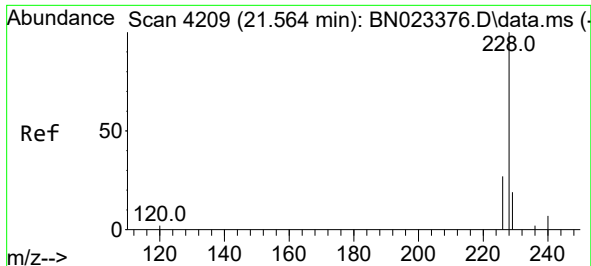

#21
Benzo(a)anthracene
Concen: 0.270 ng/ul
RT: 21.561 min Scan# 4209
Delta R.T. -0.000 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16




Instrument :
BNA_N
ClientSampleId :
DBYB3


Tgt Ion:228 Resp: 24169
Ion Ratio Lower Upper
228 100
229 20.9 15.6 23.4
226 28.8 22.2 33.2

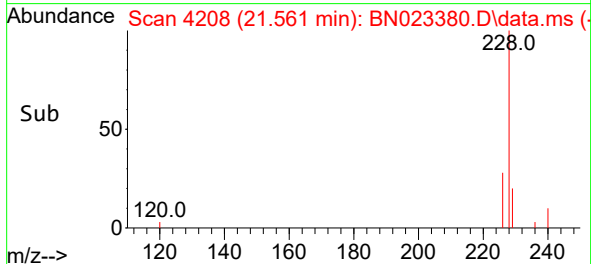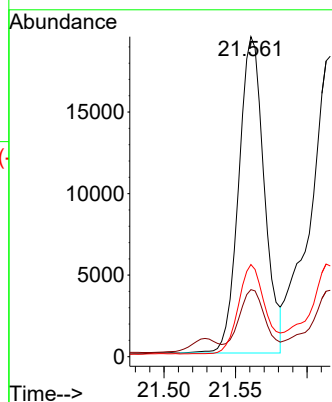

#22
Chrysene
Concen: 0.312 ng/ul
RT: 21.616 min Scan# 4227
Delta R.T. -0.000 min
Lab File: BN023380.D
Acq: 23 Dec 2022 20:16

Tgt Ion:228 Resp: 28402
Ion Ratio Lower Upper
228 100
226 30.2 24.3 36.5
229 22.1 15.8 23.6

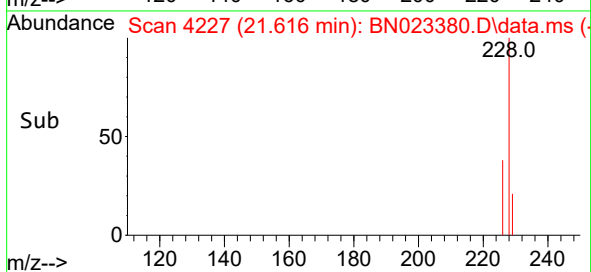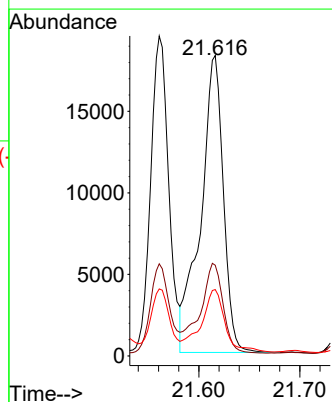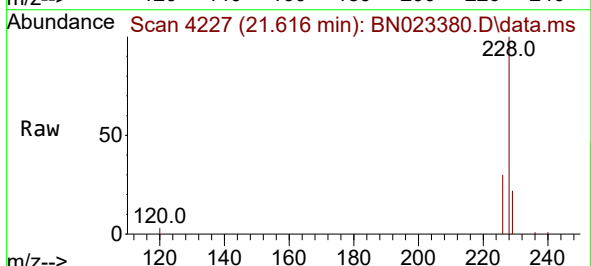



#24

Benzo(b)fluoranthene

Concen: 0.556 ng/ul

RT: 23.276 min Scan# 4795

Delta R.T. 0.003 min

Lab File: BN023380.D

Acq: 23 Dec 2022 20:16

Instrument :

BNA_N

ClientSampleId :

DBYB3





Tgt Ion:252 Resp: 52371

Ion Ratio Lower Upper

252 100

253 27.0 0.0 49.2

125 23.4 0.0 31.8

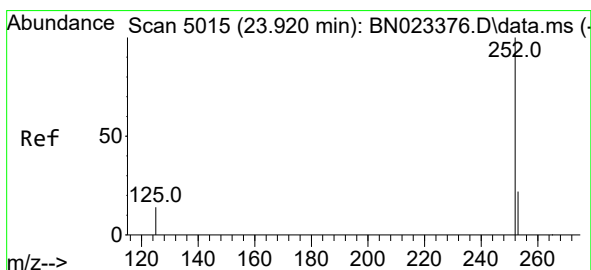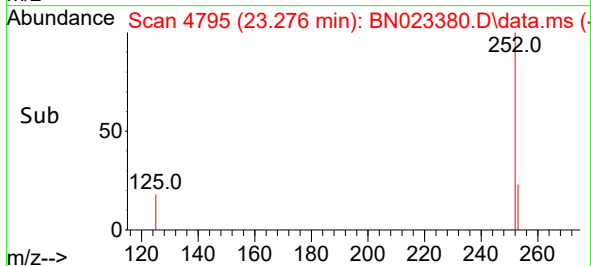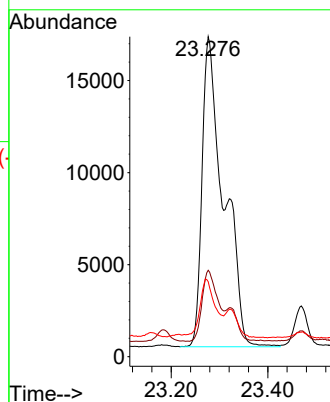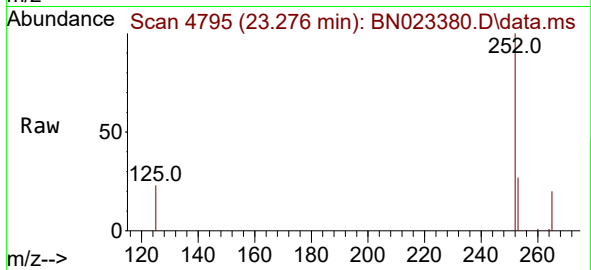

#26

Benzo(a)pyrene

Concen: 0.290 ng/ul

RT: 23.920 min Scan# 5015

Delta R.T. 0.005 min

Lab File: BN023380.D

Acq: 23 Dec 2022 20:16




Tgt Ion:252 Resp: 21649


Ion Ratio Lower Upper

252 100

253 28.3 21.4 32.2

125 26.4 16.2 24.4#

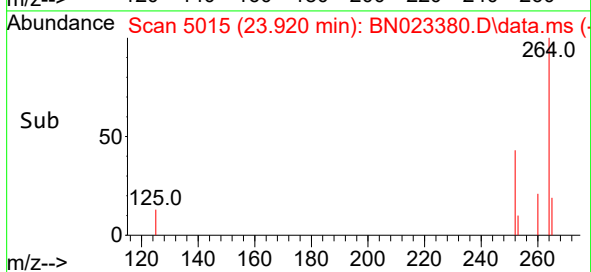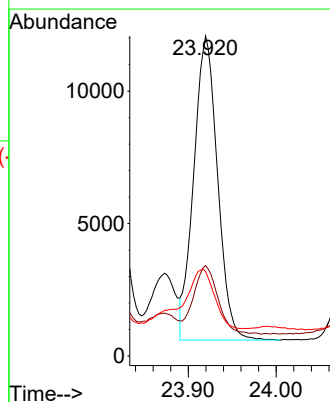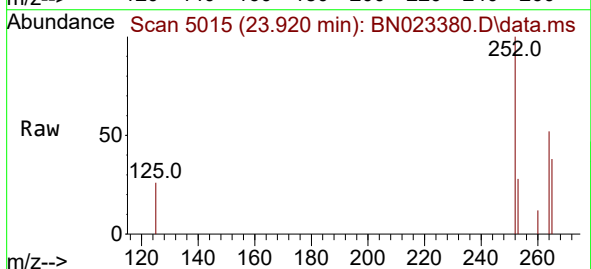

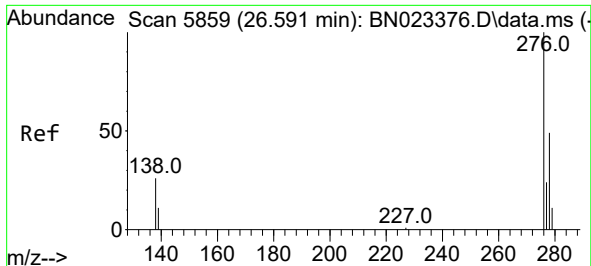

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.189 ng/ul

RT: 26.584 min Scan# 5857

Delta R.T. 0.006 min

Lab File: BN023380.D

Acq: 23 Dec 2022 20:16

Instrument :

BNA_N

ClientSampleId :

DBYB3





Tgt Ion:276 Resp: 16411

Ion Ratio Lower Upper

276 100

138 35.6 23.4 35.2#

227 0.0 0.0 0.0

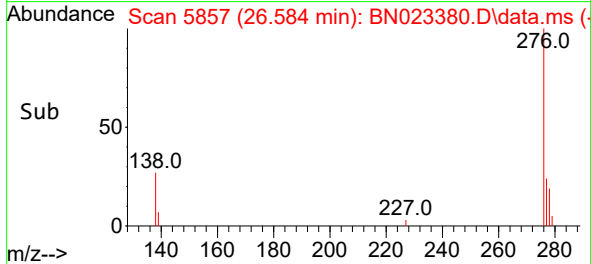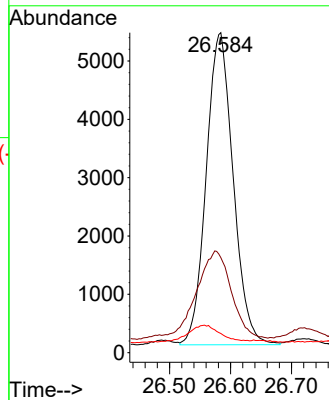

#28

Dibenzo(a,h)anthracene

Concen: 0.061 ng/ul

RT: 26.594 min Scan# 5860

Delta R.T. -0.007 min

Lab File: BN023380.D

Acq: 23 Dec 2022 20:16




Tgt Ion:278 Resp: 4123


Ion Ratio Lower Upper

278 100

139 45.7 16.6 24.8#


279 47.2 21.3 31.9#

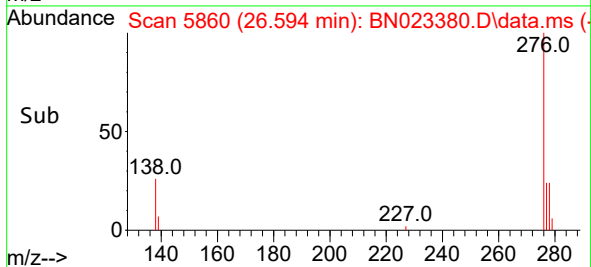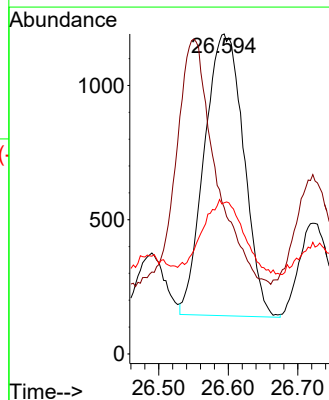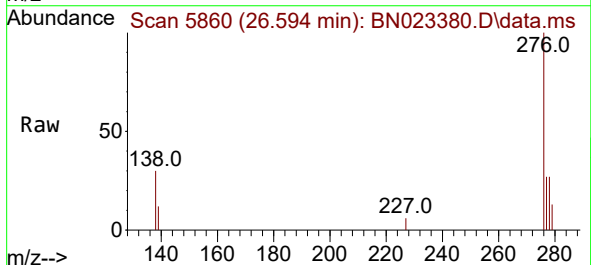

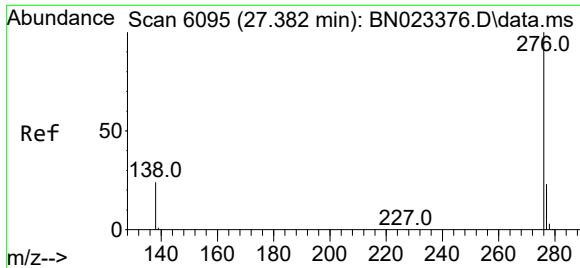

#29
 Benzo(g,h,i)perylene
 Concen: 0.221 ng/ul
 RT: 27.376 min Scan# 6093
 Delta R.T. 0.006 min
 Lab File: BN023380.D
 Acq: 23 Dec 2022 20:16

Instrument :
 BNA_N
 ClientSampleId :
 DBYB3

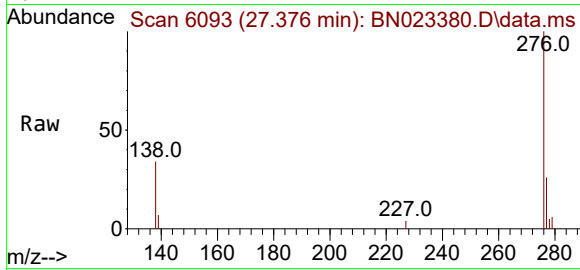

Tgt Ion: 276 Resp: 15710

Ion	Ratio	Lower	Upper
276	100		
138	33.5	20.3	30.5#
277	26.0	19.7	29.5

