

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023440.D
 Acq On : 25 Dec 2022 09:22
 Operator : CG/JU
 Sample : N6017-13
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 01:22:37 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	7017	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	22808	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	13603	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	30946	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240	22287	0.400	ng/ul	0.00
23) Perylene-d12	24.022	264	16610	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	27624	3.623	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.394	152	9551	0.271	ng/ul	0.00
18) Fluoranthene-d10	19.416	212	23135	0.287	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.854	128	3148	0.047	ng/ul#	92
7) 2-Methylnaphthalene	12.465	142	933	0.022	ng/ul	98
10) Acenaphthylene	14.358	152	2180	0.036	ng/ul#	88
15) Phenanthrene	17.428	178	12833	0.127	ng/ul#	89
16) Anthracene	17.517	178	2377	0.028	ng/ul#	77
19) Fluoranthene	19.443	202	36270	0.335	ng/ul#	92
20) Pyrene	19.811	202	29899	0.274	ng/ul	99
21) Benzo(a)anthracene	21.557	228	16970	0.196	ng/ul	95
22) Chrysene	21.610	228	19719	0.223	ng/ul#	94
24) Benzo(b)fluoranthene	23.273	252	38156	0.444	ng/ul	87
26) Benzo(a)pyrene	23.913	252	17424	0.256	ng/ul#	91
27) Indeno(1,2,3-cd)pyrene	26.574	276	14315	0.180	ng/ul#	74
28) Dibenzo(a,h)anthracene	26.590	278	3599	0.058	ng/ul#	40
29) Benzo(g,h,i)perylene	27.365	276	14472	0.224	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023440.D
Acq On : 25 Dec 2022 09:22
Operator : CG/JU
Sample : N6017-13
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 26 01:22:37 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration




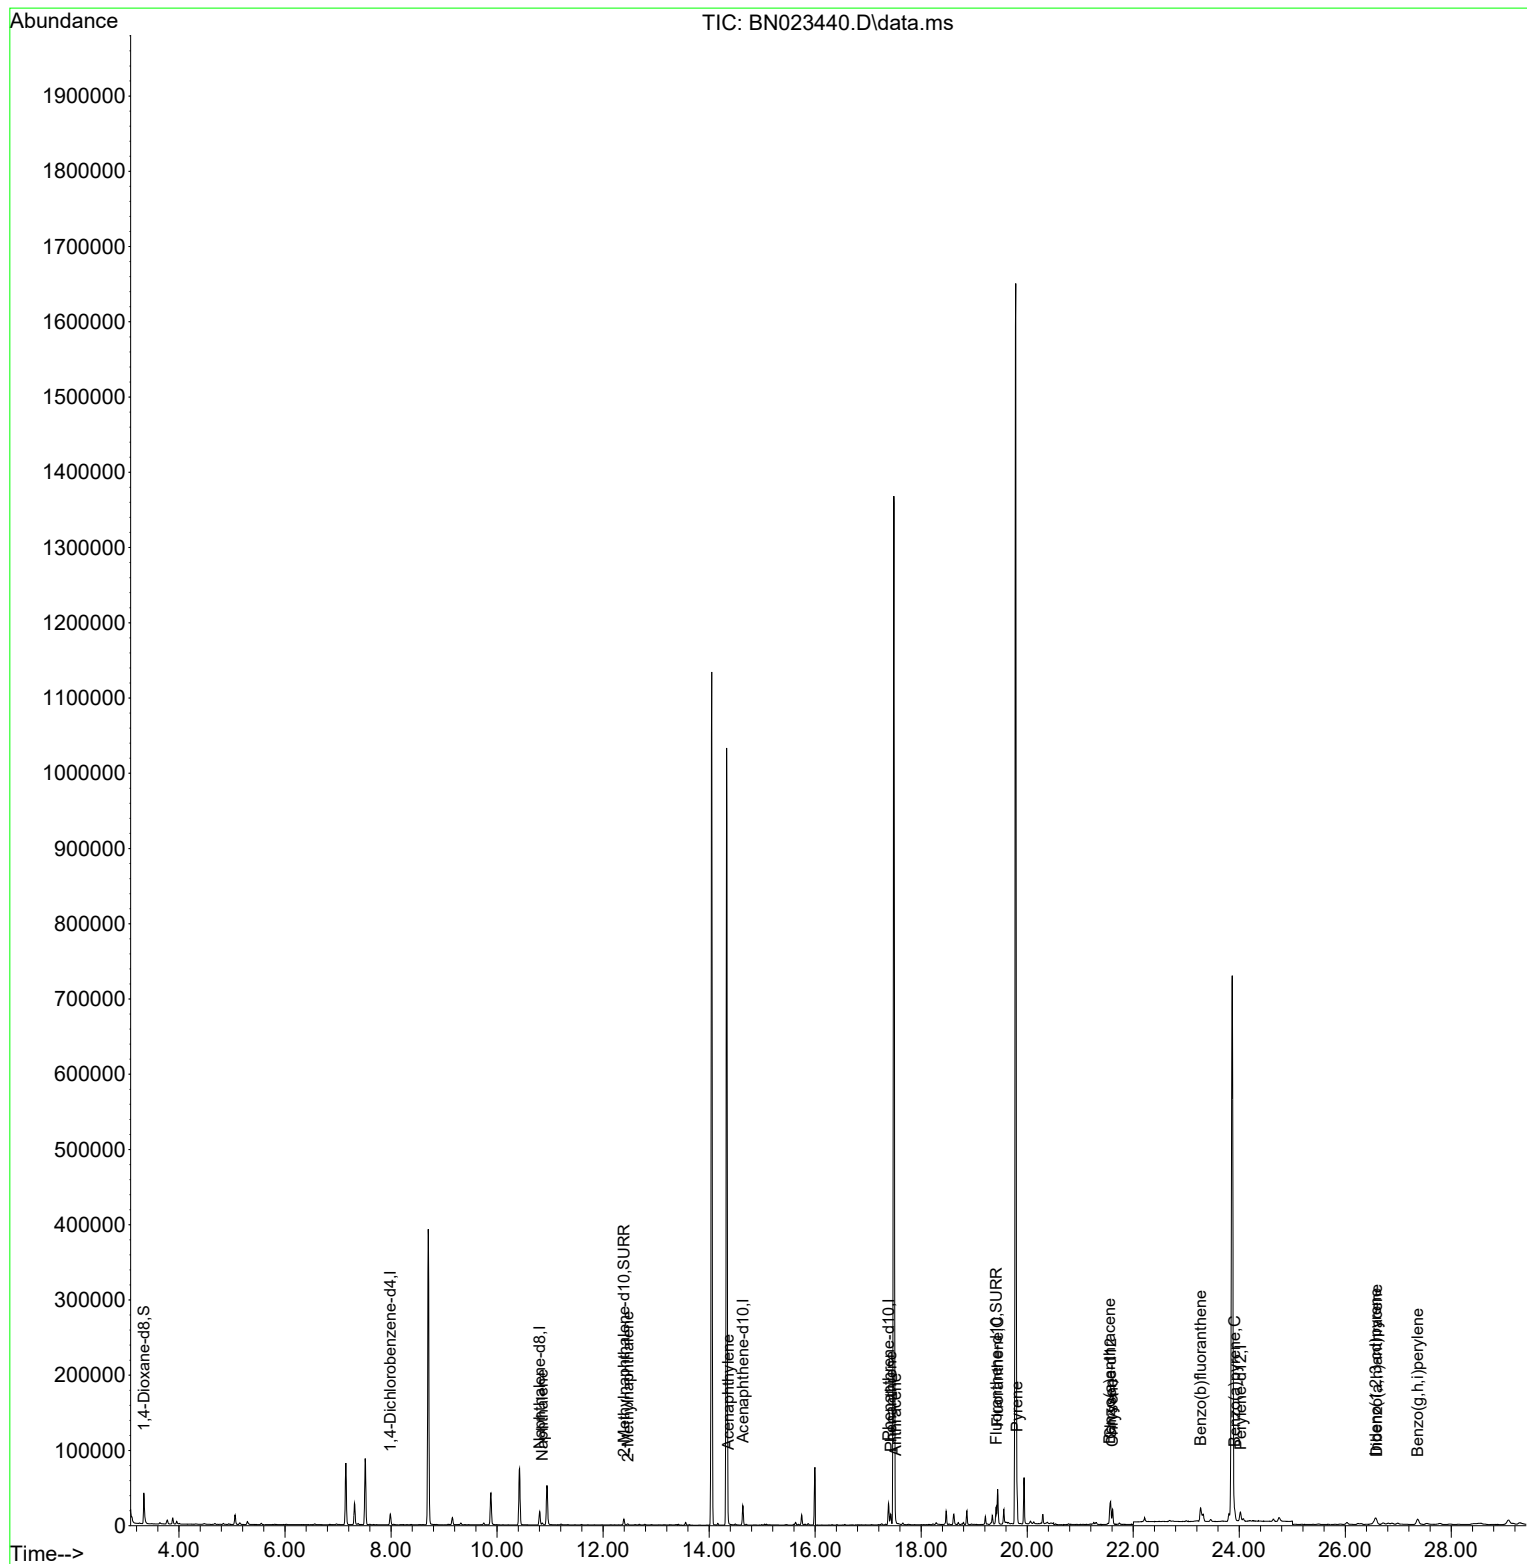


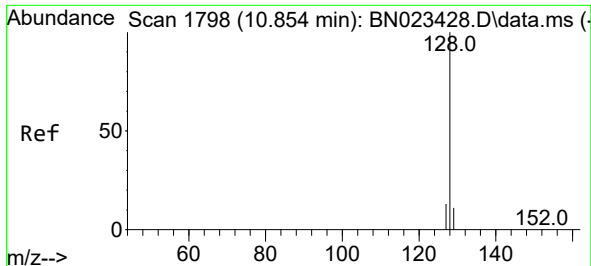

#5
Naphthalene
Concen: 0.047 ng/ul
RT: 10.854 min Scan# 1798
Delta R.T. 0.000 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:128 Resp: 3148
Ion Ratio Lower Upper
128 100
129 14.8 9.0 13.4#
127 15.8 10.7 16.1

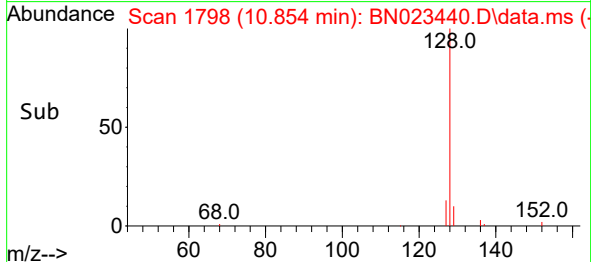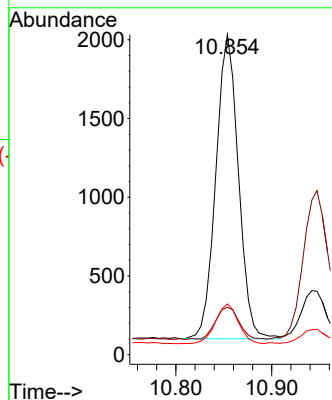

#7
2-Methylnaphthalene
Concen: 0.022 ng/ul
RT: 12.465 min Scan# 2091
Delta R.T. 0.000 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Tgt Ion:142 Resp: 933
Ion Ratio Lower Upper
142 100
141 91.1 71.4 107.2

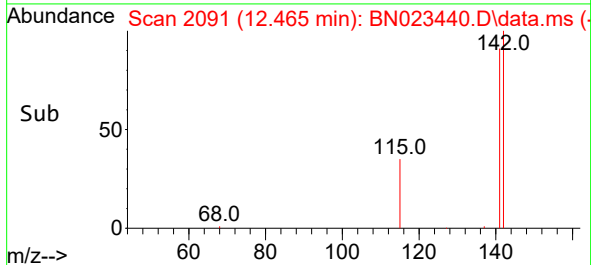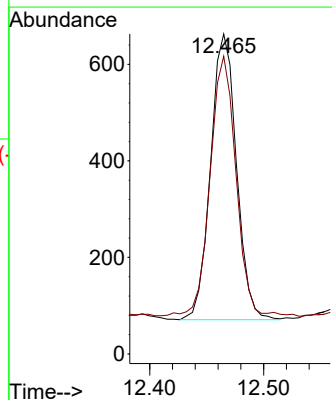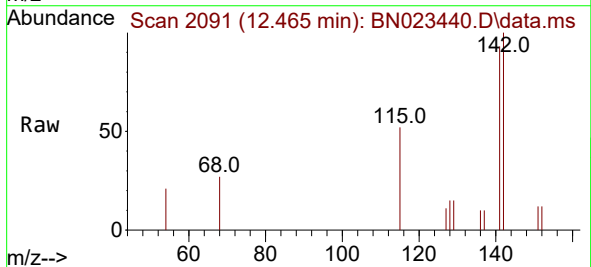



#10

Acenaphthylene

Concen: 0.036 ng/ul

RT: 14.358 min Scan# 2468

Delta R.T. 0.000 min


Lab File: BN023440.D

Acq: 25 Dec 2022 09:22

Instrument :

BNA_N

ClientSampleId :





Tgt Ion:152 Resp: 2180

Ion Ratio Lower Upper

152 100

151 24.9 16.1 24.1#

153 19.1 10.9 16.3#

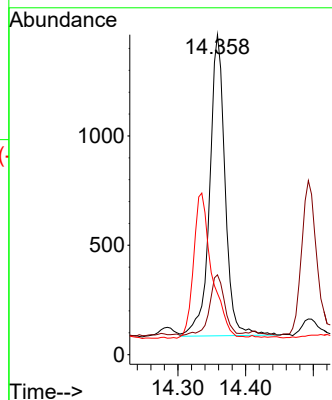

#15

Phenanthrene

Concen: 0.127 ng/ul

RT: 17.428 min Scan# 3161

Delta R.T. 0.000 min

Lab File: BN023440.D

Acq: 25 Dec 2022 09:22




Tgt Ion:178 Resp: 12833


Ion Ratio Lower Upper

178 100

179 17.5 12.5 18.7

176 26.9 15.7 23.5#

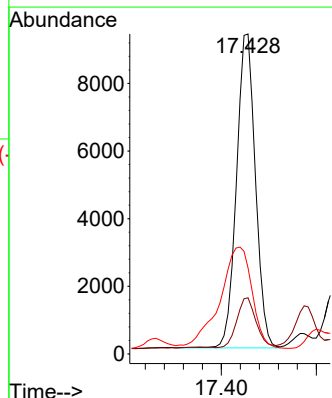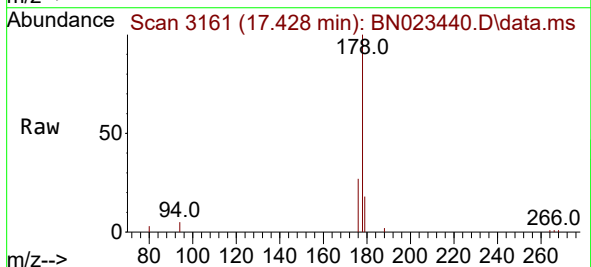



#16

Anthracene

Concen: 0.028 ng/ul

RT: 17.517 min Scan# 3182

Delta R.T. -0.004 min


Lab File: BN023440.D

Acq: 25 Dec 2022 09:22

Instrument :

BNA_N

ClientSampleId :






Tgt Ion:178 Resp: 2377

Ion Ratio Lower Upper

178 100

179 22.8 12.6 18.8#

176 31.8 15.4 23.0#

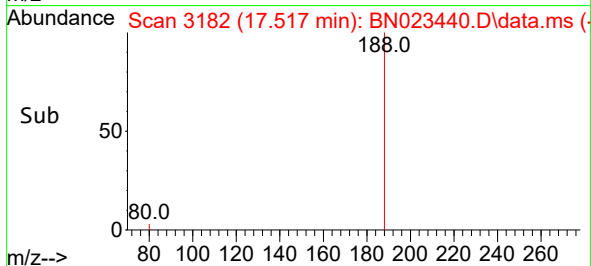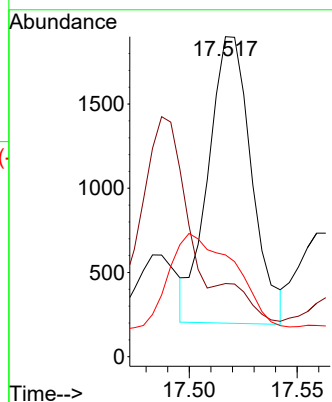

#19

Fluoranthene

Concen: 0.335 ng/ul

RT: 19.443 min Scan# 3618

Delta R.T. 0.000 min

Lab File: BN023440.D

Acq: 25 Dec 2022 09:22




Tgt Ion:202 Resp: 36270


Ion Ratio Lower Upper

202 100

101 15.5 9.4 14.2#

100 11.1 7.0 10.6#


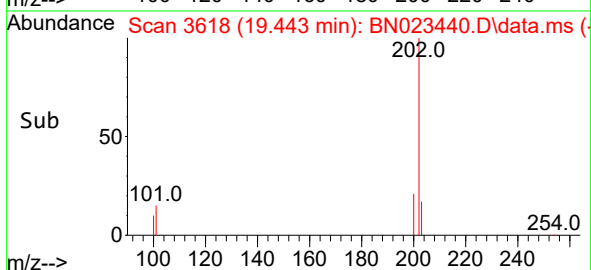
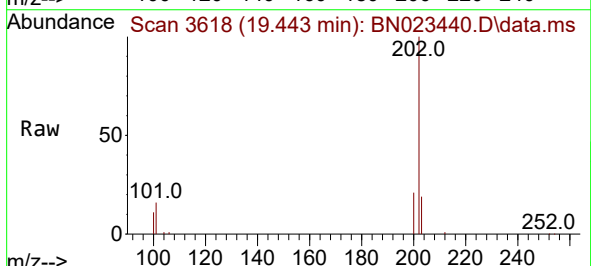
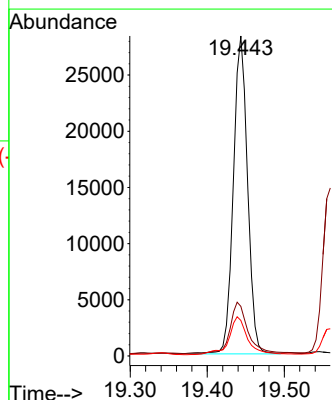


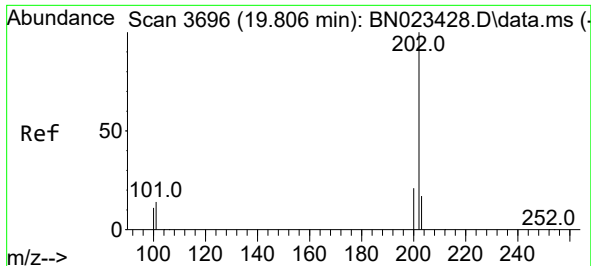

#20
Pyrene
Concen: 0.274 ng/ul
RT: 19.811 min Scan# 3697
Delta R.T. 0.005 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:202 Resp: 29899
Ion Ratio Lower Upper
202 100
101 13.6 11.3 16.9
100 10.6 9.0 13.4

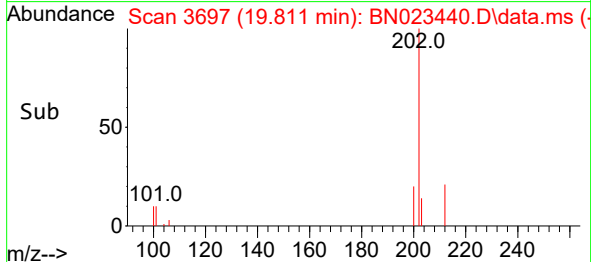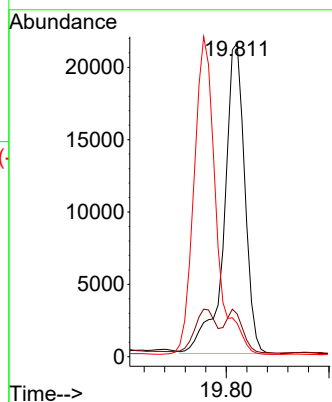

#21
Benzo(a)anthracene
Concen: 0.196 ng/ul
RT: 21.557 min Scan# 4207
Delta R.T. 0.001 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22


Tgt Ion:228 Resp: 16970
Ion Ratio Lower Upper
228 100
229 23.2 15.6 23.4
226 29.5 22.2 33.2

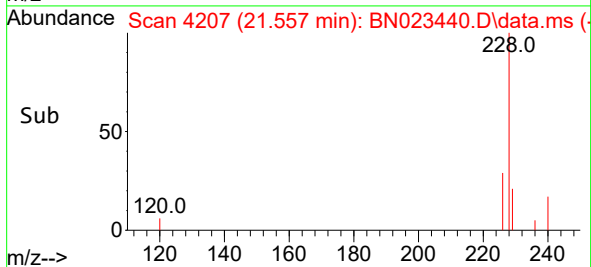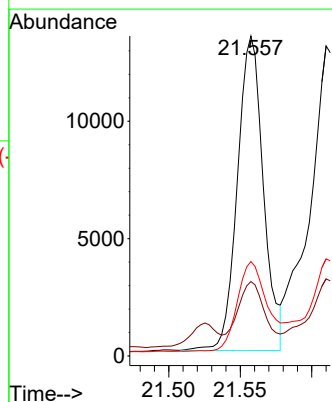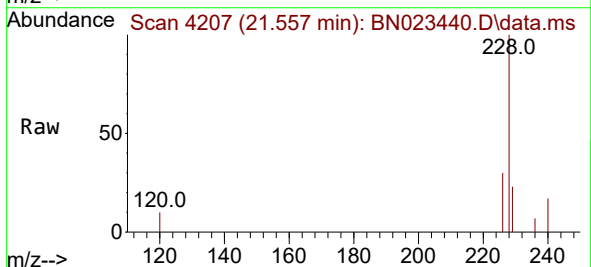



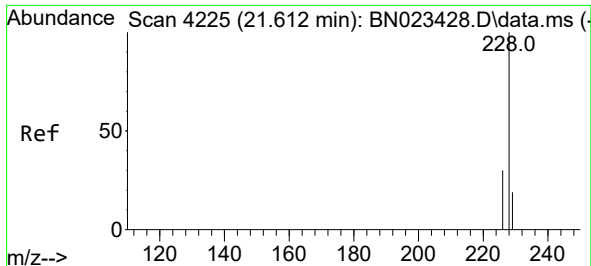


#22
Chrysene
Concen: 0.223 ng/ul
RT: 21.610 min Scan# 41
Delta R.T. -0.002 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Instrument :
BNA_N
ClientSampleId :







Tgt Ion:228 Resp: 19719
Ion Ratio Lower Upper
228 100
226 31.3 24.3 36.5
229 24.9 15.8 23.6#

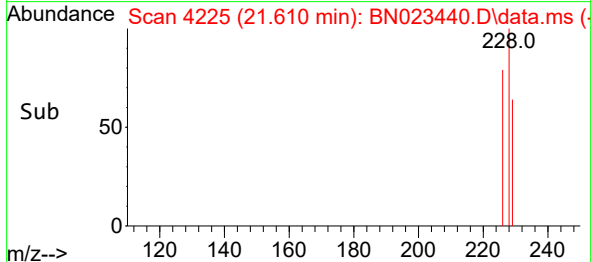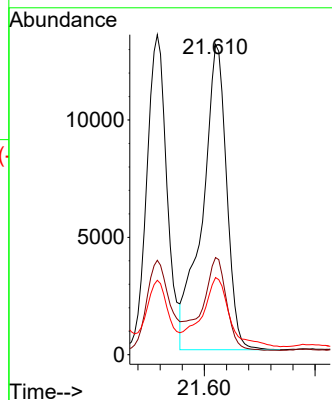

#24
Benzo(b)fluoranthene
Concen: 0.444 ng/ul
RT: 23.273 min Scan# 4794
Delta R.T. 0.004 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22


Tgt Ion:252 Resp: 38156
Ion Ratio Lower Upper
252 100
253 28.2 0.0 49.2
125 25.5 0.0 31.8

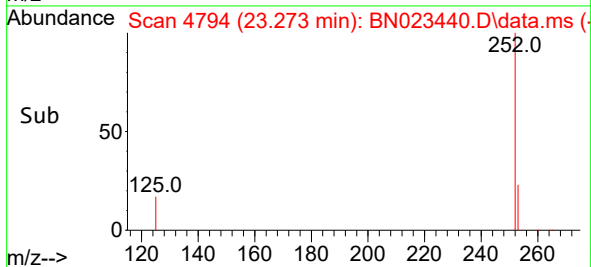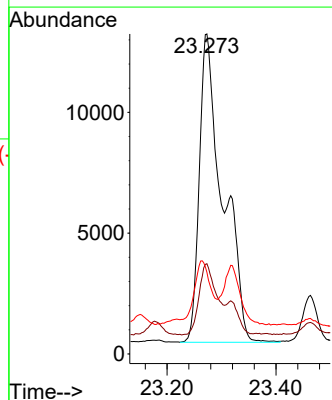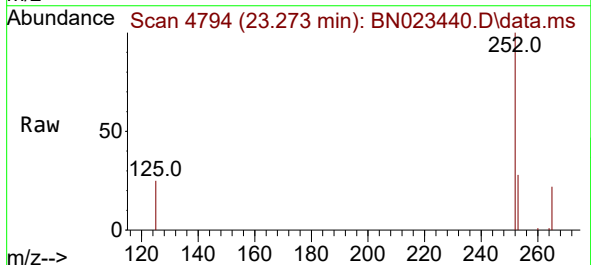



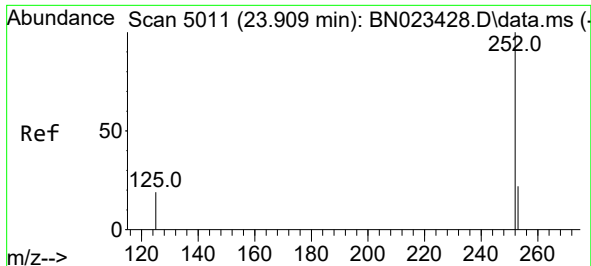


#26
Benzo(a)pyrene
Concen: 0.256 ng/ul
RT: 23.913 min Scan# 5011
Delta R.T. 0.004 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Instrument :
BNA_N
ClientSampleId :



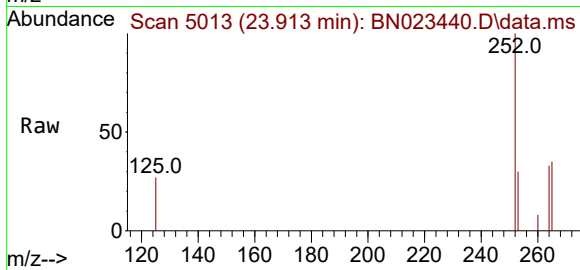



Tgt Ion:252 Resp: 17424
Ion Ratio Lower Upper
252 100
253 29.6 21.4 32.2
125 26.6 16.2 24.4#

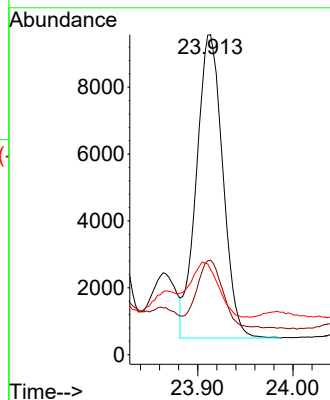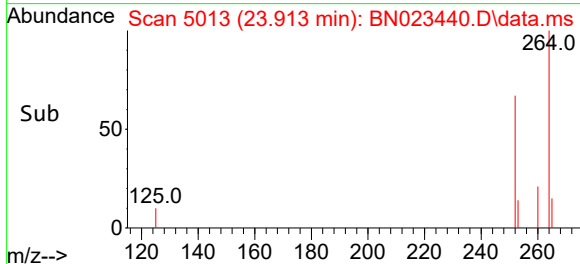

#27
Indeno(1,2,3-cd)pyrene
Concen: 0.180 ng/ul
RT: 26.574 min Scan# 5854
Delta R.T. -0.002 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Tgt Ion:276 Resp: 14315
Ion Ratio Lower Upper
276 100
138 43.4 23.4 35.2#
227 0.0 0.0 0.0


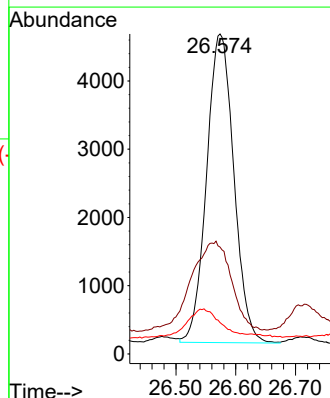
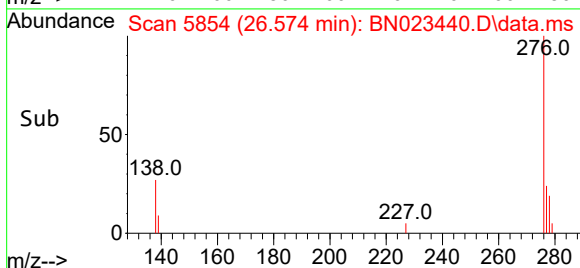
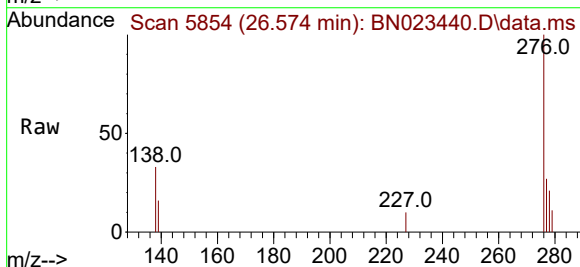


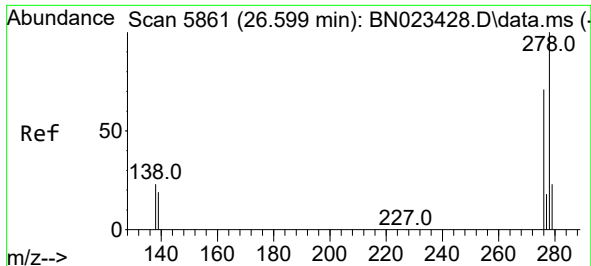

#28
Dibenzo(a,h)anthracene
Concen: 0.058 ng/ul
RT: 26.590 min Scan# 5859
Delta R.T. -0.008 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:278 Resp: 3599
Ion Ratio Lower Upper
278 100
139 56.0 16.6 24.8#
279 51.0 21.3 31.9#

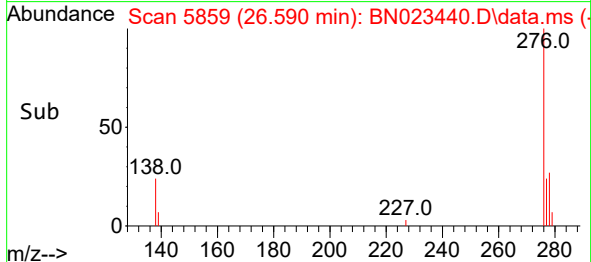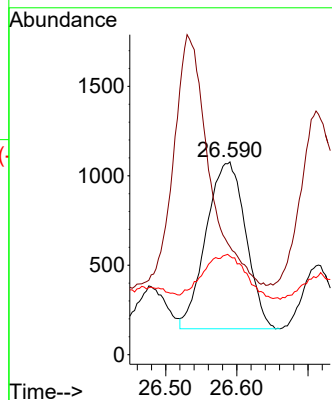

#29
Benzo(g,h,i)perylene
Concen: 0.224 ng/ul
RT: 27.365 min Scan# 6090
Delta R.T. -0.002 min
Lab File: BN023440.D
Acq: 25 Dec 2022 09:22

Tgt Ion:276 Resp: 14472
Ion Ratio Lower Upper
276 100
138 40.8 20.3 30.5#
277 26.7 19.7 29.5

