

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023448.D
 Acq On : 25 Dec 2022 14:10
 Operator : CG/JU
 Sample : N6017-18
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 01:23:46 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	7835	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	25658	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	15373	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	34171	0.400	ng/ul	0.00
17) Chrysene-d12	21.575	240	23824	0.400	ng/ul	0.00
23) Perylene-d12	24.022	264	17355	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	30726	3.609	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.394	152	10978	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.416	212	26362	0.306	ng/ul	0.00
Target Compounds						
					Qvalue	
15) Phenanthrene	17.428	178	10386	0.093	ng/ul	97
19) Fluoranthene	19.443	202	25645	0.222	ng/ul#	67
20) Pyrene	19.811	202	22358	0.192	ng/ul	100
21) Benzo(a)anthracene	21.557	228	10800	0.116	ng/ul#	92
22) Chrysene	21.613	228	14011	0.149	ng/ul#	92
24) Benzo(b)fluoranthene	23.273	252	25874	0.288	ng/ul#	51
26) Benzo(a)pyrene	23.913	252	11332	0.159	ng/ul#	78
27) Indeno(1,2,3-cd)pyrene	26.574	276	9614	0.116	ng/ul#	78
28) Dibenzo(a,h)anthracene	26.590	278	2394	0.037	ng/ul#	25
29) Benzo(g,h,i)perylene	27.368	276	10109	0.150	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023448.D
Acq On : 25 Dec 2022 14:10
Operator : CG/JU
Sample : N6017-18
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 26 01:23:46 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

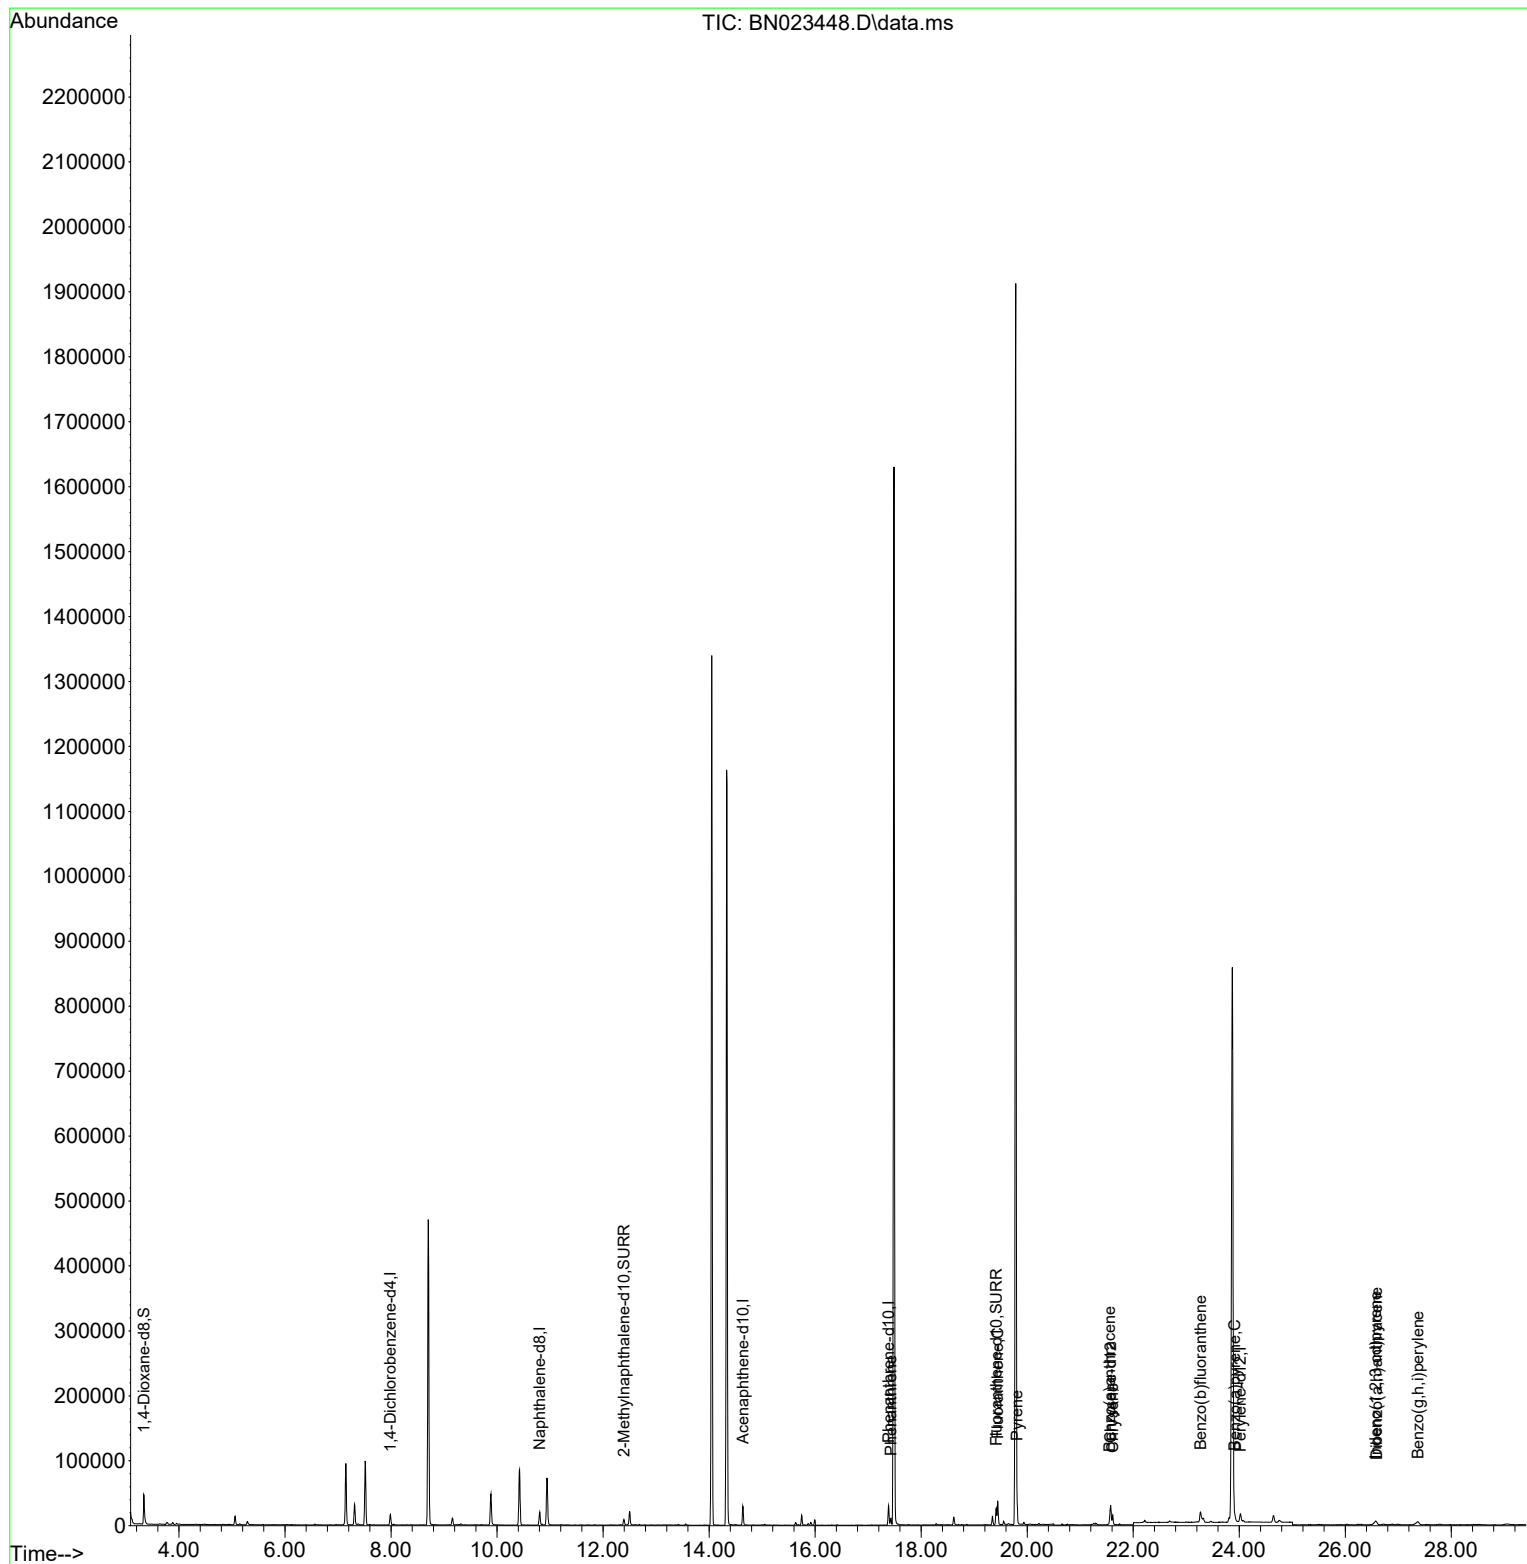



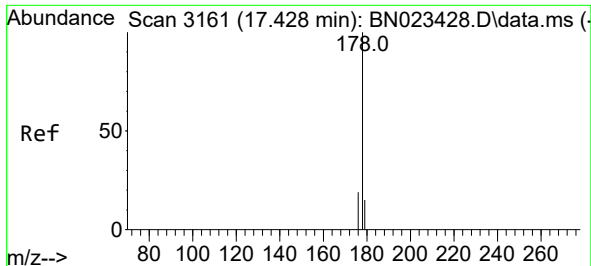


#15
Phenanthrene
Concen: 0.093 ng/ul
RT: 17.428 min Scan# 3161
Delta R.T. 0.000 min
Lab File: BN023448.D
Acq: 25 Dec 2022 14:10

Instrument :
BNA_N
ClientSampleId :



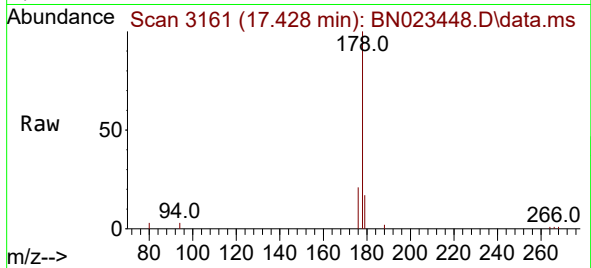



Tgt Ion:178 Resp: 10386
Ion Ratio Lower Upper
178 100
179 16.9 12.5 18.7
176 20.8 15.7 23.5

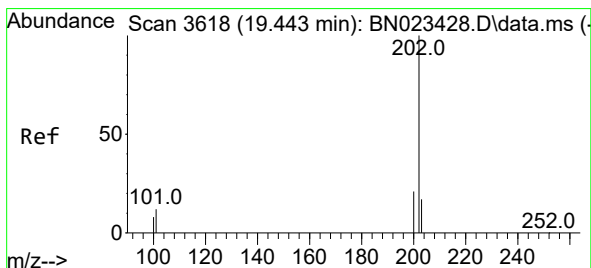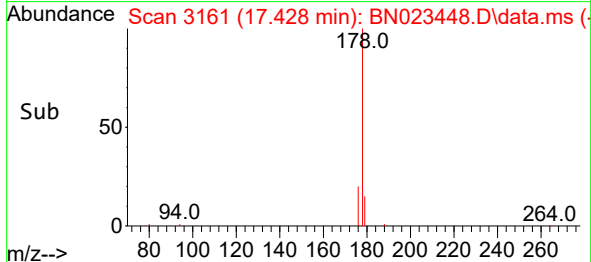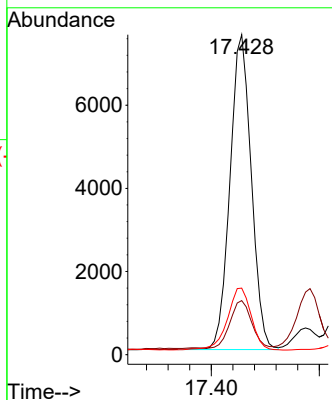

#19
Fluoranthene
Concen: 0.222 ng/ul
RT: 19.443 min Scan# 3618
Delta R.T. 0.000 min
Lab File: BN023448.D
Acq: 25 Dec 2022 14:10

Tgt Ion:202 Resp: 25645
Ion Ratio Lower Upper
202 100
101 26.1 9.4 14.2#
100 19.2 7.0 10.6#


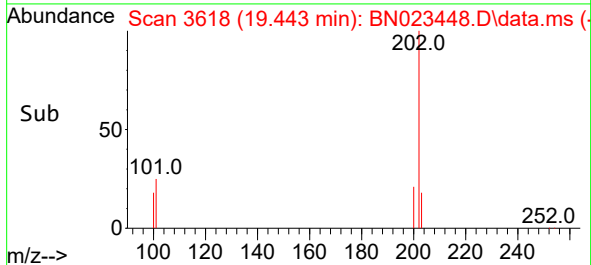
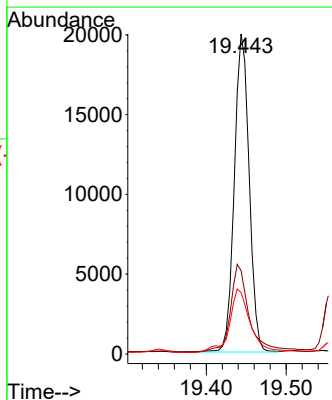
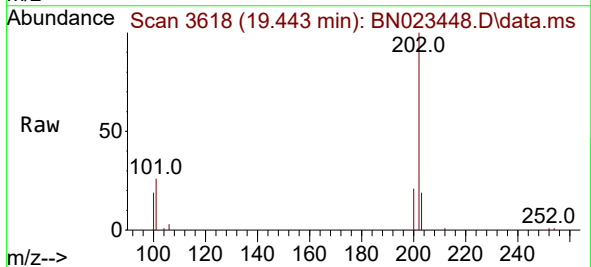


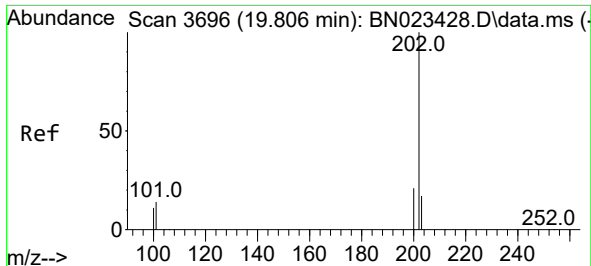

#20
Pyrene
Concen: 0.192 ng/ul
RT: 19.811 min Scan# 30
Delta R.T. 0.005 min
Lab File: BN023448.D
Acq: 25 Dec 2022 14:10




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:202 Resp: 22358
Ion Ratio Lower Upper
202 100
101 14.1 11.3 16.9
100 11.3 9.0 13.4

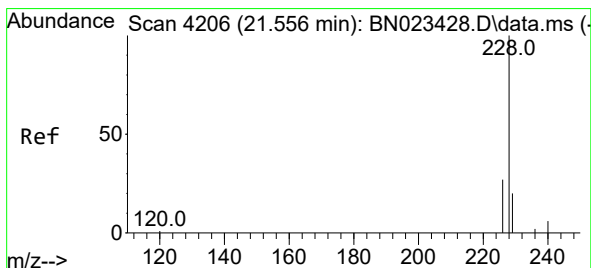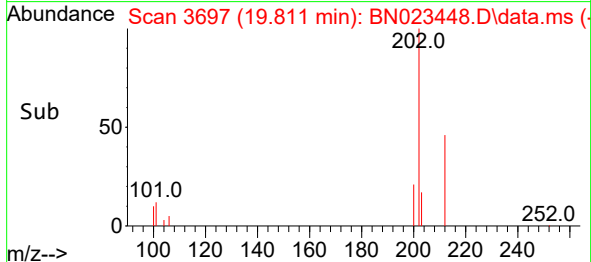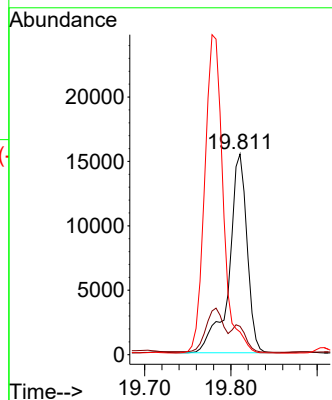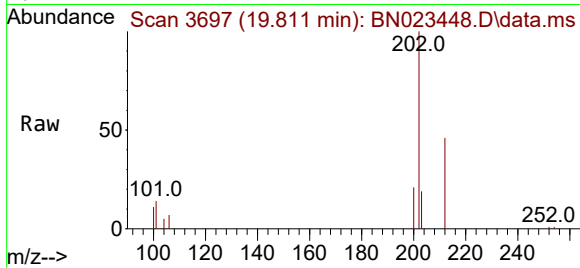

#21
Benzo(a)anthracene
Concen: 0.116 ng/ul
RT: 21.557 min Scan# 4207
Delta R.T. 0.001 min
Lab File: BN023448.D
Acq: 25 Dec 2022 14:10

Tgt Ion:228 Resp: 10800
Ion Ratio Lower Upper
228 100
229 25.7 15.6 23.4#
226 29.4 22.2 33.2

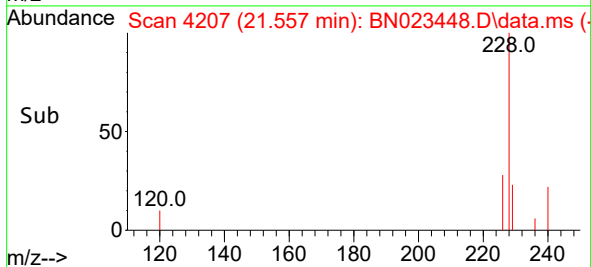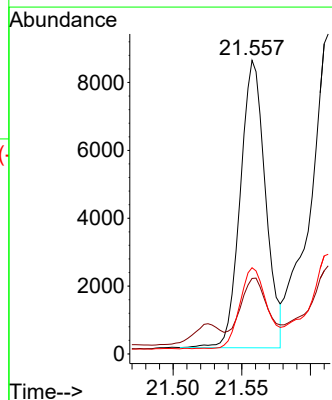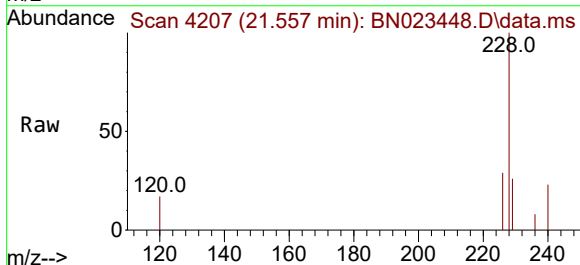

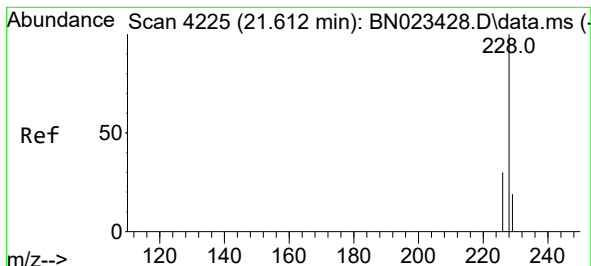

#22

Chrysene

Concen: 0.149 ng/ul

RT: 21.613 min Scan# 41

Delta R.T. 0.001 min


Lab File: BN023448.D

Acq: 25 Dec 2022 14:10

Instrument :

BNA_N

ClientSampleId :

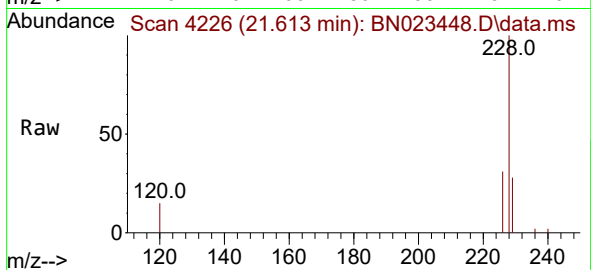




Tgt Ion:228 Resp: 14011

Ion Ratio Lower Upper

228 100

226 31.1 24.3 36.5

229 27.6 15.8 23.6#

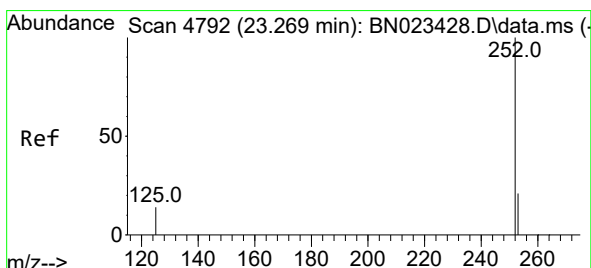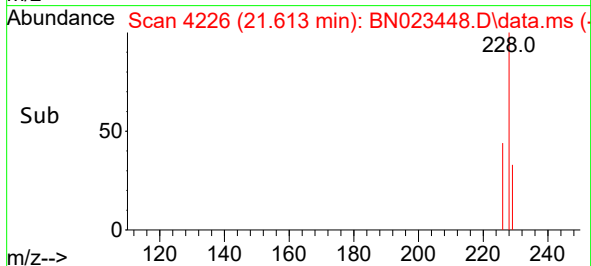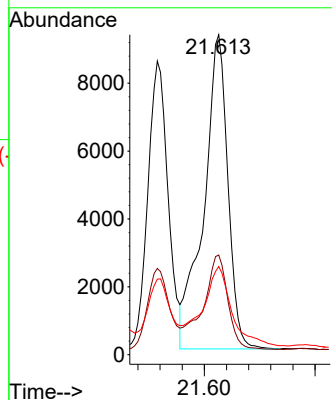

#24

Benzo(b)fluoranthene

Concen: 0.288 ng/ul

RT: 23.273 min Scan# 4794

Delta R.T. 0.004 min

Lab File: BN023448.D

Acq: 25 Dec 2022 14:10




Tgt Ion:252 Resp: 25874


Ion Ratio Lower Upper

252 100

253 32.6 0.0 49.2

125 58.3 0.0 31.8#

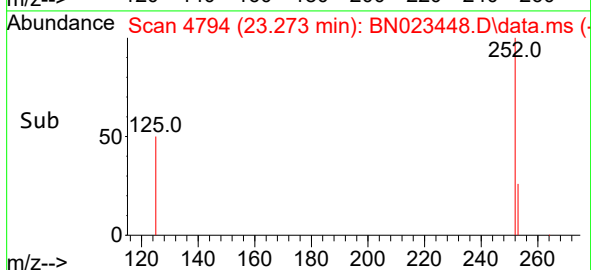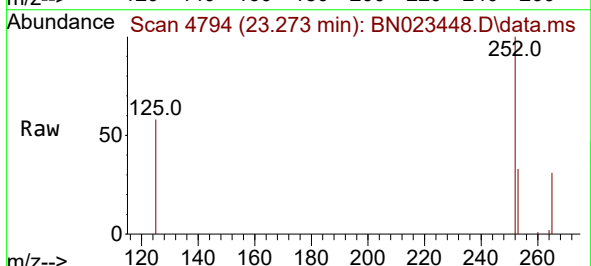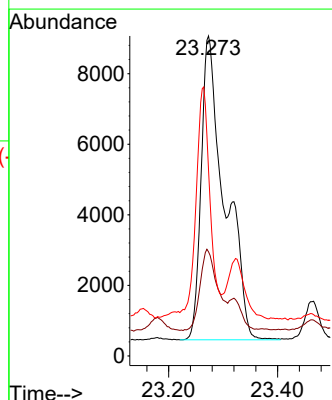

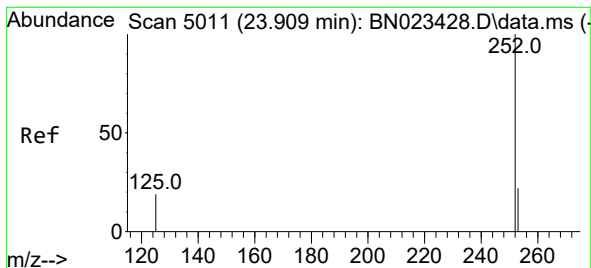

#26

Benzo(a)pyrene

Concen: 0.159 ng/ul

RT: 23.913 min Scan# 5011

Delta R.T. 0.004 min

Lab File: BN023448.D

Acq: 25 Dec 2022 14:10





Instrument :

BNA_N

ClientSampleId :

Tgt Ion:252 Resp: 11332

Ion	Ratio	Lower	Upper
252	100		
253	32.5	21.4	32.2#
125	36.9	16.2	24.4#

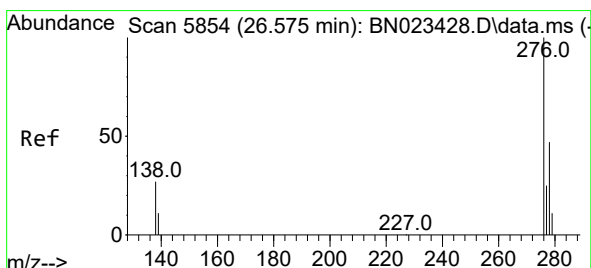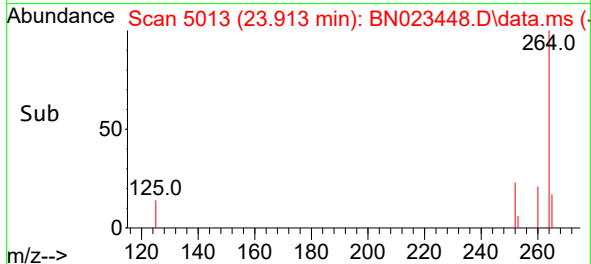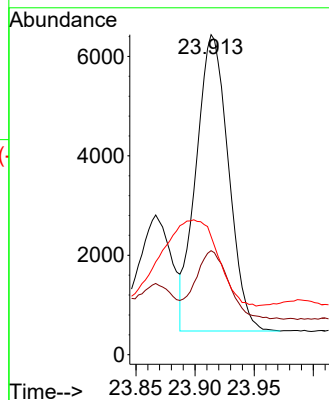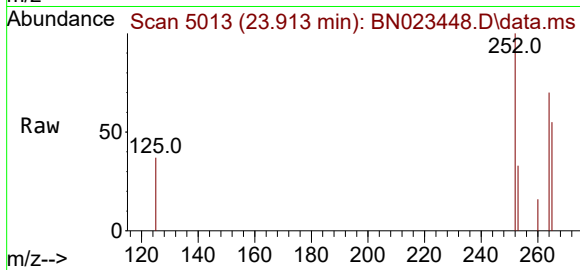

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.116 ng/ul

RT: 26.574 min Scan# 5854




Delta R.T. -0.002 min


Lab File: BN023448.D

Acq: 25 Dec 2022 14:10

Tgt Ion:276 Resp: 9614

Ion	Ratio	Lower	Upper
276	100		
138	41.0	23.4	35.2#
227	0.0	0.0	0.0


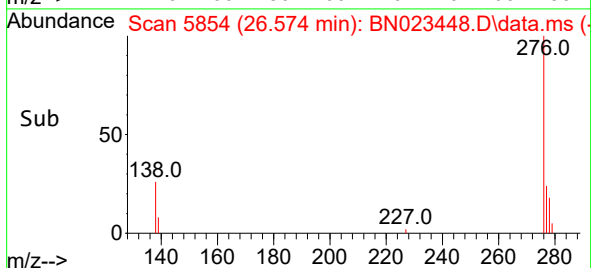
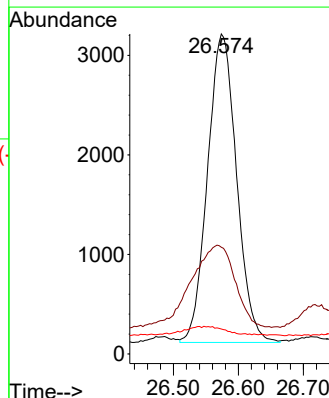
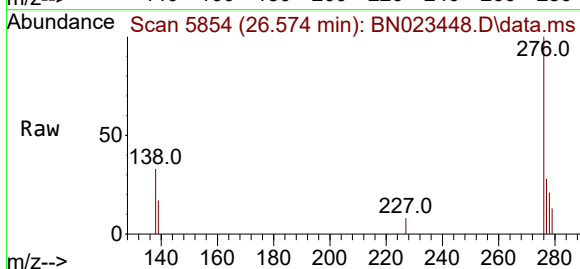


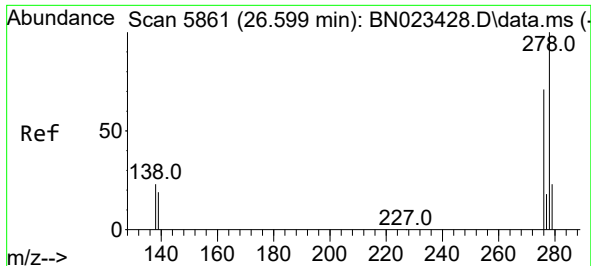

#28
 Dibenzo(a,h)anthracene
 Concen: 0.037 ng/ul
 RT: 26.590 min Scan# 5859
 Delta R.T. -0.008 min
 Lab File: BN023448.D
 Acq: 25 Dec 2022 14:10

Instrument :
 BNA_N
 ClientSampleId :

Tgt Ion:278 Resp: 2394
 Ion Ratio Lower Upper
 278 100
 139 60.3 16.6 24.8#
 279 61.0 21.3 31.9#

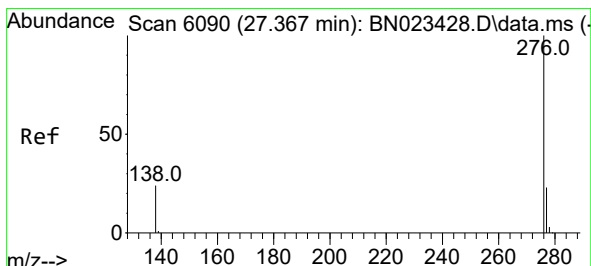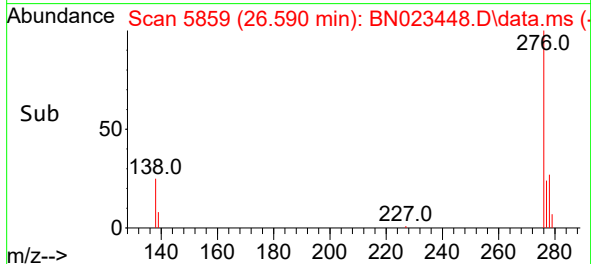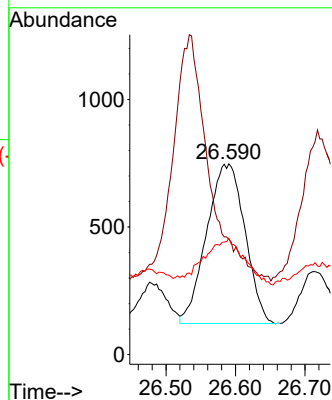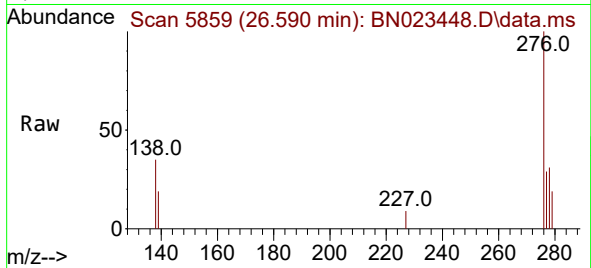

#29
 Benzo(g,h,i)perylene
 Concen: 0.150 ng/ul
 RT: 27.368 min Scan# 6091
 Delta R.T. 0.002 min
 Lab File: BN023448.D
 Acq: 25 Dec 2022 14:10

Tgt Ion:276 Resp: 10109
 Ion Ratio Lower Upper
 276 100
 138 36.0 20.3 30.5#
 277 27.8 19.7 29.5

