

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023456.D
 Acq On : 25 Dec 2022 20:19
 Operator : CG/JU
 Sample : PB149683BL
 Misc :
 ALS Vial : 92 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 02:57:47 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	5590	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	18431	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	10634	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	23928	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240	14987	0.400	ng/ul	0.00
23) Perylene-d12	24.019	264	12310	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	31570	5.198	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.394	152	9041	0.317	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	19611	0.362	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.631	166	2795	0.063	ng/ul#	14
20) Pyrene	19.778	202	2401	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.861	252	3854	0.076	ng/ul#	44


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023456.D
Acq On : 25 Dec 2022 20:19
Operator : CG/JU
Sample : PB149683BL
Misc :
ALS Vial : 92 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 26 02:57:47 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

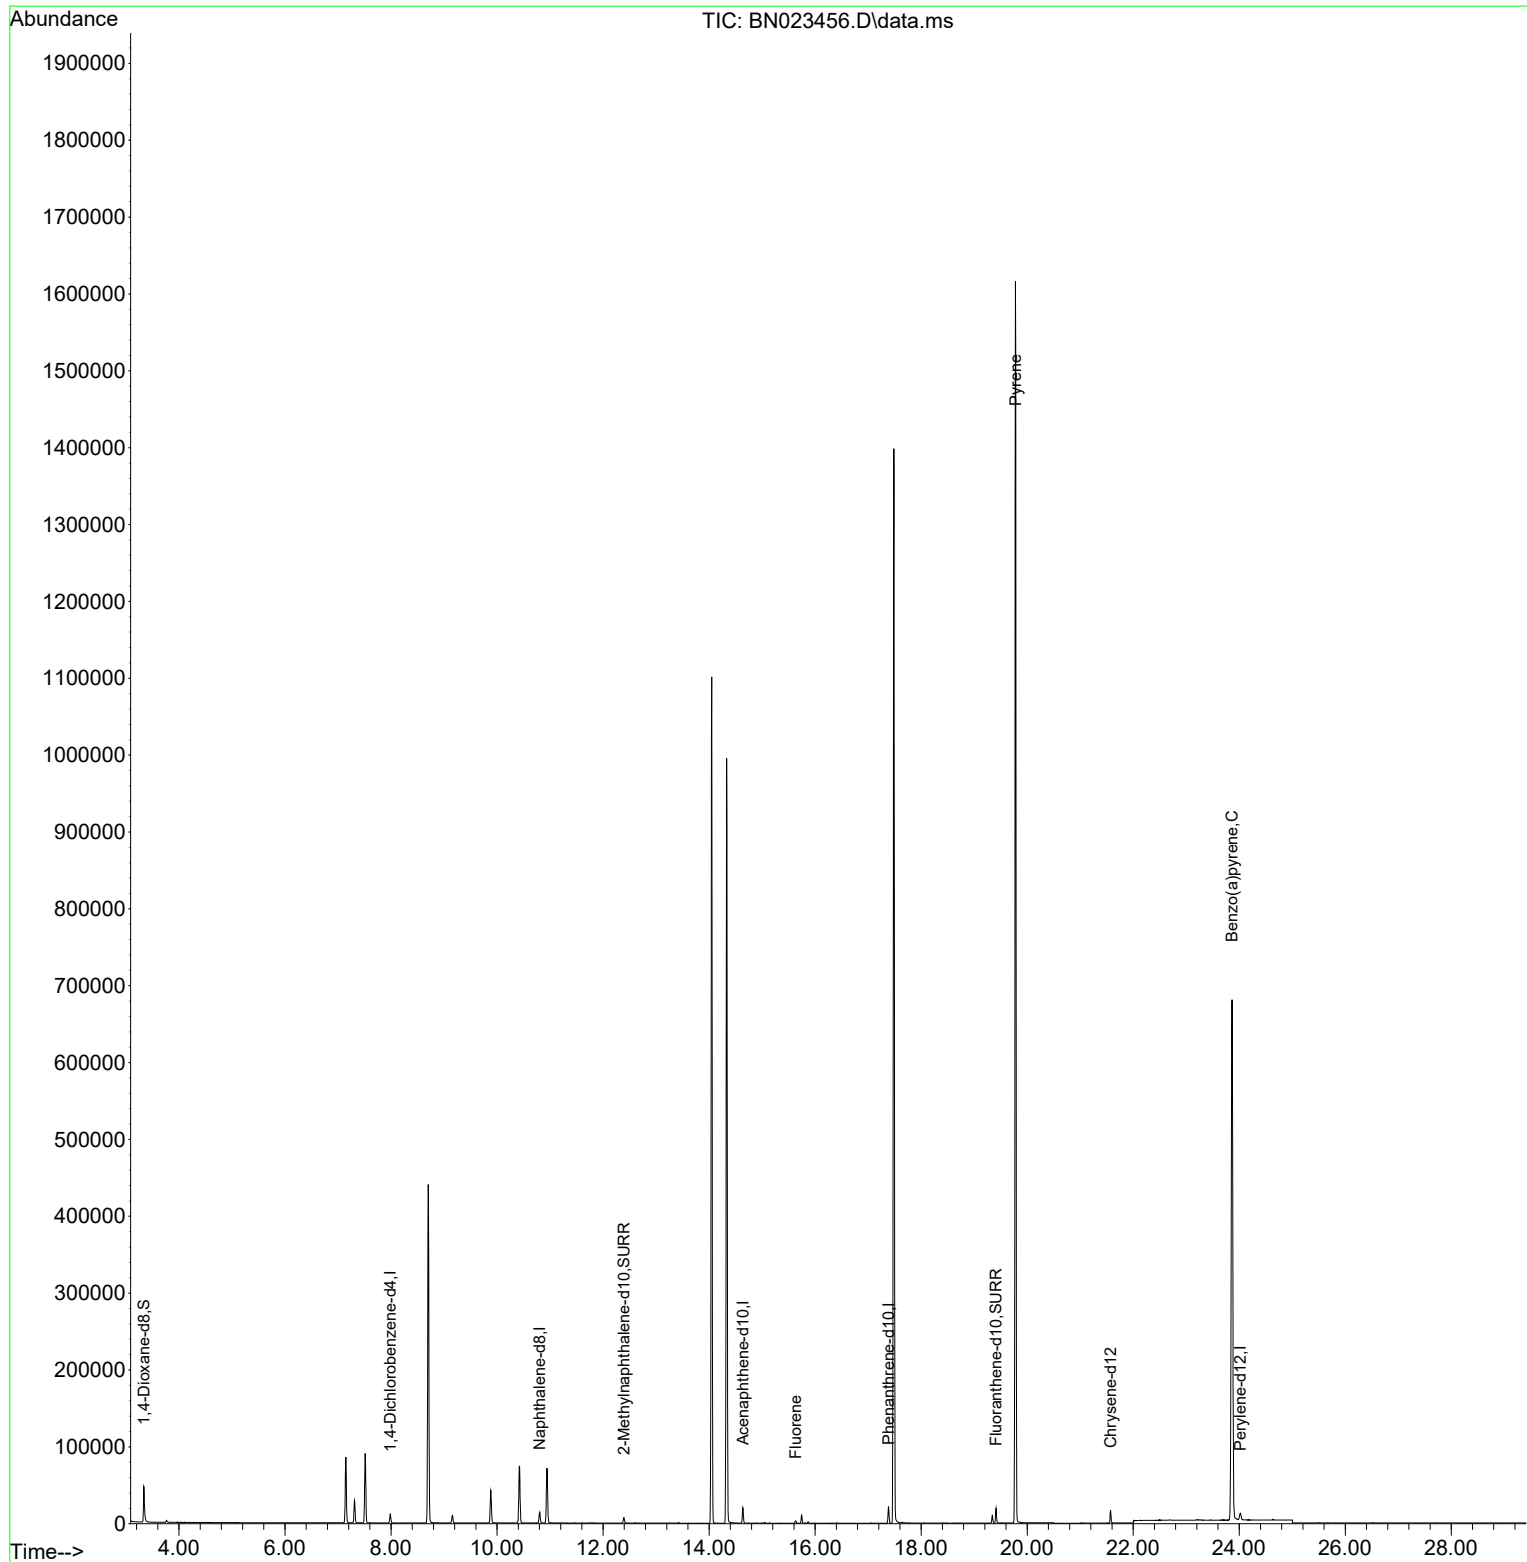



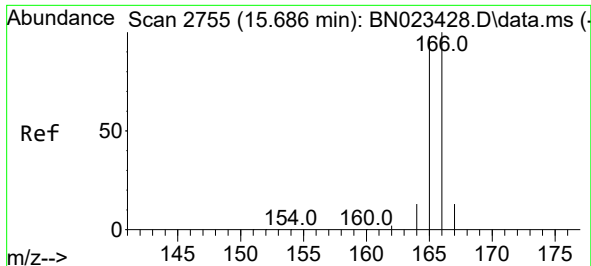


#12
Fluorene
Concen: 0.063 ng/ul
RT: 15.631 min Scan# 21
Delta R.T. -0.055 min
Lab File: BN023456.D
Acq: 25 Dec 2022 20:19

Instrument :
BNA_N
ClientSampleId :



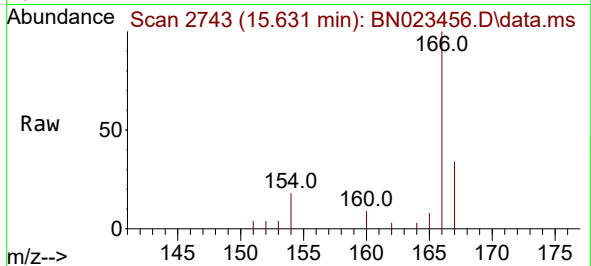



Tgt Ion:166 Resp: 2795
Ion Ratio Lower Upper
166 100
165 7.9 79.1 118.7#
167 33.7 11.0 16.4#

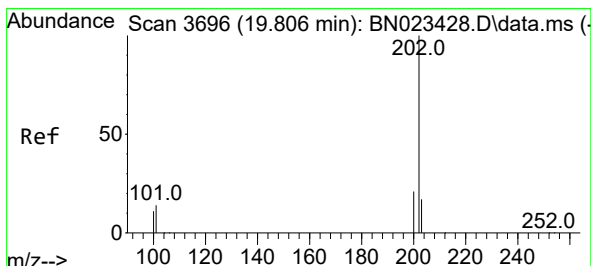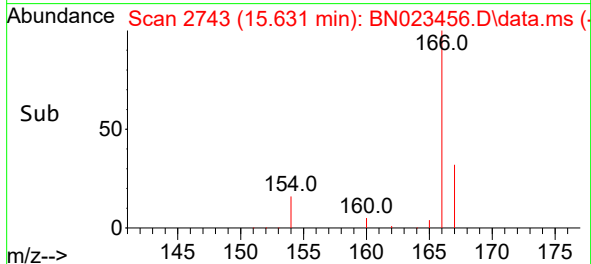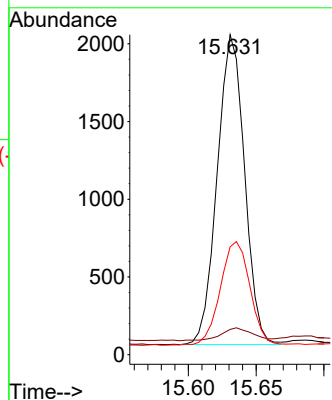

#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.778 min Scan# 3690
Delta R.T. -0.028 min
Lab File: BN023456.D
Acq: 25 Dec 2022 20:19


Tgt Ion:202 Resp: 2401
Ion Ratio Lower Upper
202 100
101 159.2 11.3 16.9#
100 1199.3 9.0 13.4#

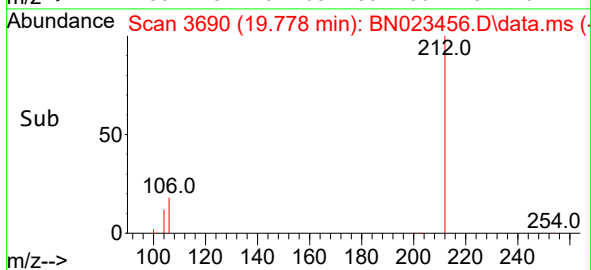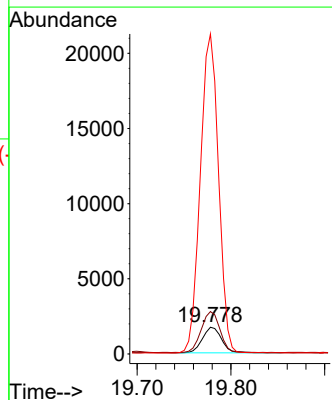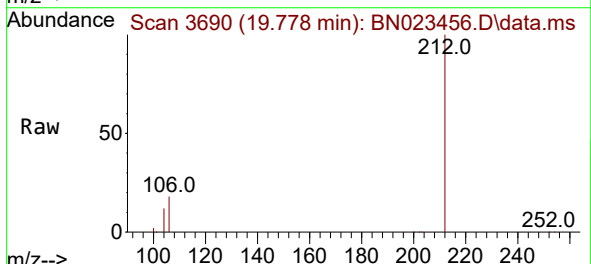

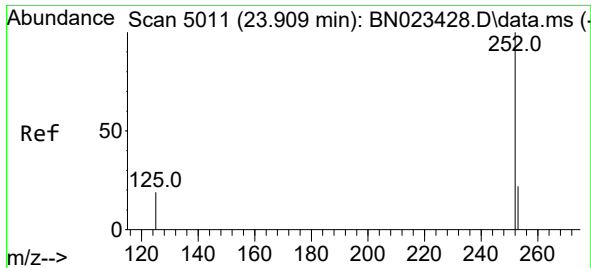

#26
Benzo(a)pyrene
Concen: 0.076 ng/ul
RT: 23.861 min Scan# 4995
Delta R.T. -0.048 min
Lab File: BN023456.D
Acq: 25 Dec 2022 20:19

Instrument :
BNA_N
ClientSampleId :

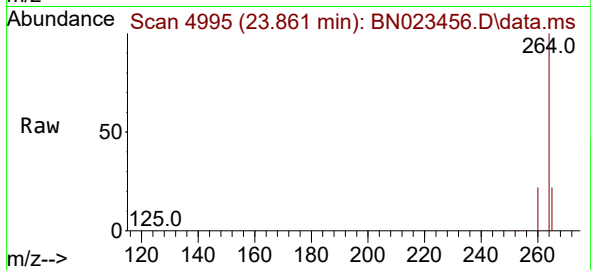

Tgt Ion:252 Resp: 3854
Ion Ratio Lower Upper
252 100
253 51.2 21.4 32.2#
125 51.1 16.2 24.4#

