

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023457.D
 Acq On : 25 Dec 2022 20:55
 Operator : CG/JU
 Sample : N6032-01
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 02:57:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	6385	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	21150	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	12077	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	26906	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	15834	0.400	ng/ul	0.00
23) Perylene-d12	24.017	264	13007	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	27664	3.988	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.393	152	5502	0.168	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	14294	0.250	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	942	0.133	ng/ul#	65
20) Pyrene	19.778	202	1854	0.024	ng/ul#	1
26) Benzo(a)pyrene	23.860	252	2742	0.051	ng/ul#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023457.D
Acq On : 25 Dec 2022 20:55
Operator : CG/JU
Sample : N6032-01
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 26 02:57:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration




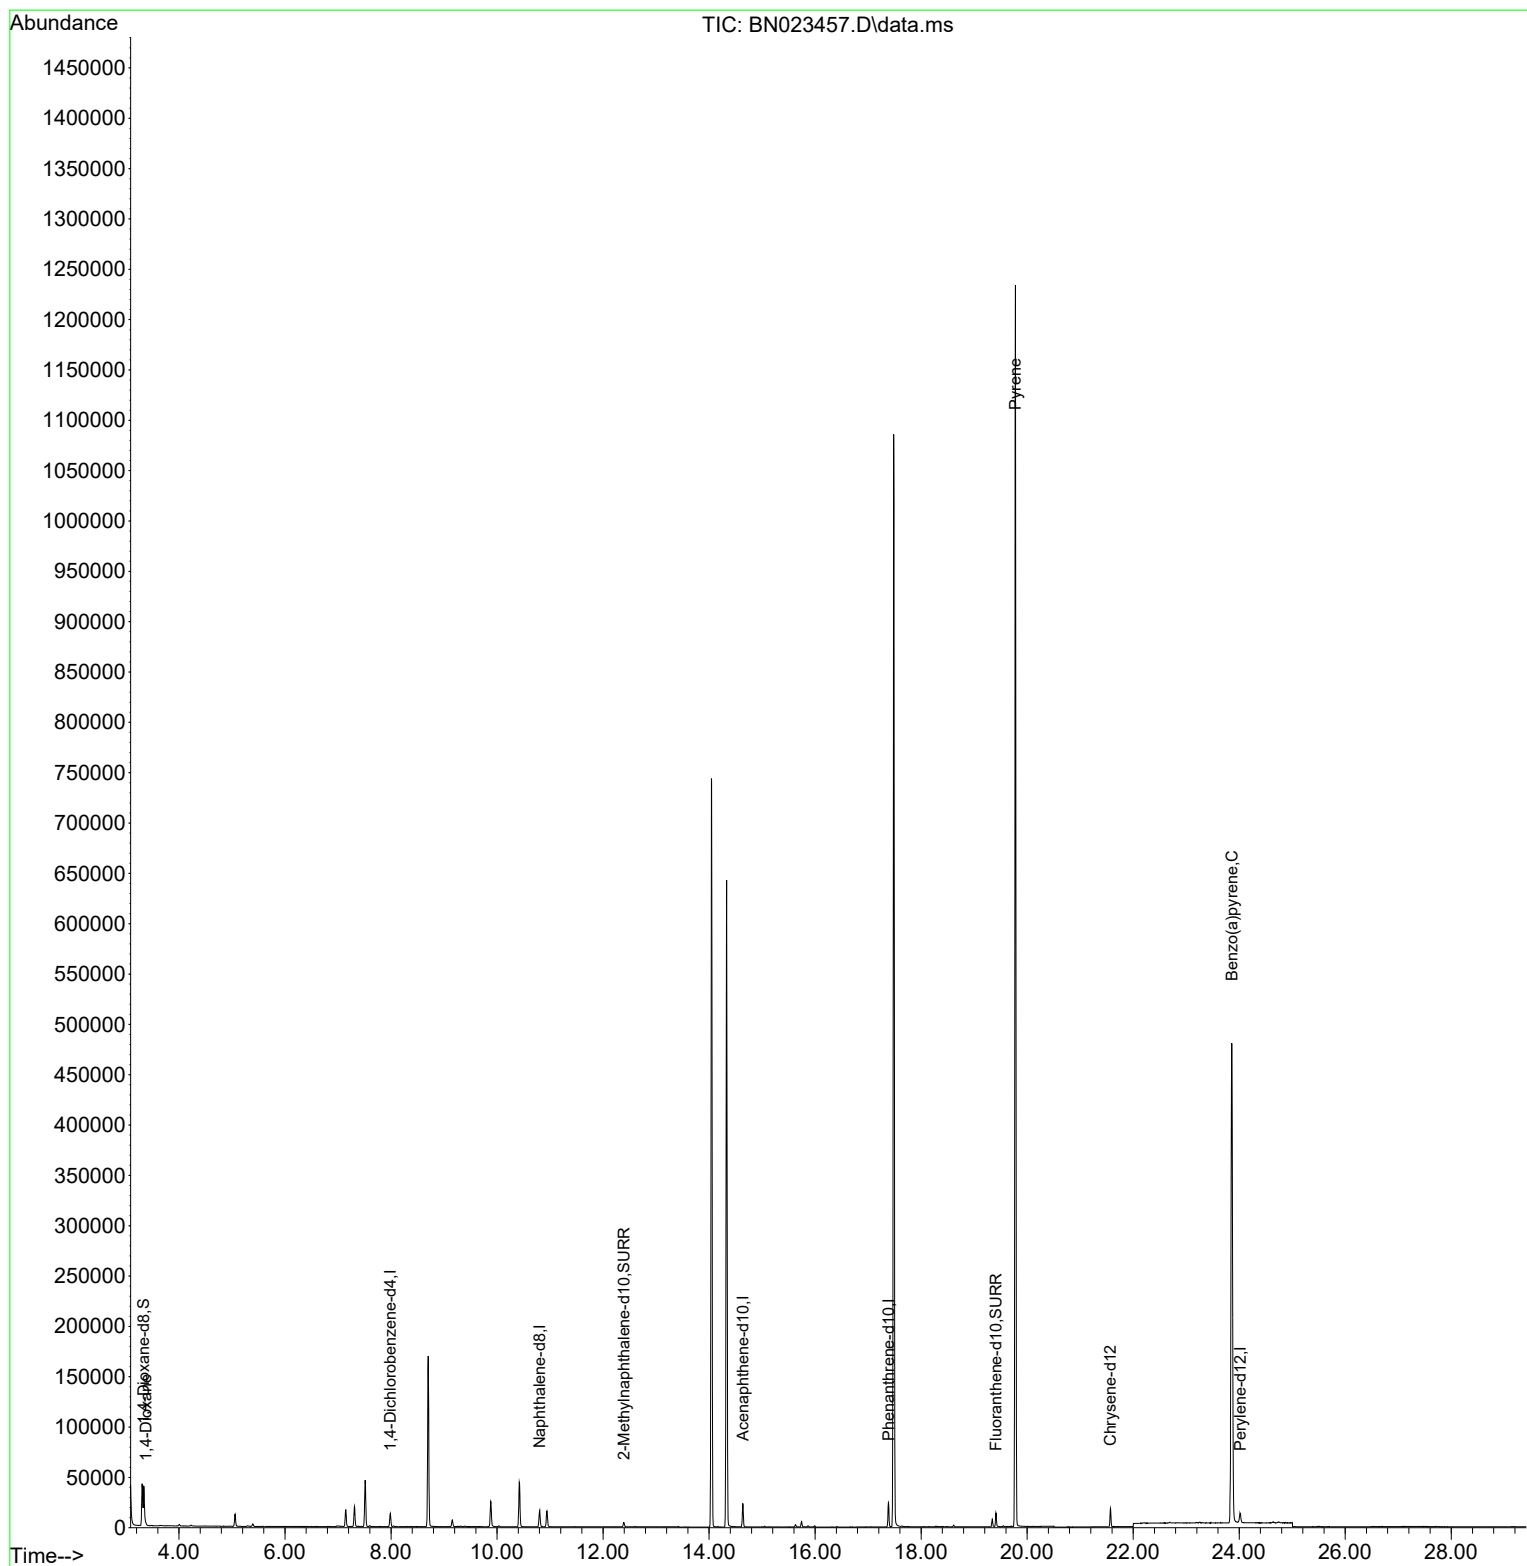


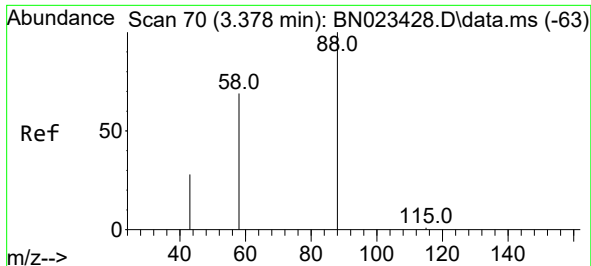

#2
1,4-Dioxane
Concen: 0.133 ng/ul
RT: 3.378 min Scan# 70
Delta R.T. -0.000 min
Lab File: BN023457.D
Acq: 25 Dec 2022 20:55




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 88 Resp: 942
Ion Ratio Lower Upper
88 100
43 76.1 28.4 42.6#
58 47.5 45.6 68.4

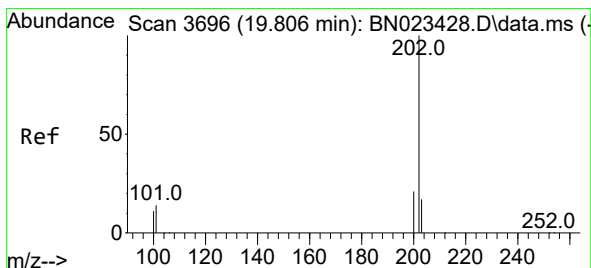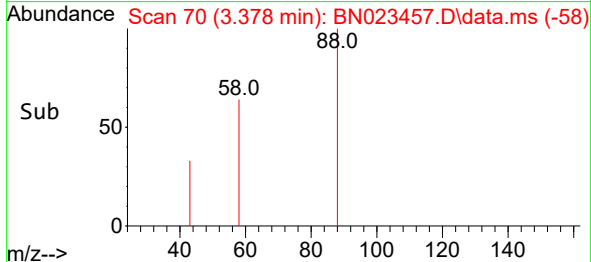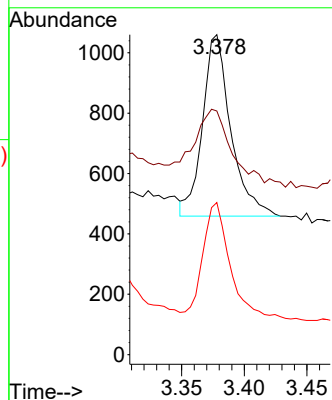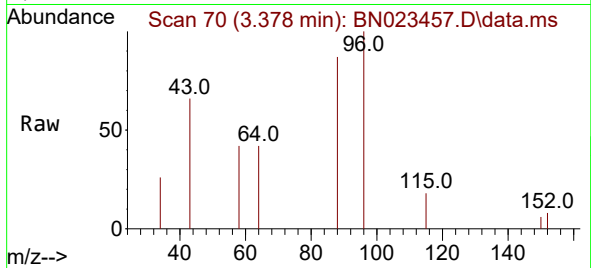

#20
Pyrene
Concen: 0.024 ng/ul
RT: 19.778 min Scan# 3690
Delta R.T. -0.028 min
Lab File: BN023457.D
Acq: 25 Dec 2022 20:55


Tgt Ion: 202 Resp: 1854
Ion Ratio Lower Upper
202 100
101 159.4 11.3 16.9#
100 1135.8 9.0 13.4#

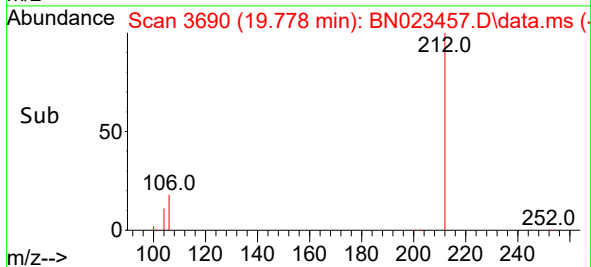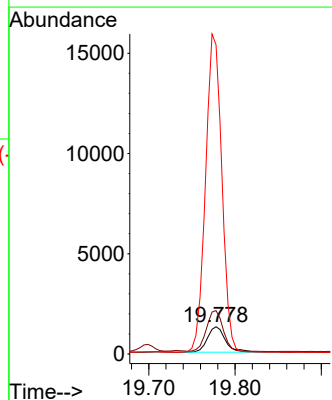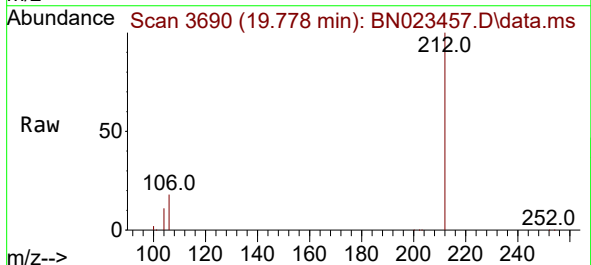

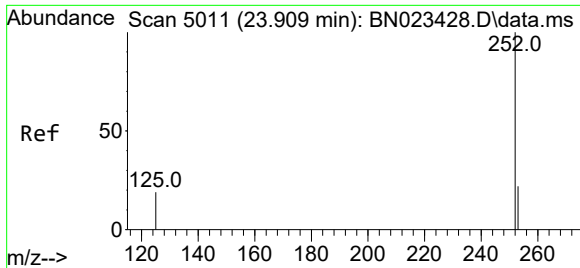

#26
Benzo(a)pyrene
Concen: 0.051 ng/ul
RT: 23.860 min Scan# 4994
Delta R.T. -0.050 min
Lab File: BN023457.D
Acq: 25 Dec 2022 20:55

Instrument :
BNA_N
ClientSampleId :

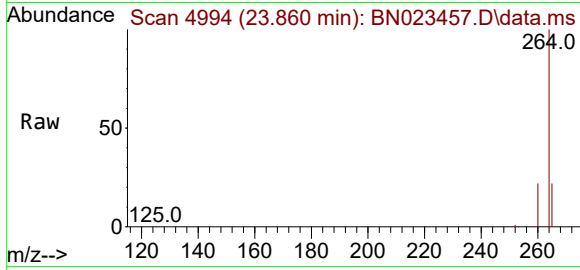

Tgt Ion:252 Resp: 2742
Ion Ratio Lower Upper
252 100
253 60.2 21.4 32.2#
125 65.0 16.2 24.4#

