

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023459.D
 Acq On : 25 Dec 2022 22:07
 Operator : CG/JU
 Sample : N6032-03
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 02:58:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	5841	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	19424	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	11121	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	25181	0.400	ng/ul	0.00
17) Chrysene-d12	21.570	240	15818	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264	13039	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.393	152	8405	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	22601	0.395	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	720	0.111	ng/ul#	61
20) Pyrene	19.778	202	3116	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.859	252	4259	0.080	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023459.D
Acq On : 25 Dec 2022 22:07
Operator : CG/JU
Sample : N6032-03
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Dec 26 02:58:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration




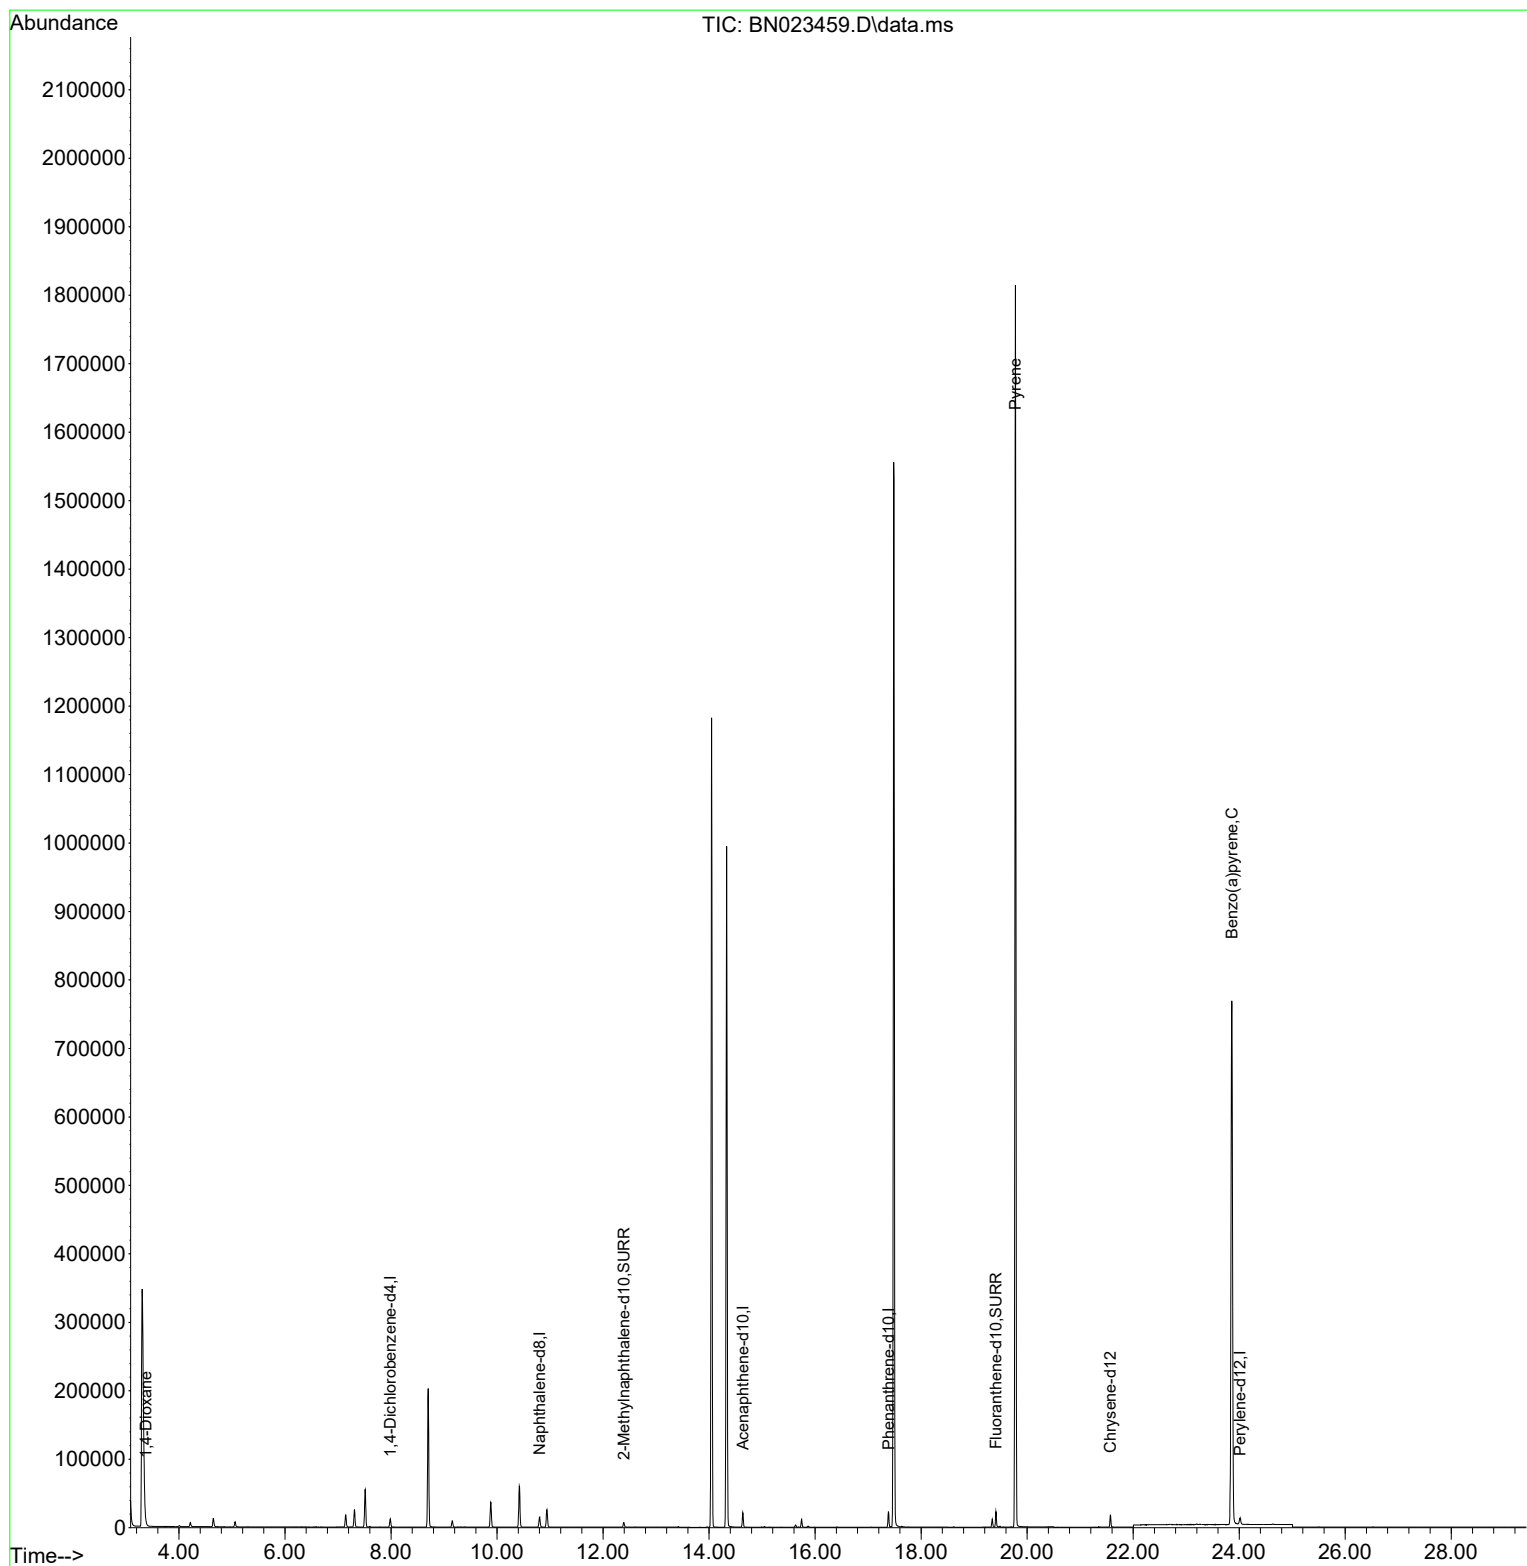


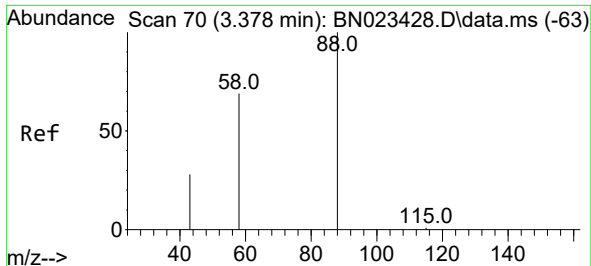

#2
1,4-Dioxane
Concen: 0.111 ng/ul
RT: 3.378 min Scan# 70
Delta R.T. -0.000 min
Lab File: BN023459.D
Acq: 25 Dec 2022 22:07




Instrument :
BNA_N
ClientSampleId :


Tgt Ion: 88 Resp: 720
Ion Ratio Lower Upper
88 100
43 76.3 28.4 42.6#
58 42.0 45.6 68.4#

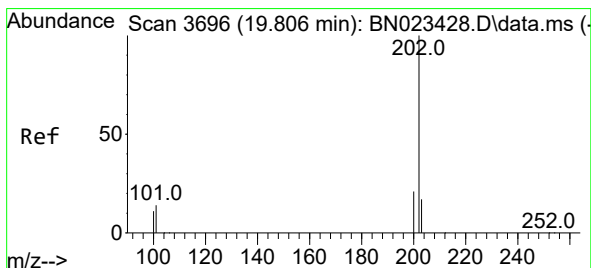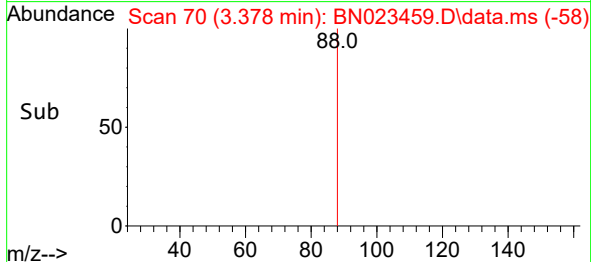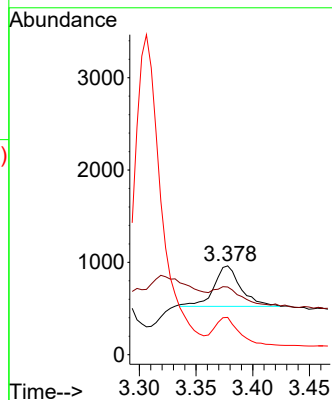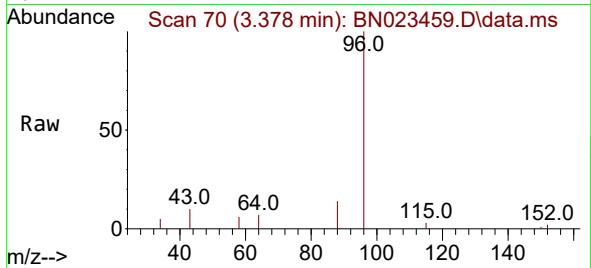

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.778 min Scan# 3690
Delta R.T. -0.028 min
Lab File: BN023459.D
Acq: 25 Dec 2022 22:07


Tgt Ion: 202 Resp: 3116
Ion Ratio Lower Upper
202 100
101 161.6 11.3 16.9#
100 1196.0 9.0 13.4#

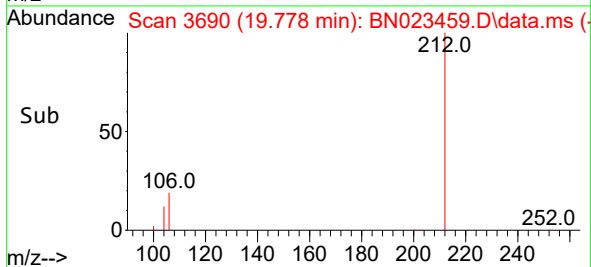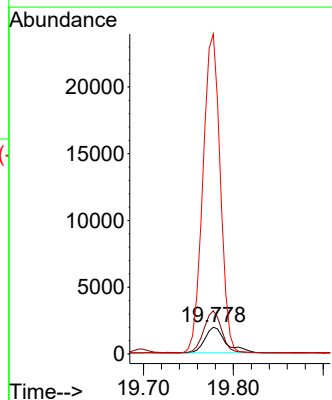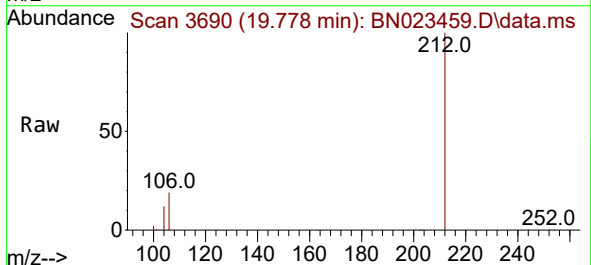

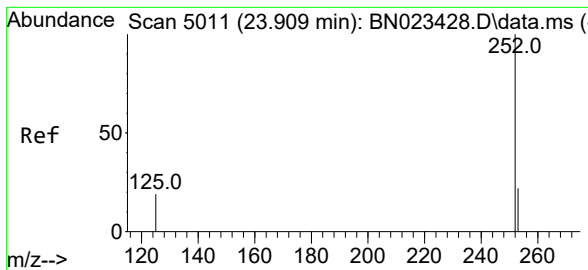

#26
 Benzo(a)pyrene
 Concen: 0.080 ng/ul
 RT: 23.859 min Scan# 4994
 Delta R.T. -0.050 min
 Lab File: BN023459.D
 Acq: 25 Dec 2022 22:07

Instrument :
 BNA_N
 ClientSampleId :

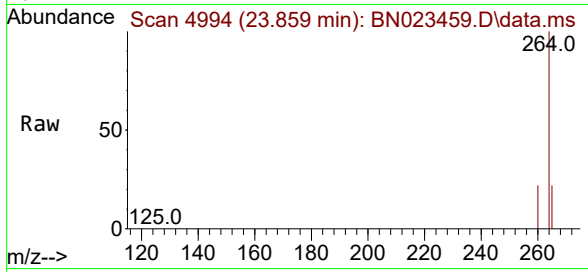

Tgt Ion:252	Resp:	4259
Ion	Ratio	Lower Upper
252	100	
253	49.8	21.4 32.2#
125	48.9	16.2 24.4#

