

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023465.D
 Acq On : 26 Dec 2022 01:43
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 02:58:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	5877	0.400	ng/ul	0.00
4) Naphthalene-d8	10.803	136	19535	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.635	164	11465	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.385	188	25470	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240	15995	0.400	ng/ul	0.00
23) Perylene-d12	24.016	264	13170	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.387	152	10471	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.410	212	24074	0.416	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	908	0.139	ng/ul#	67
20) Pyrene	19.781	202	3149	0.040	ng/ul#	1
26) Benzo(a)pyrene	23.861	252	4498	0.083	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023465.D
Acq On : 26 Dec 2022 01:43
Operator : CG/JU
Sample : N6032-09
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 26 02:58:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

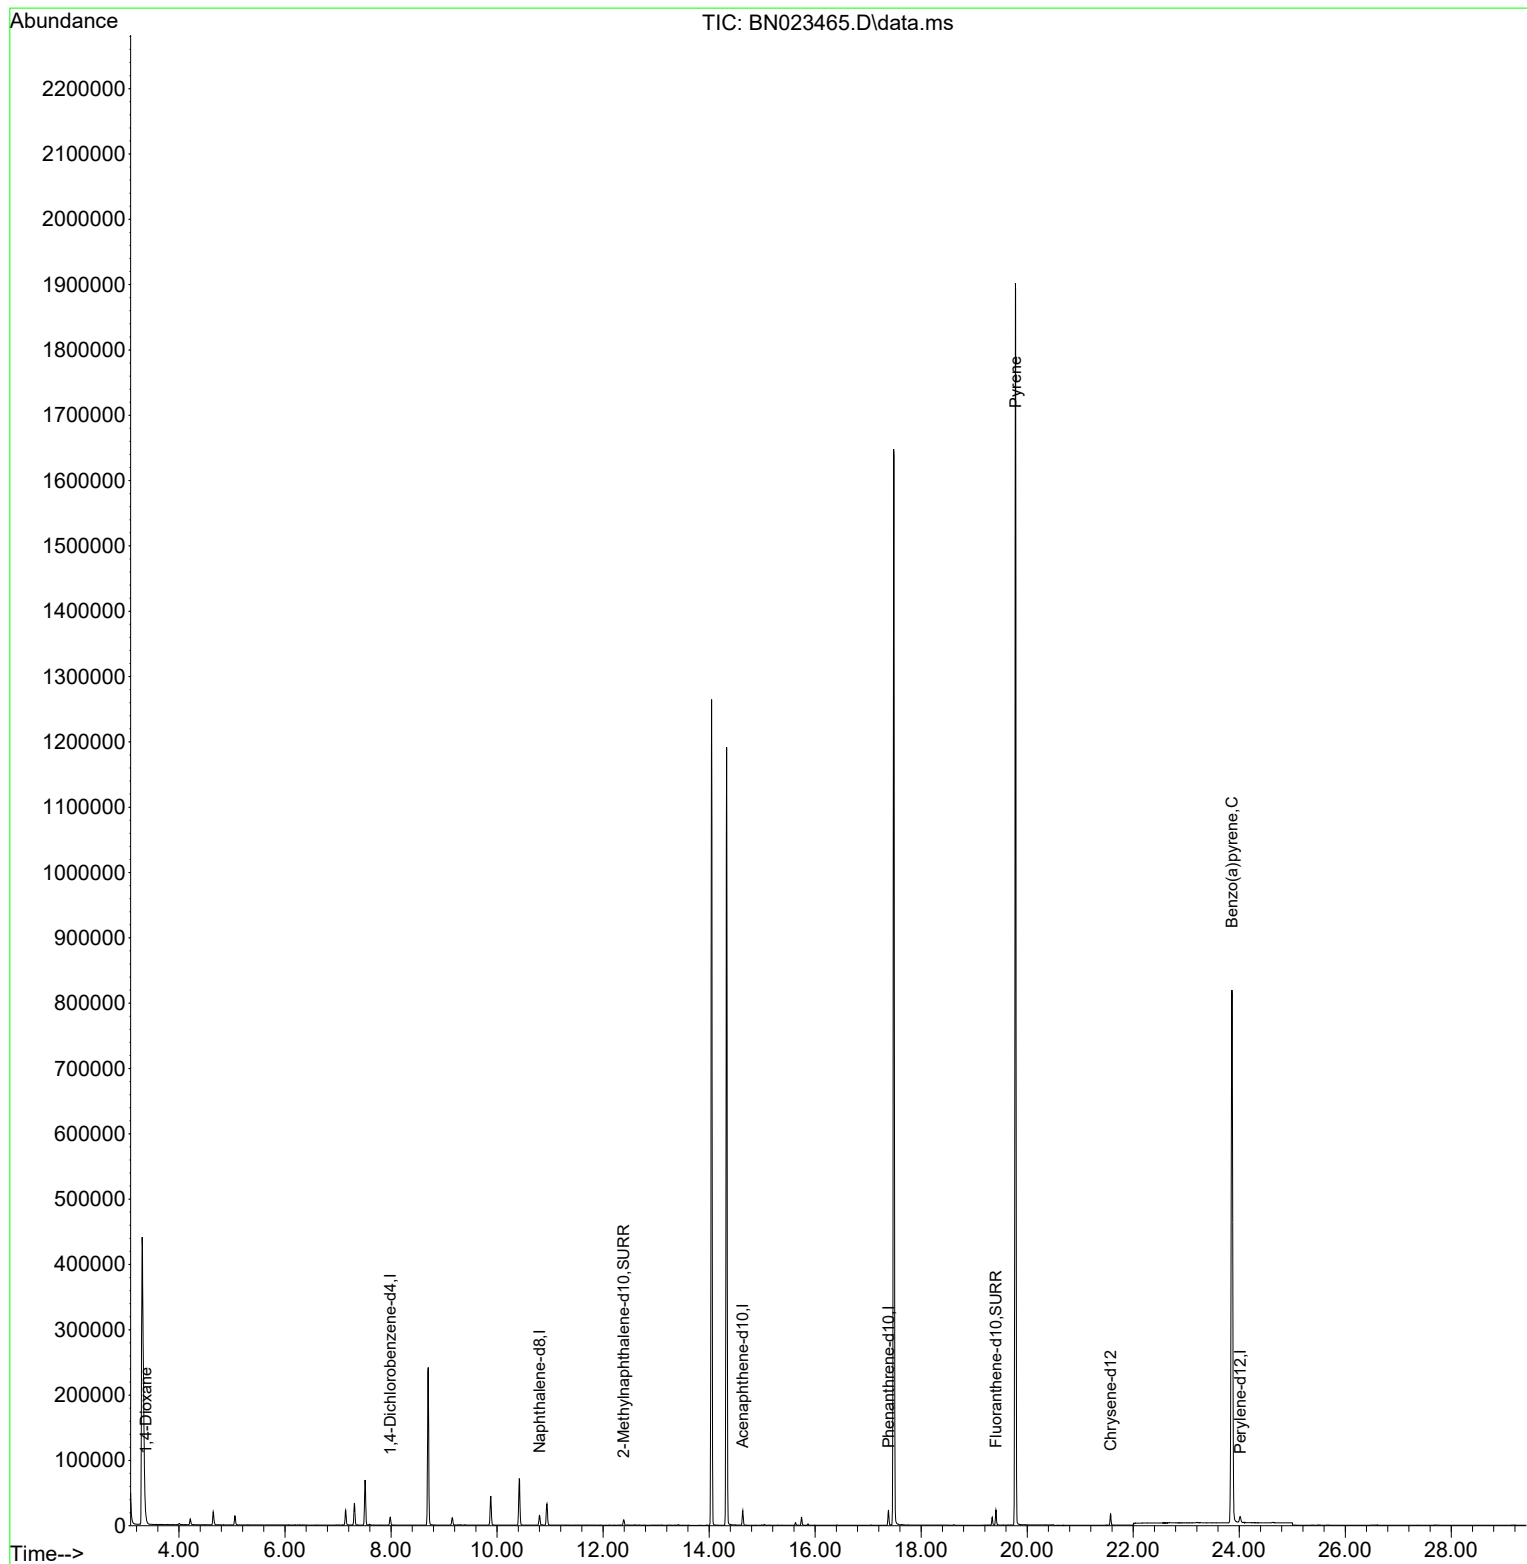



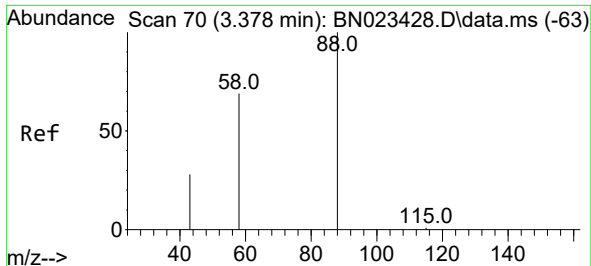


#2
1,4-Dioxane
Concen: 0.139 ng/ul
RT: 3.378 min Scan# 70
Delta R.T. 0.000 min
Lab File: BN023465.D
Acq: 26 Dec 2022 01:43

Instrument :
BNA_N
ClientSampleId :



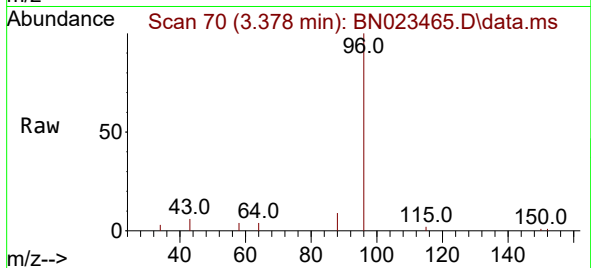



Tgt Ion: 88 Resp: 908
Ion Ratio Lower Upper
88 100
43 67.9 28.4 42.6#
58 42.8 45.6 68.4#

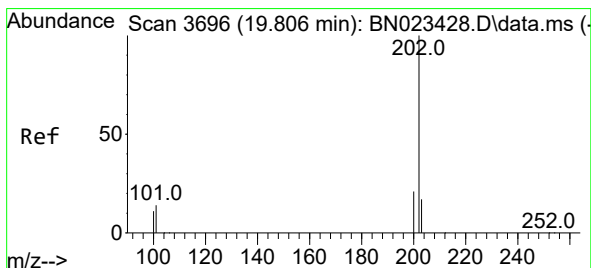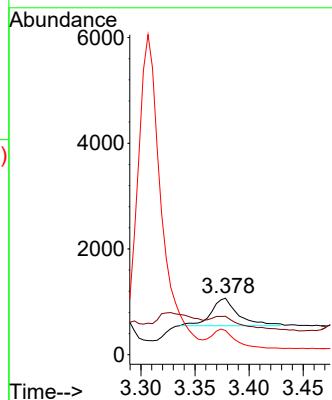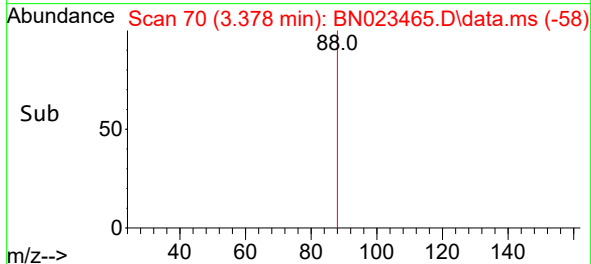

#20
Pyrene
Concen: 0.040 ng/ul
RT: 19.781 min Scan# 3691
Delta R.T. -0.024 min
Lab File: BN023465.D
Acq: 26 Dec 2022 01:43


Tgt Ion: 202 Resp: 3149
Ion Ratio Lower Upper
202 100
101 153.6 11.3 16.9#
100 1091.2 9.0 13.4#

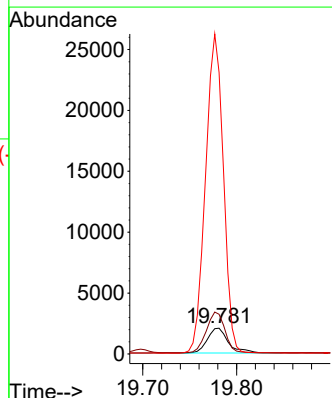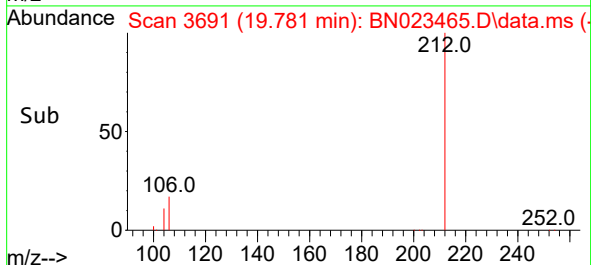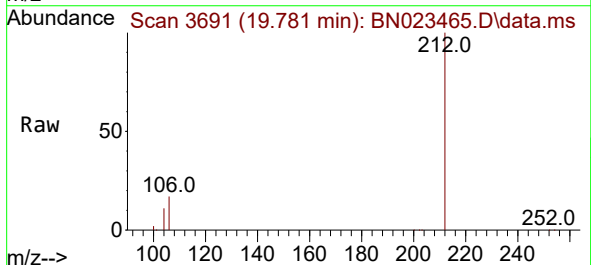

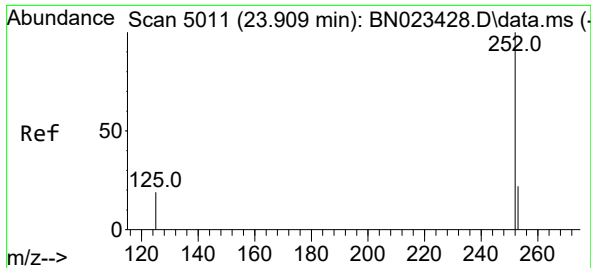

#26
Benzo(a)pyrene
Concen: 0.083 ng/ul
RT: 23.861 min Scan# 4995
Delta R.T. -0.048 min
Lab File: BN023465.D
Acq: 26 Dec 2022 01:43

Instrument :
BNA_N
ClientSampleId :

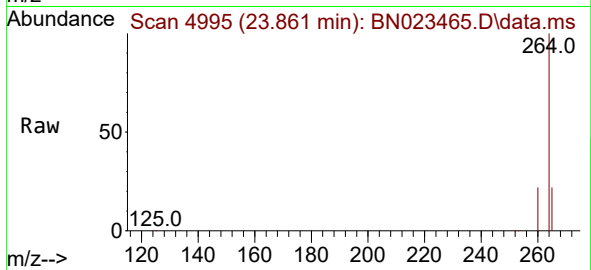

Tgt Ion:252 Resp: 4498
Ion Ratio Lower Upper
252 100
253 47.5 21.4 32.2#
125 45.5 16.2 24.4#

