

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023466.D
 Acq On : 26 Dec 2022 02:19
 Operator : CG/JU
 Sample : N6032-10
 Misc :
 ALS Vial : 102 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Dec 26 02:58:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	6453	0.400	ng/ul	0.00
4) Naphthalene-d8	10.799	136	21402	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	12344	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.382	188	27969	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240	17375	0.400	ng/ul	0.00
23) Perylene-d12	24.016	264	14199	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0	0.000	ng/ul	
6) 2-Methylnaphthalene-d10	12.388	152	9186	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	23114	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	855	0.119	ng/ul#	67
20) Pyrene	19.778	202	2948	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.861	252	4284	0.074	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023466.D
Acq On : 26 Dec 2022 02:19
Operator : CG/JU
Sample : N6032-10
Misc :
ALS Vial : 102 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Dec 26 02:58:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

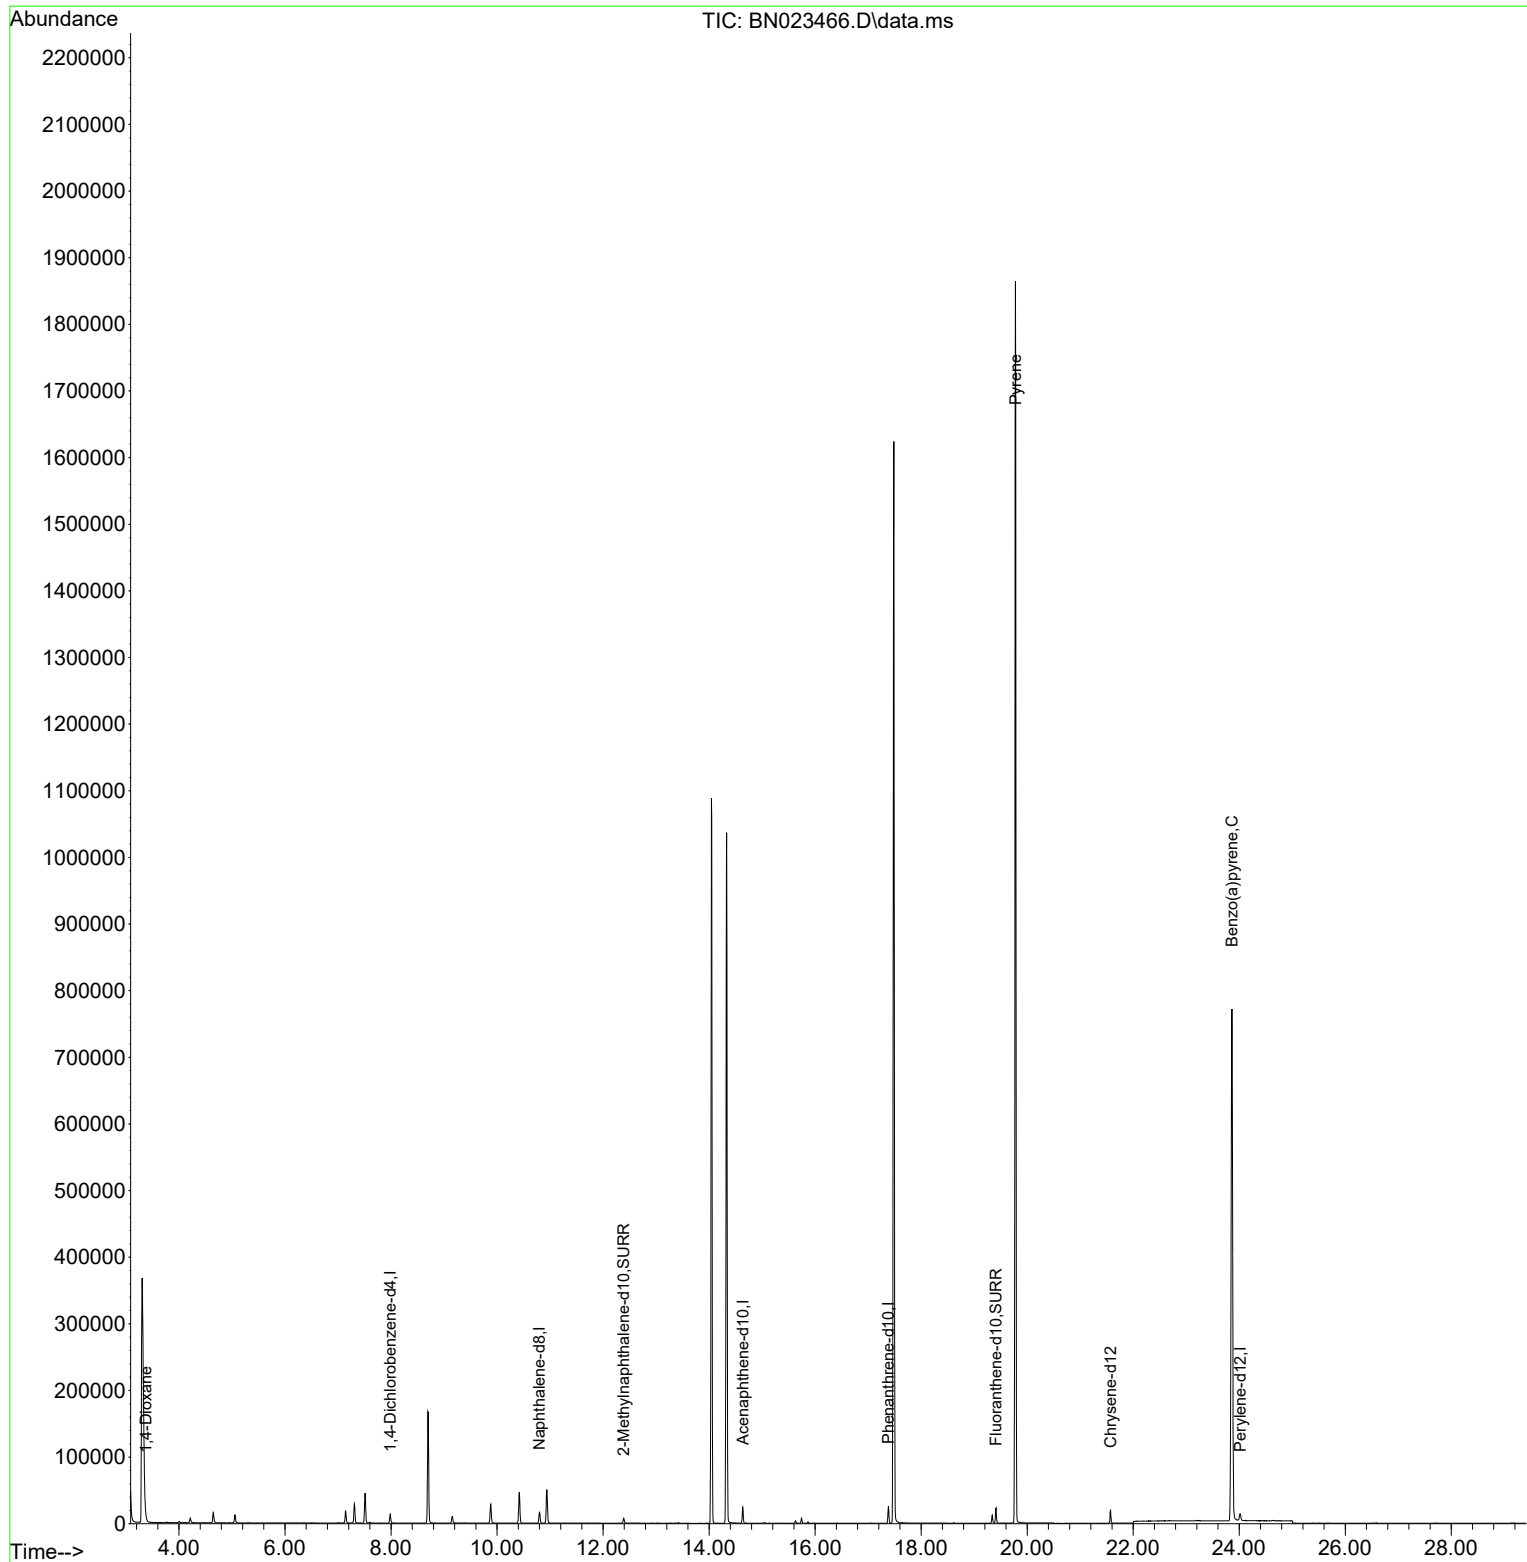



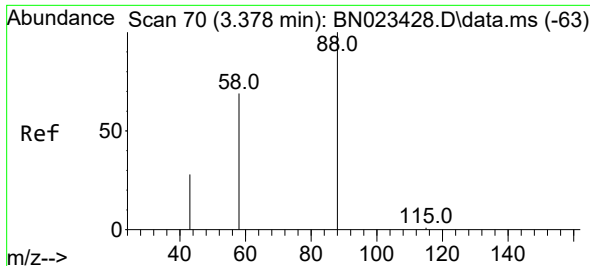


#2
 1,4-Dioxane
 Concen: 0.119 ng/ul
 RT: 3.378 min Scan# 70
 Delta R.T. 0.000 min
 Lab File: BN023466.D
 Acq: 26 Dec 2022 02:19

Instrument :
 BNA_N
 ClientSampleId :



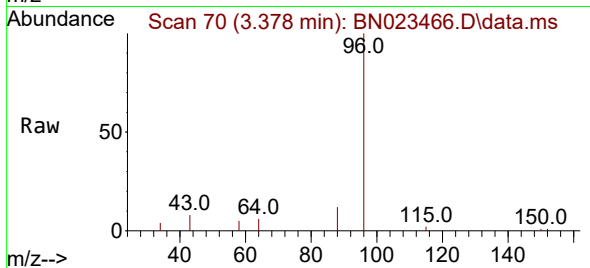



Tgt Ion: 88 Resp: 855
 Ion Ratio Lower Upper
 88 100
 43 63.7 28.4 42.6#
 58 39.3 45.6 68.4#

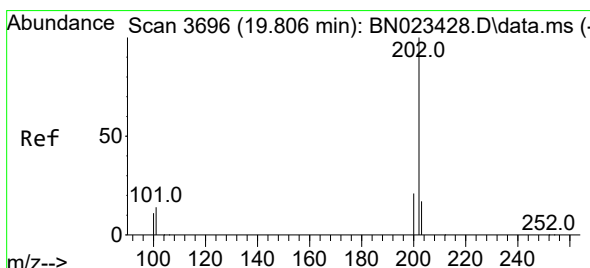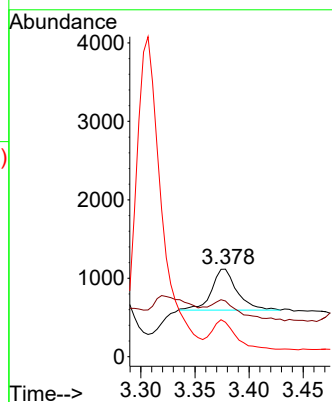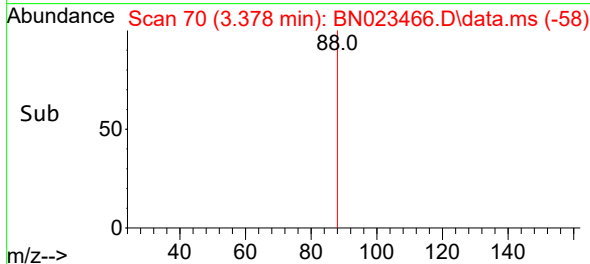

#20
 Pyrene
 Concen: 0.035 ng/ul
 RT: 19.778 min Scan# 3690
 Delta R.T. -0.028 min
 Lab File: BN023466.D
 Acq: 26 Dec 2022 02:19


Tgt Ion: 202 Resp: 2948
 Ion Ratio Lower Upper
 202 100
 101 160.7 11.3 16.9#
 100 1180.5 9.0 13.4#

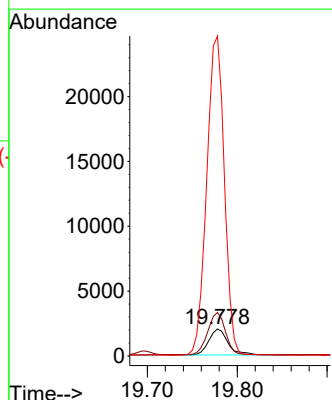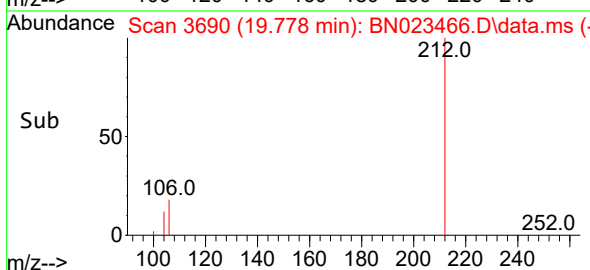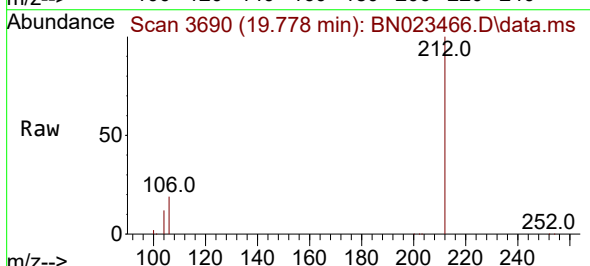

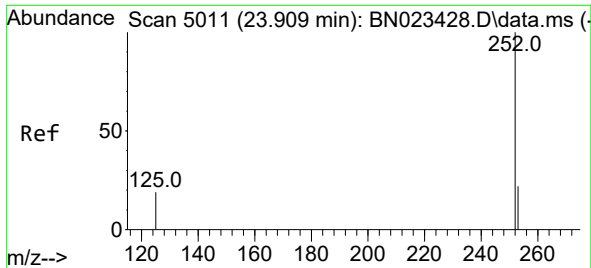

#26
Benzo(a)pyrene
Concen: 0.074 ng/ul
RT: 23.861 min Scan# 4995
Delta R.T. -0.048 min
Lab File: BN023466.D
Acq: 26 Dec 2022 02:19

Instrument :
BNA_N
ClientSampleId :

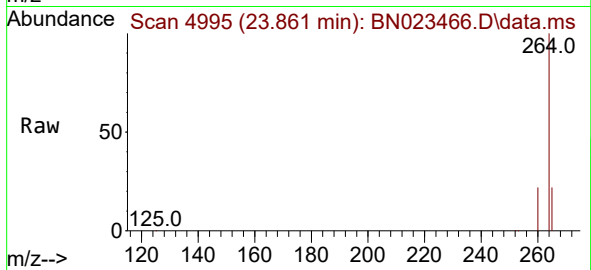

Tgt Ion:252 Resp: 4284
Ion Ratio Lower Upper
252 100
253 48.0 21.4 32.2#
125 46.5 16.2 24.4#

