




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023458.D
Acq On : 25 Dec 2022 21:31
Operator : CG/JU
Sample : N6032-02
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COL85

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

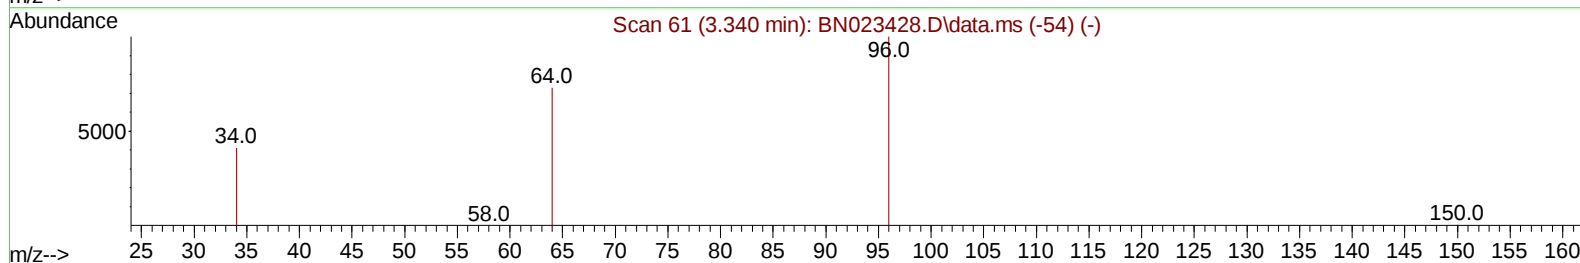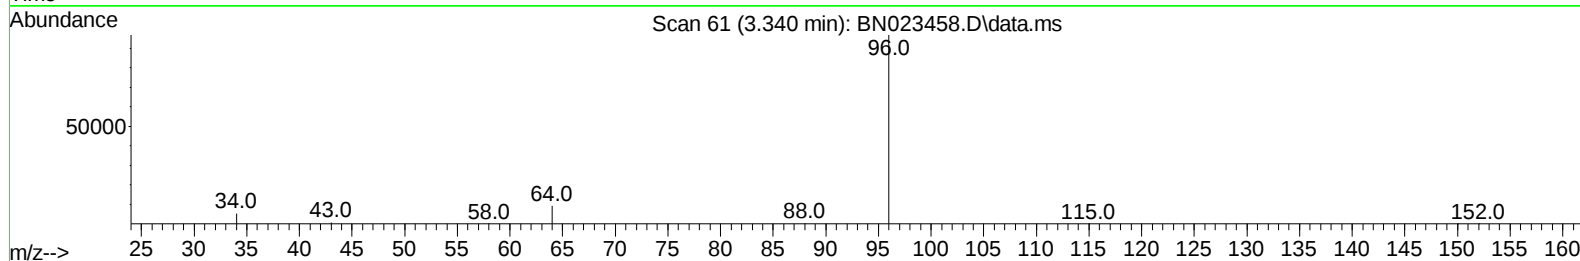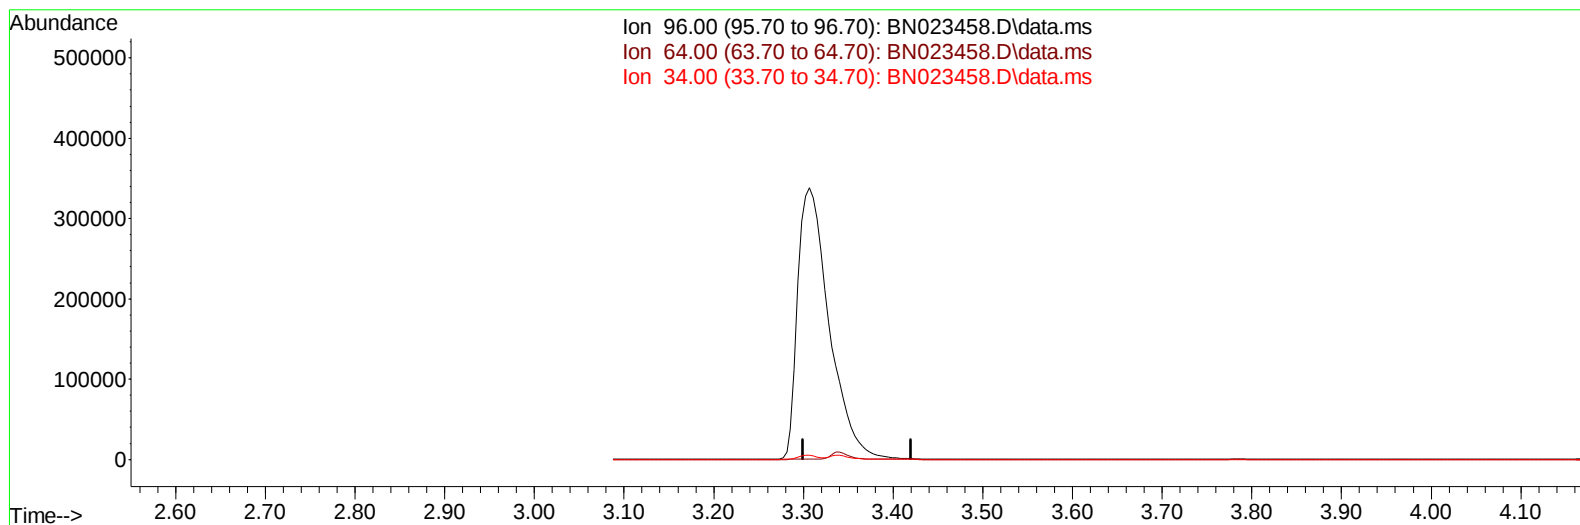

TIC: BN023458.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-3.340) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	61.20	0.00#
34.00	36.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023458.D
 Acq On : 25 Dec 2022 21:31
 Operator : CG/JU
 Sample : N6032-02
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COL85

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

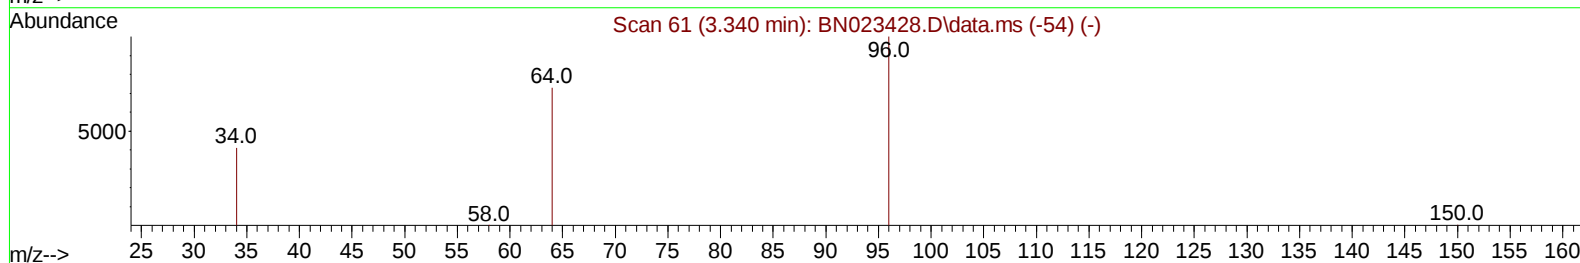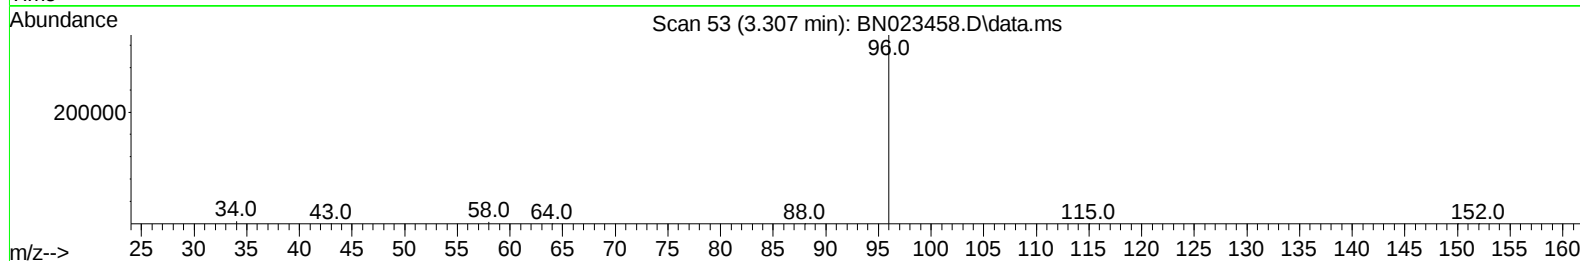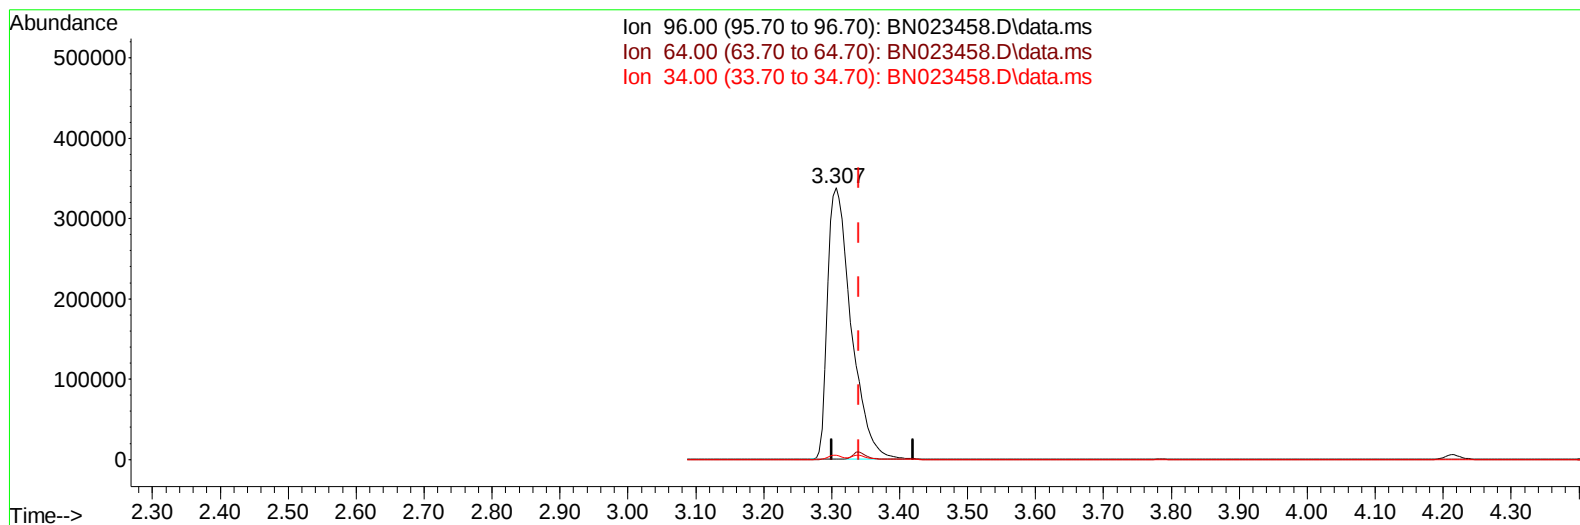

TIC: BN023458.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.307min (-0.034) 132.37 ng/ul m

response 819966

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.20	0.17#
34.00	36.20	1.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023458.D
 Acq On : 25 Dec 2022 21:31
 Operator : CG/JU
 Sample : N6032-02
 Misc :
 ALS Vial : 94 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COL85

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 02:58:00 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.985	152		5701	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136		19050	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164		11037	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.382	188		24833	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240		15807	0.400	ng/ul	0.00
23) Perylene-d12	24.016	264		12868	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.307	96		819966m	132.373	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	12.394	152		8853	0.300	ng/ul	0.00
18) Fluoranthene-d10	19.411	212		21185	0.371	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.378	88		734	0.116	ng/ul#	60

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023458.D
Acq On : 25 Dec 2022 21:31
Operator : CG/JU
Sample : N6032-02
Misc :
ALS Vial : 94 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0L85

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:00 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

