




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023459.D
 Acq On : 25 Dec 2022 22:07
 Operator : CG/JU
 Sample : N6032-03
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COL86

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

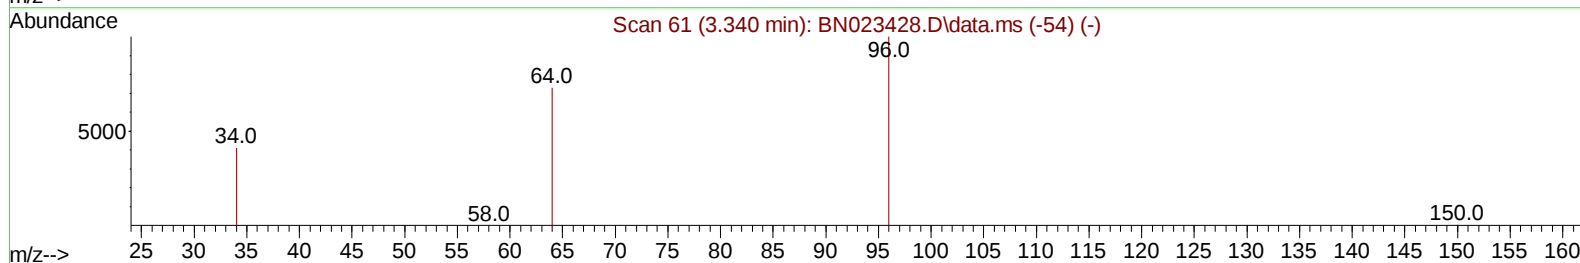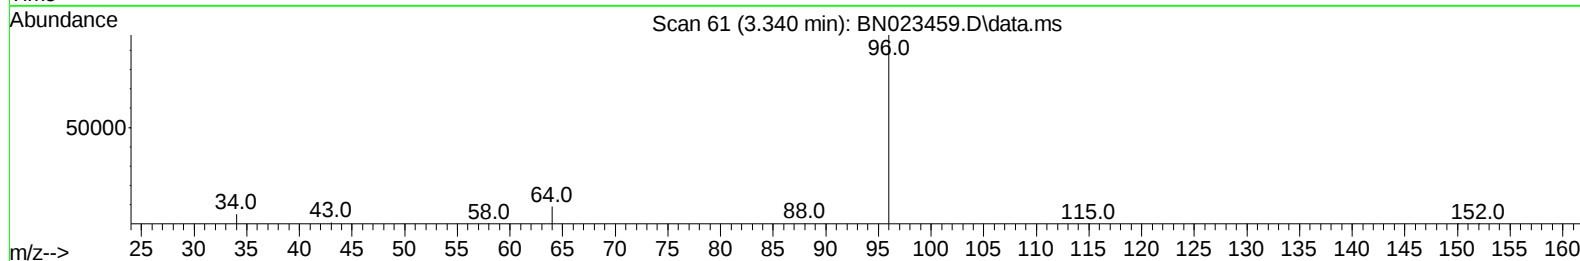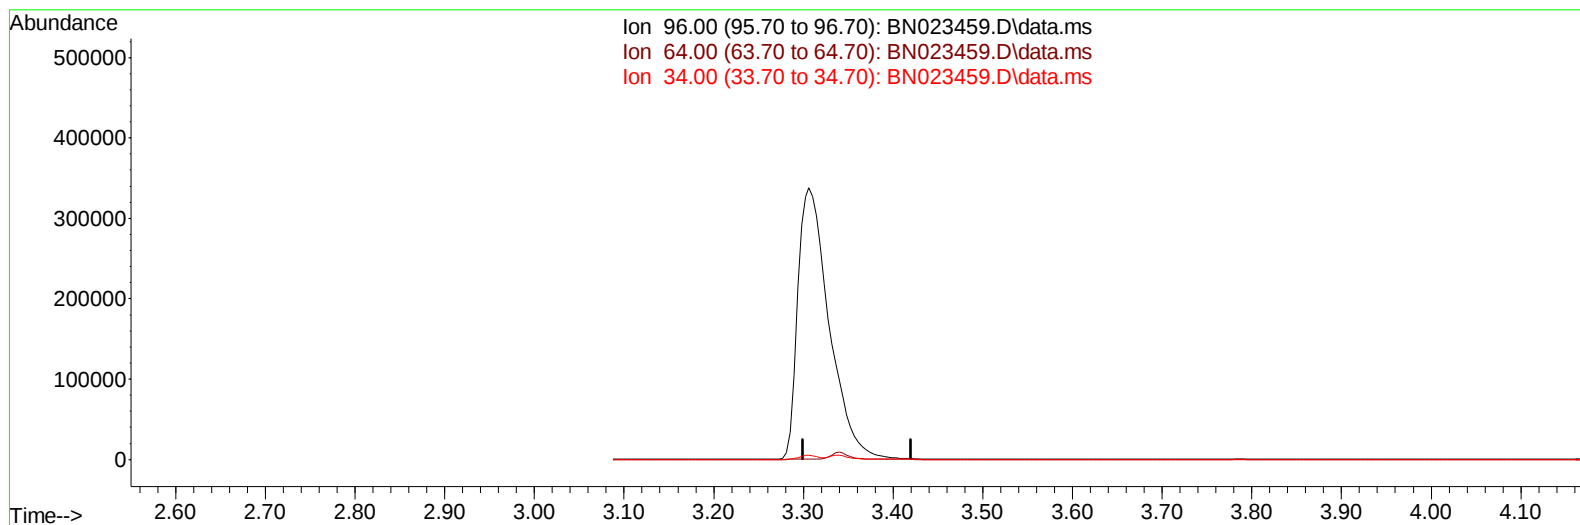

TIC: BN023459.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-3.340) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	61.20	0.00#
34.00	36.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023459.D
Acq On : 25 Dec 2022 22:07
Operator : CG/JU
Sample : N6032-03
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COL86

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 02:58:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

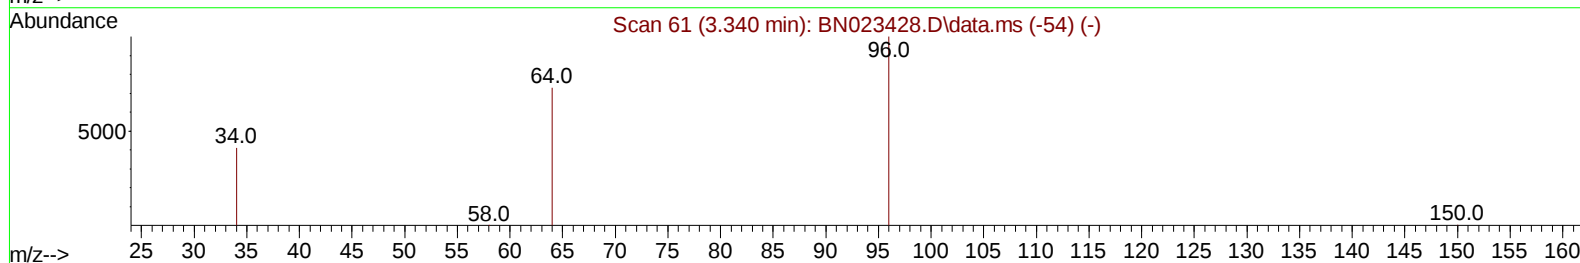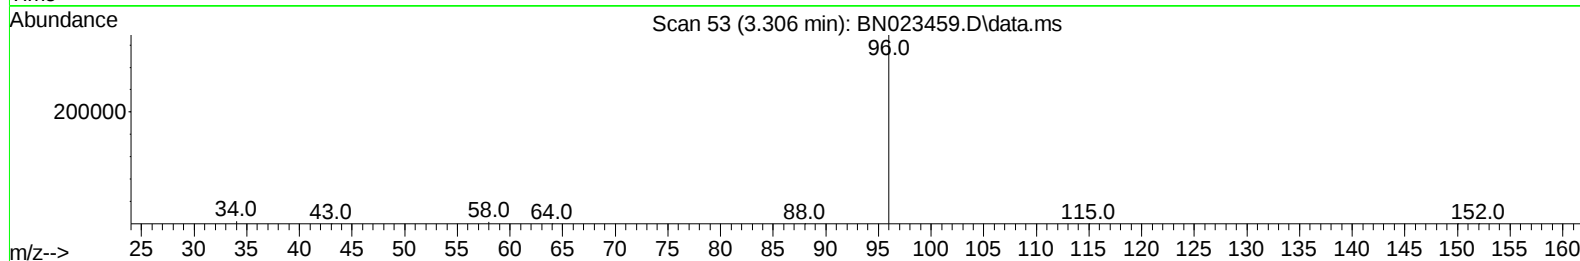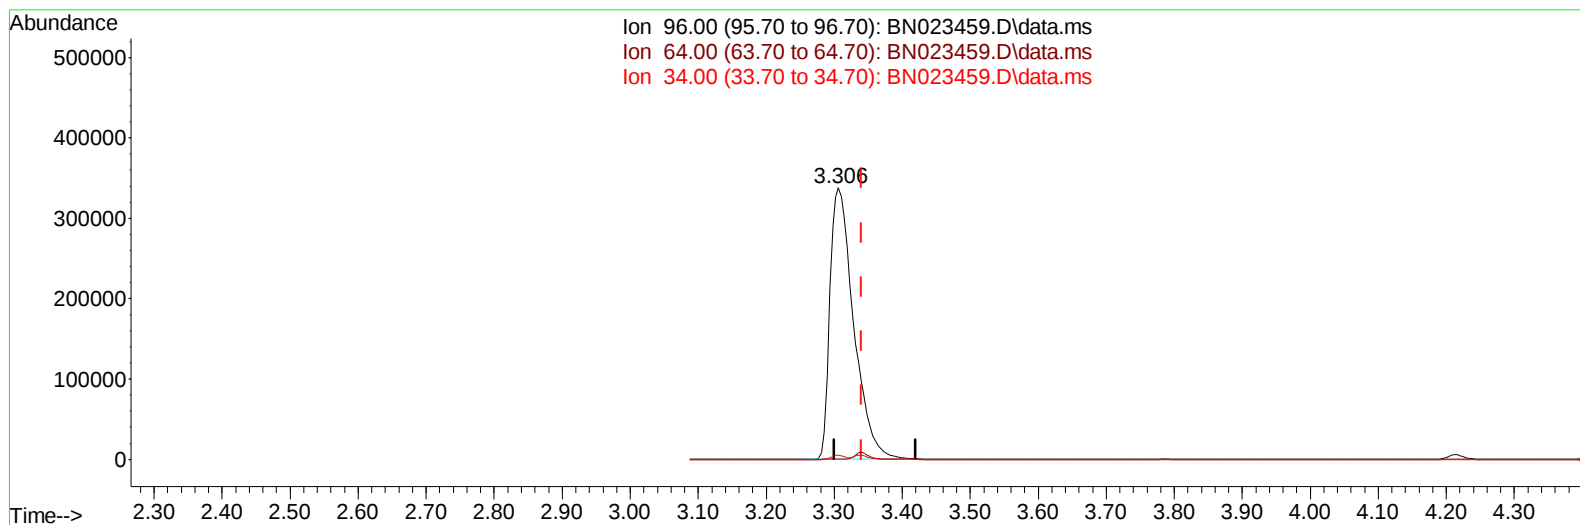

TIC: BN023459.D\data.ms

(3) 1,4-Dioxane-d8 (S)**3.306min (-0.034) 129.29 ng/ul m****response 820563**

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.20	0.17#
34.00	36.20	1.56#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023459.D
 Acq On : 25 Dec 2022 22:07
 Operator : CG/JU
 Sample : N6032-03
 Misc :
 ALS Vial : 95 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COL86

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 02:58:06 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.985	152		5841	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136		19424	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164		11121	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188		25181	0.400	ng/ul	0.00
17) Chrysene-d12	21.570	240		15818	0.400	ng/ul	0.00
23) Perylene-d12	24.014	264		13039	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.306	96		820563m	129.294	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	12.393	152		8405	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.411	212		22601	0.395	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.378	88		720	0.111	ng/ul#	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023459.D
Acq On : 25 Dec 2022 22:07
Operator : CG/JU
Sample : N6032-03
Misc :
ALS Vial : 95 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COL86

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:06 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

