




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023465.D
 Acq On : 26 Dec 2022 01:43
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLA1

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

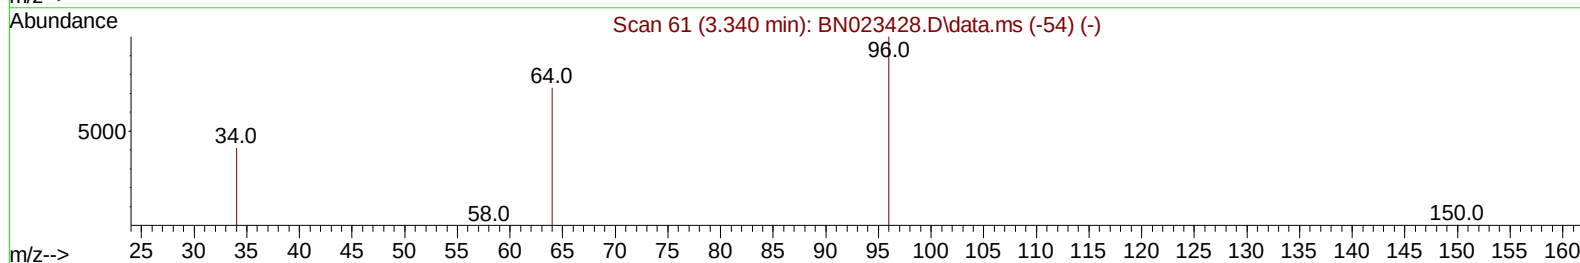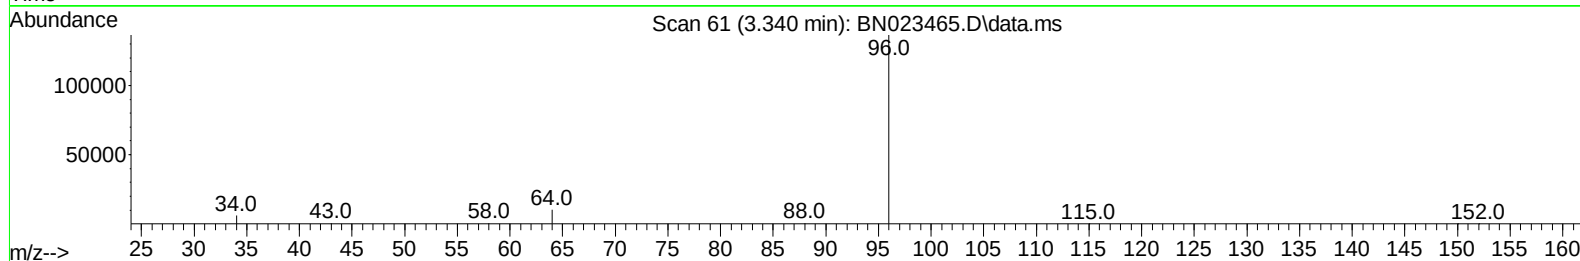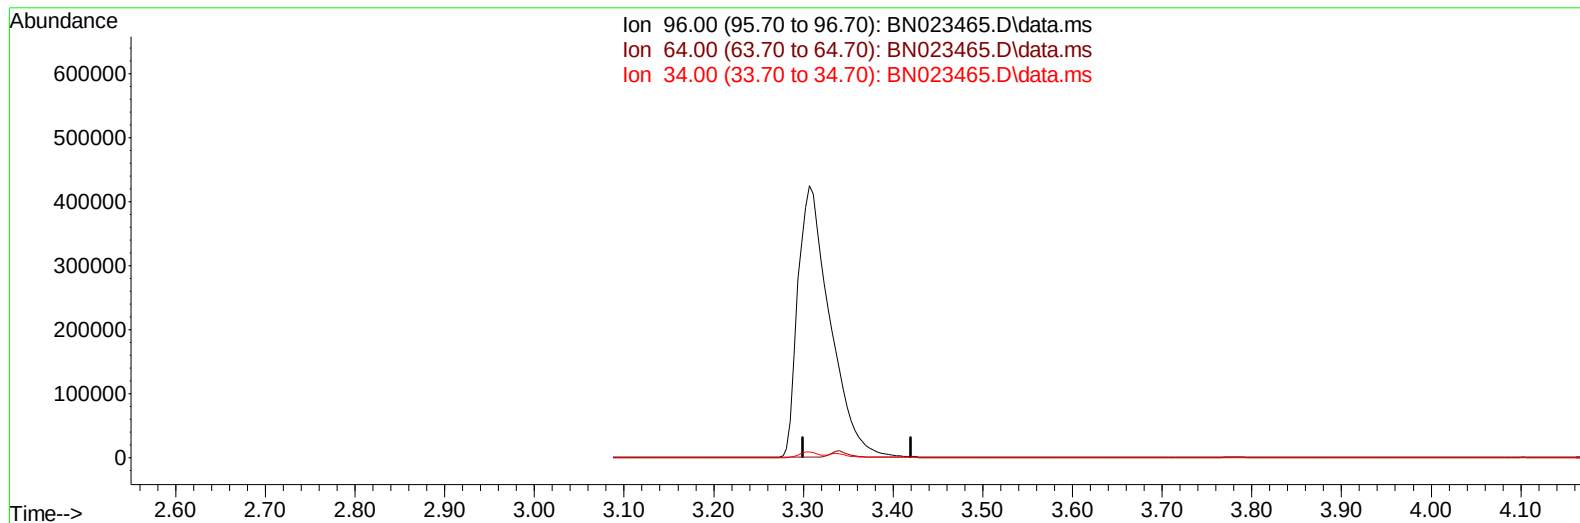

TIC: BN023465.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-3.340) 0.00 ng/ul

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	61.20	0.00#
34.00	36.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023465.D
Acq On : 26 Dec 2022 01:43
Operator : CG/JU
Sample : N6032-09
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLA1

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

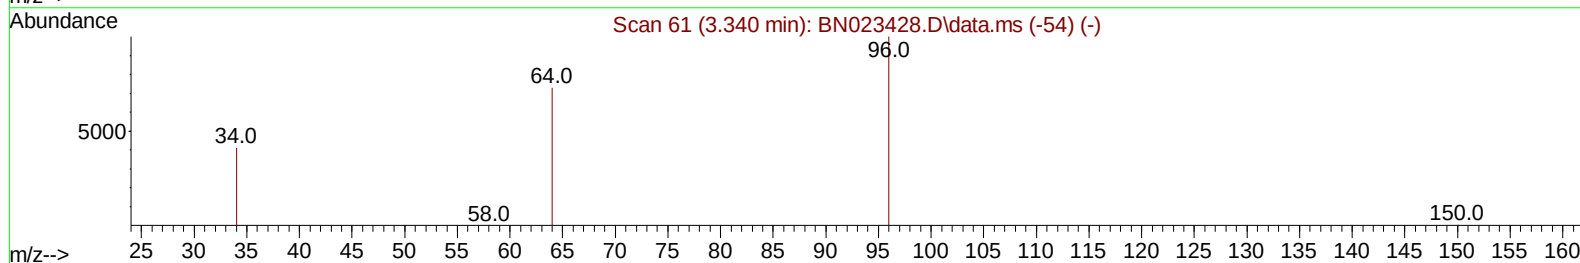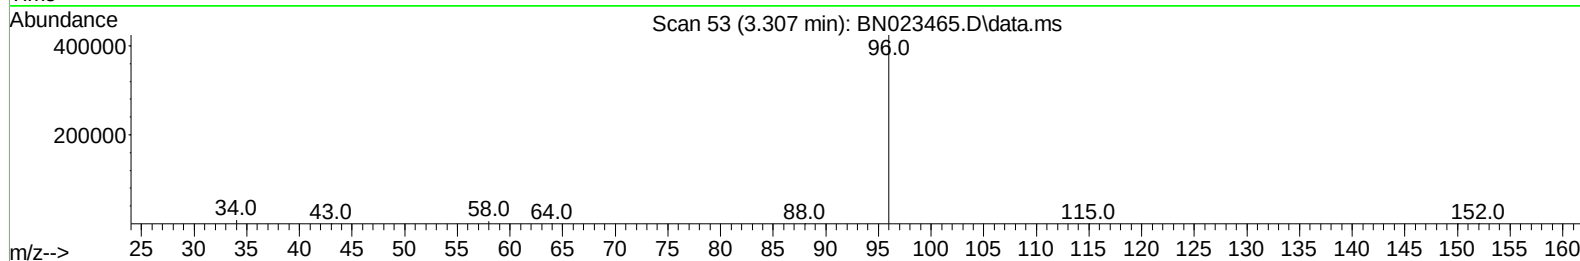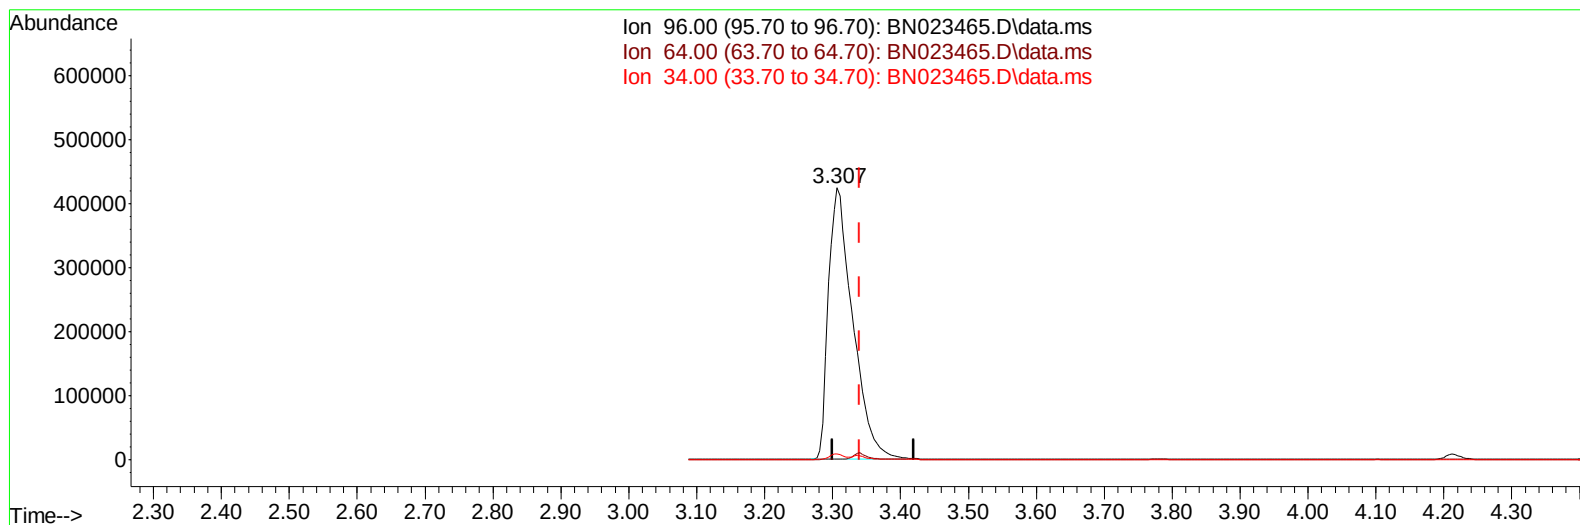

TIC: BN023465.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.307min (-0.034) 164.59 ng/ul m

response 1051006

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.20	0.20#
34.00	36.20	2.14#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023465.D
 Acq On : 26 Dec 2022 01:43
 Operator : CG/JU
 Sample : N6032-09
 Misc :
 ALS Vial : 101 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLA1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 02:58:42 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.985	152		5877	0.400	ng/ul	0.00
4) Naphthalene-d8	10.803	136		19535	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.635	164		11465	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.385	188		25470	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240		15995	0.400	ng/ul	0.00
23) Perylene-d12	24.016	264		13170	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.307	96	1051006m		164.590	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	12.387	152		10471	0.347	ng/ul	0.00
18) Fluoranthene-d10	19.410	212		24074	0.416	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.378	88		908	0.139	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023465.D
Acq On : 26 Dec 2022 01:43
Operator : CG/JU
Sample : N6032-09
Misc :
ALS Vial : 101 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LA1

Manual IntegrationsAPPROVED

Quant Time: Dec 26 02:58:42 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

