




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023469.D
Acq On : 26 Dec 2022 04:06
Operator : CG/JU
Sample : N0032-13
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLB7

Manual IntegrationsAPPROVED

Quant Time: Dec 26 04:40:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

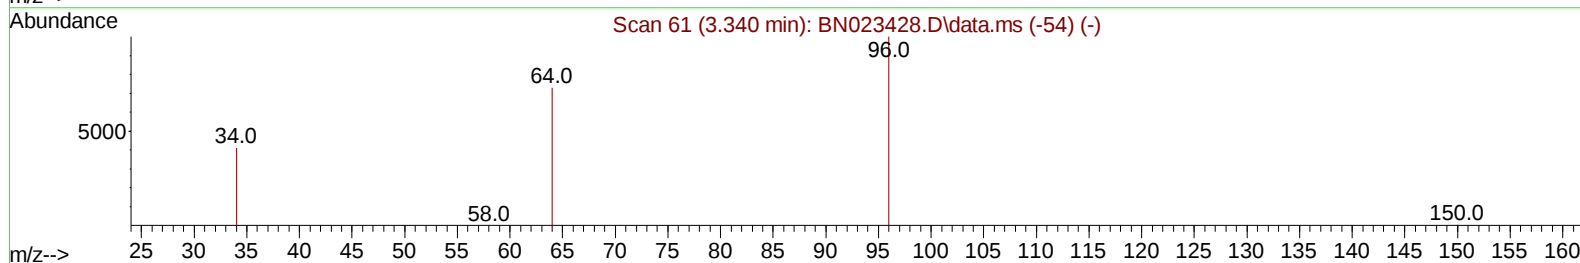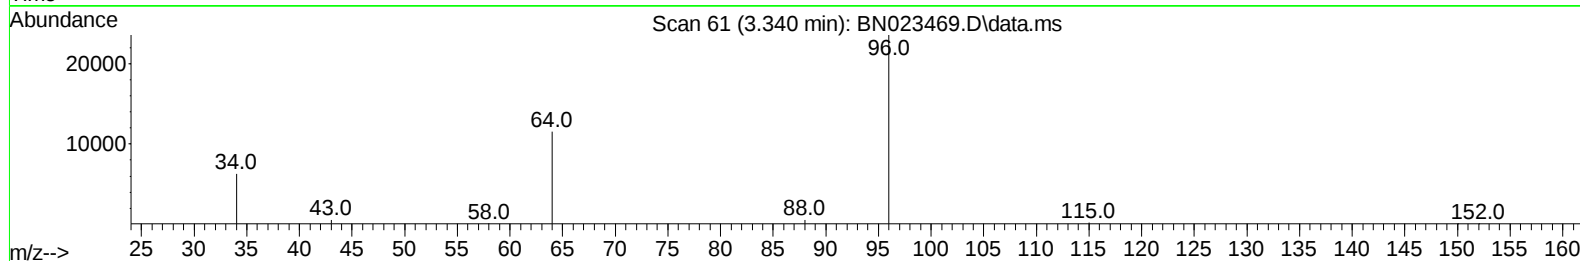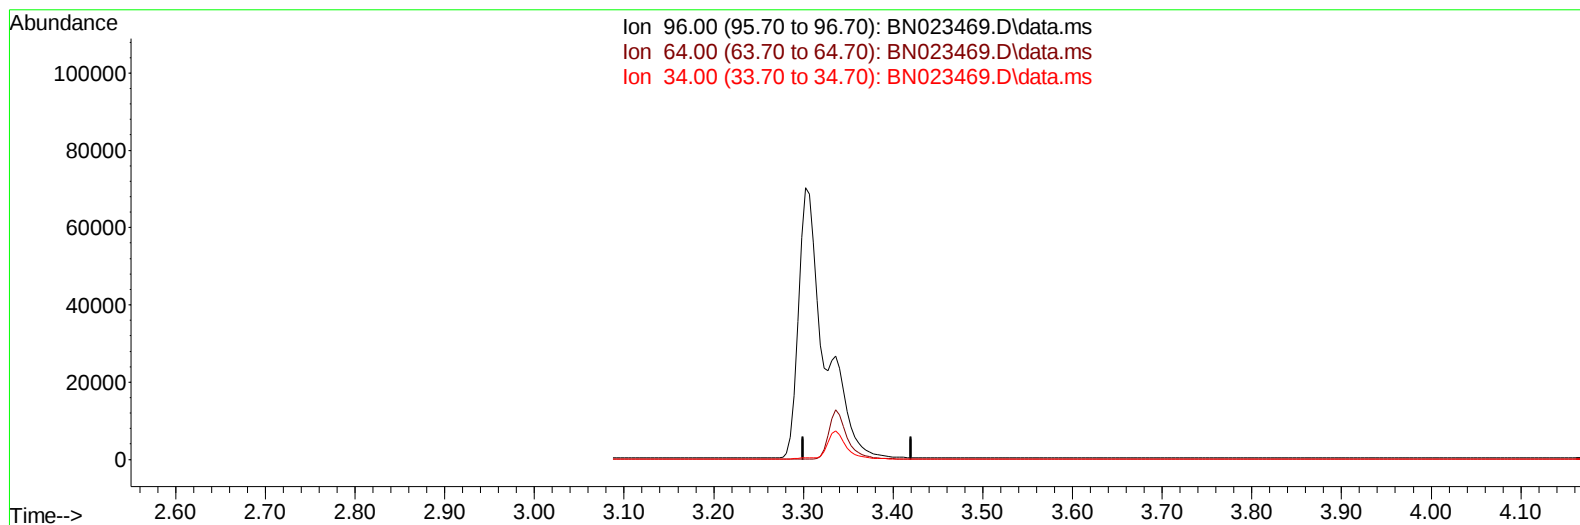

TIC: BN023469.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.340min (-3.340) 0.00 ng/u1

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	61.20	0.00#
34.00	36.20	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023469.D
Acq On : 26 Dec 2022 04:06
Operator : CG/JU
Sample : N0032-13
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COLB7

Manual IntegrationsAPPROVED

Quant Time: Dec 26 04:40:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

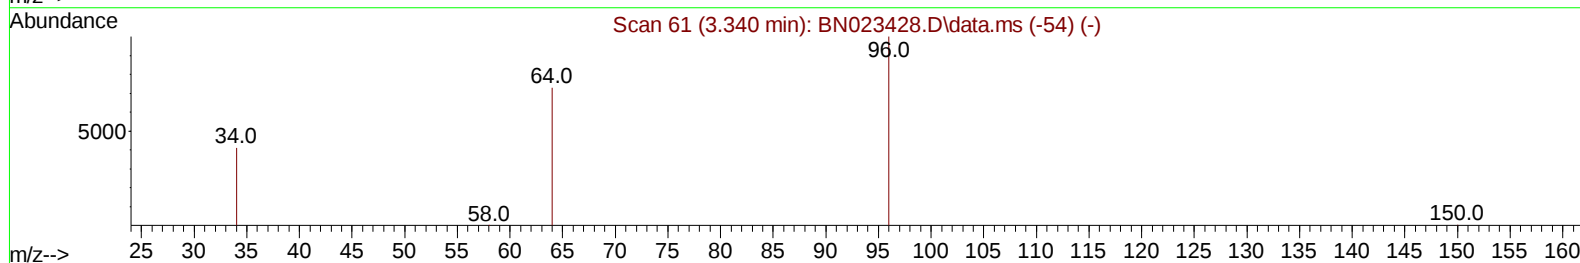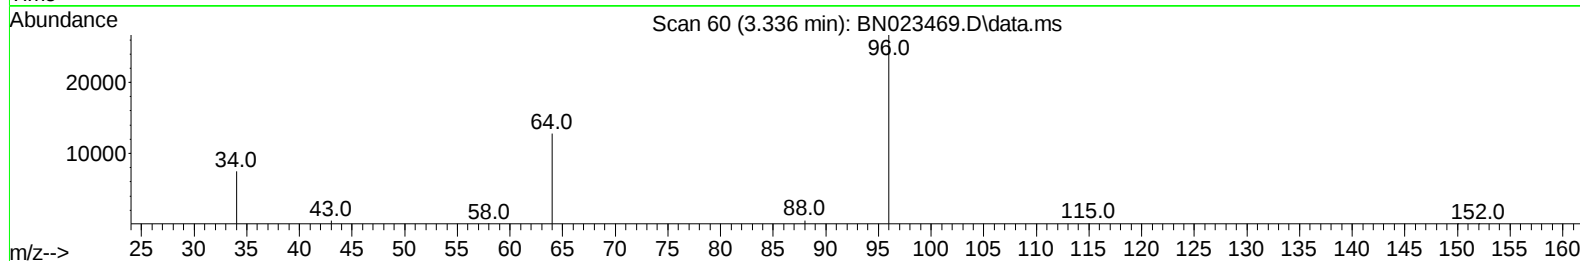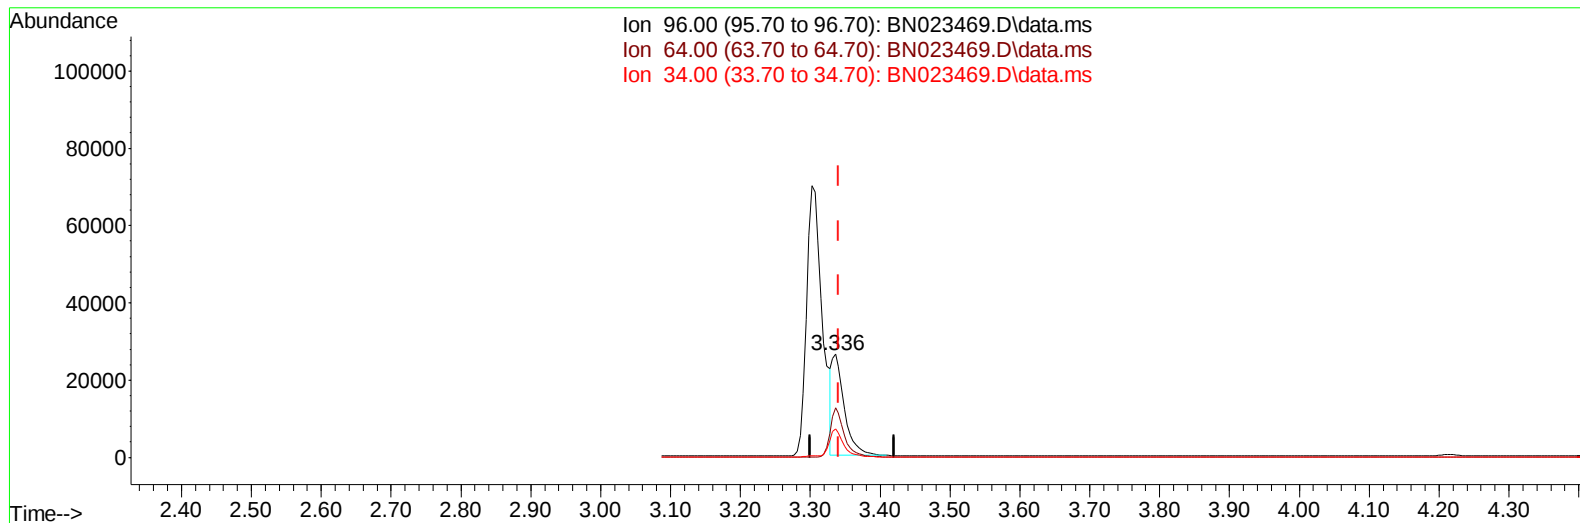

TIC: BN023469.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.336min (-0.004) 5.00 ng/ul m

response 32608

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.20	47.91#
34.00	36.20	27.92#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023469.D
 Acq On : 26 Dec 2022 04:06
 Operator : CG/JU
 Sample : N6032-13
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLB7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 04:40:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.985	152		5998	0.400	ng/ul	0.00
4) Naphthalene-d8	10.799	136		20072	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164		11723	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.382	188		26390	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240		16364	0.400	ng/ul	0.00
23) Perylene-d12	24.013	264		13559	0.400	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.336	96		32608m	5.003	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.388	152		8272	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.411	212		20876	0.353	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.374	88		985	0.148	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023469.D
Acq On : 26 Dec 2022 04:06
Operator : CG/JU
Sample : N6032-13
Misc :
ALS Vial : 105 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0LB7

Manual IntegrationsAPPROVED

Quant Time: Dec 26 04:40:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022

