

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023457.D
 Acq On : 25 Dec 2022 20:55
 Operator : CG/JU
 Sample : N6032-01
 Misc :
 ALS Vial : 93 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COL84

Quant Time: Dec 26 02:57:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	6385	0.400	ng/ul	0.00
4) Naphthalene-d8	10.804	136	21150	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	12077	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.386	188	26906	0.400	ng/ul	0.00
17) Chrysene-d12	21.571	240	15834	0.400	ng/ul	0.00
23) Perylene-d12	24.017	264	13007	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	27664	3.988	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.393	152	5502	0.168	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	14294	0.250	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	942	0.133	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023457.D
Acq On : 25 Dec 2022 20:55
Operator : CG/JU
Sample : N6032-01
Misc :
ALS Vial : 93 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COL84


Quant Time: Dec 26 02:57:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

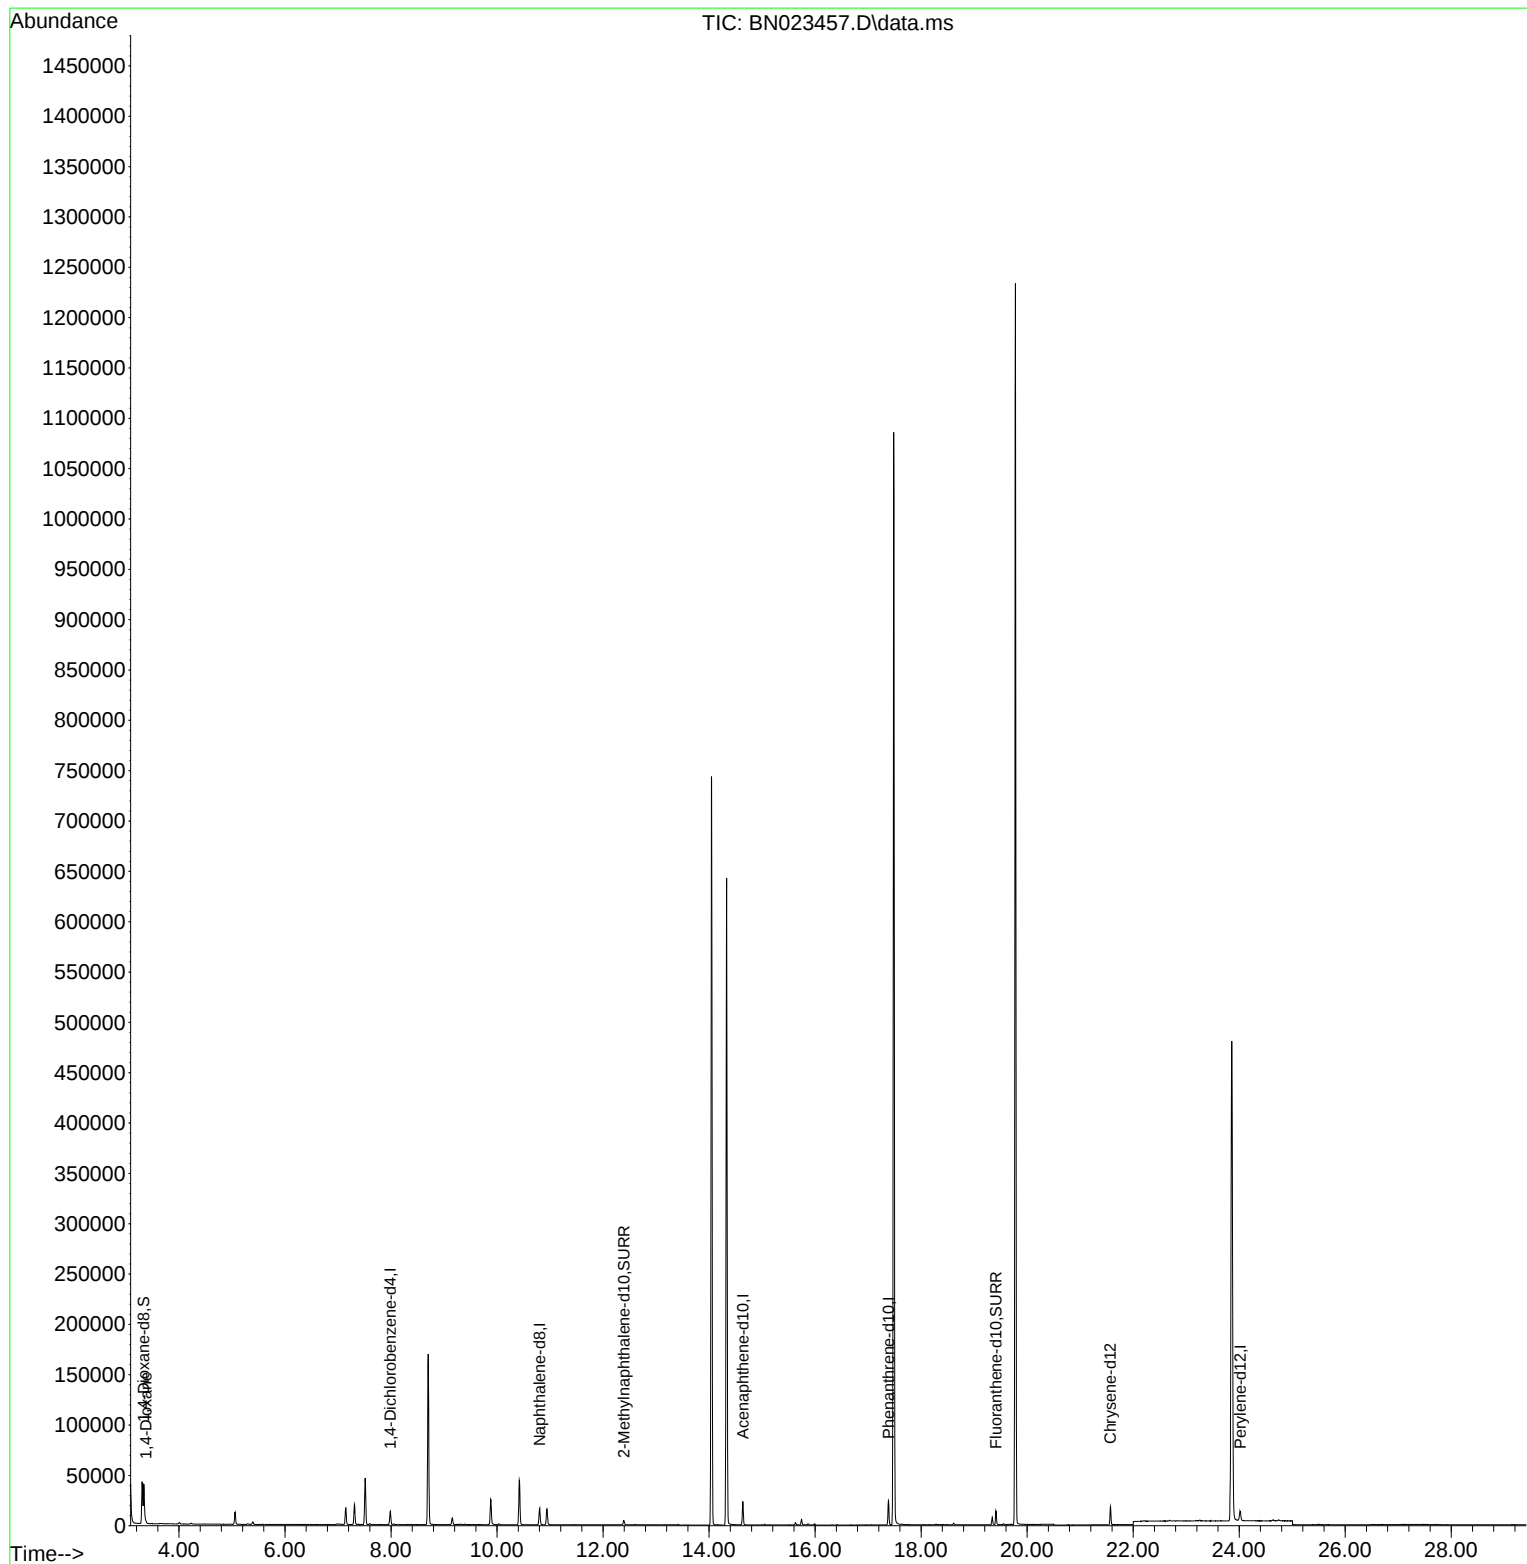

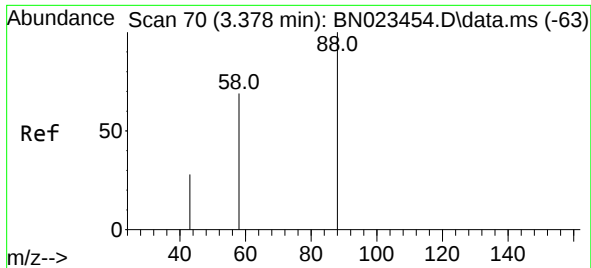

#2
 1,4-Dioxane
 Concen: 0.133 ng/ul
 RT: 3.378 min Scan# 70
 Delta R.T. -0.000 min
 Lab File: BN023457.D
 Acq: 25 Dec 2022 20:55

Instrument :
 BNA_N
 ClientSampleId :
 COL84

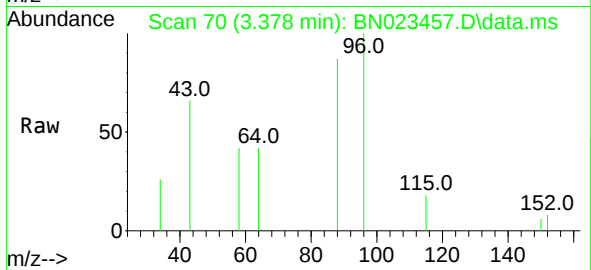

Tgt Ion:	88	Resp:	942
Ion	Ratio	Lower	Upper
88	100		
43	76.1	28.4	42.6#
58	47.5	45.6	68.4

