

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023462.D
 Acq On : 25 Dec 2022 23:55
 Operator : CG/JU
 Sample : N6032-06
 Misc :
 ALS Vial : 98 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0L89

Quant Time: Dec 26 02:58:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	5537	0.400	ng/ul	0.00
4) Naphthalene-d8	10.799	136	18171	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	10875	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.382	188	25036	0.400	ng/ul	0.00
17) Chrysene-d12	21.569	240	16817	0.400	ng/ul	# 0.00
23) Perylene-d12	24.016	264	13731	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	23830	3.961	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.388	152	8957	0.319	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	23331	0.384	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.374	88	1149	0.187	ng/ul#	71


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023462.D
Acq On : 25 Dec 2022 23:55
Operator : CG/JU
Sample : N6032-06
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
COL89


Quant Time: Dec 26 02:58:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

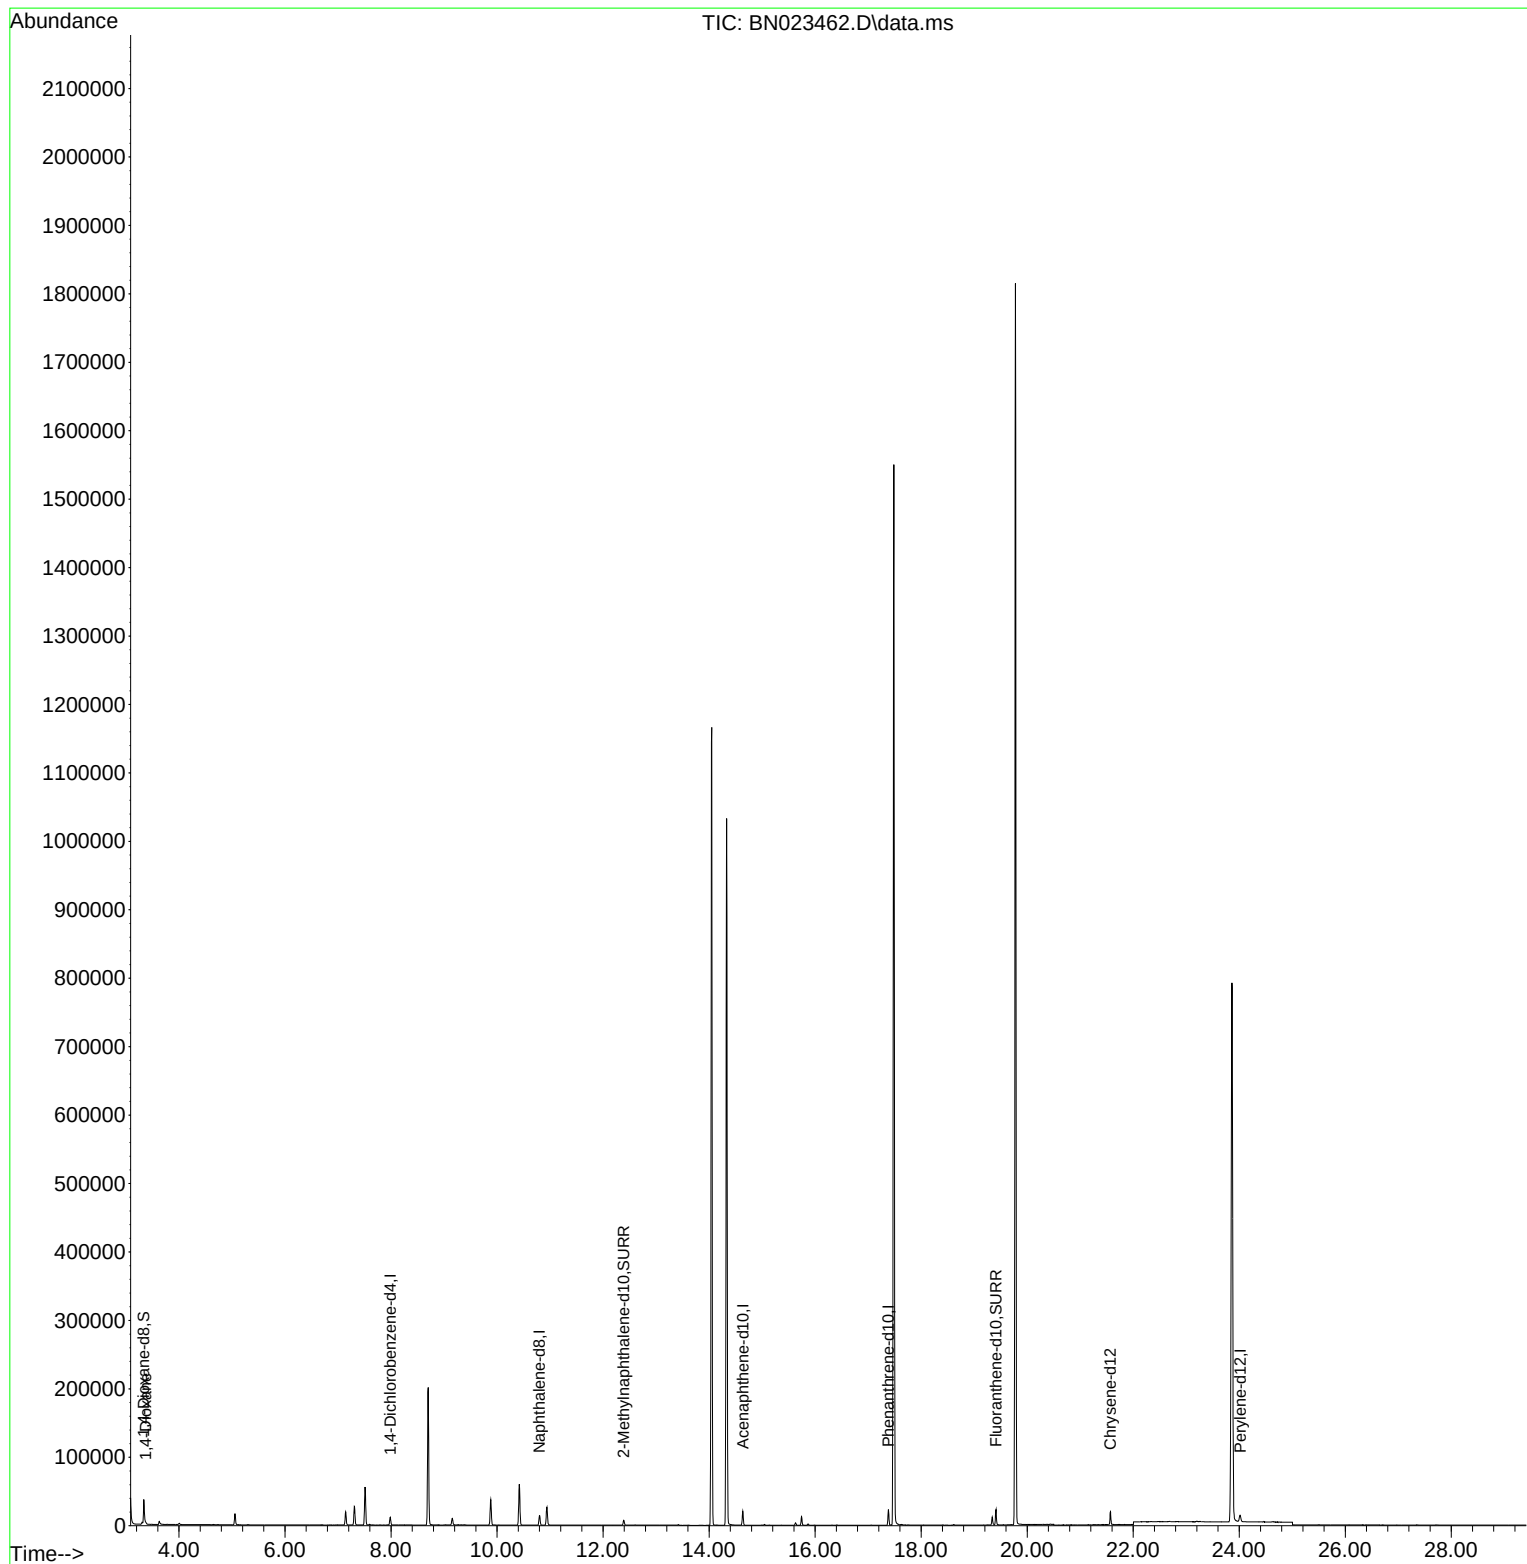

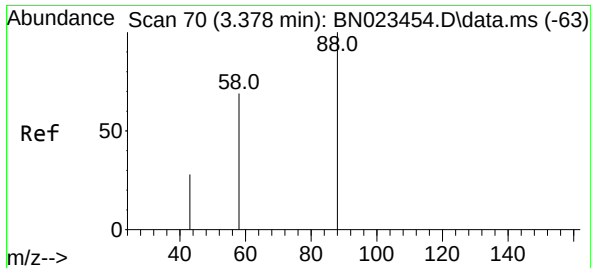

#2
 1,4-Dioxane
 Concen: 0.187 ng/ul
 RT: 3.374 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN023462.D
 Acq: 25 Dec 2022 23:55

Instrument :
 BNA_N
 ClientSampleId :
 COL89

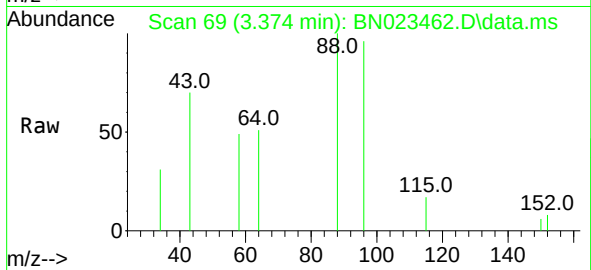

Tgt Ion: 88 Resp: 1149

Ion	Ratio	Lower	Upper
88	100		
43	69.7	28.4	42.6#
58	49.1	45.6	68.4

