

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023466.D
 Acq On : 26 Dec 2022 02:19
 Operator : CG/JU
 Sample : N6032-10
 Misc :
 ALS Vial : 102 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLA3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 02:58:48 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.985	152	6453	0.400	ng/ul	0.00
4) Naphthalene-d8	10.799	136	21402	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.636	164	12344	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.382	188	27969	0.400	ng/ul	0.00
17) Chrysene-d12	21.572	240	17375	0.400	ng/ul	0.00
23) Perylene-d12	24.016	264	14199	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.307	96	900930m	128.494	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	12.388	152	9186	0.277	ng/ul	0.00
18) Fluoranthene-d10	19.411	212	23114	0.368	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.378	88	855	0.119	ng/ul#	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023466.D
Acq On : 26 Dec 2022 02:19
Operator : CG/JU
Sample : N6032-10
Misc :
ALS Vial : 102 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
COLA3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022


Quant Time: Dec 26 02:58:48 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

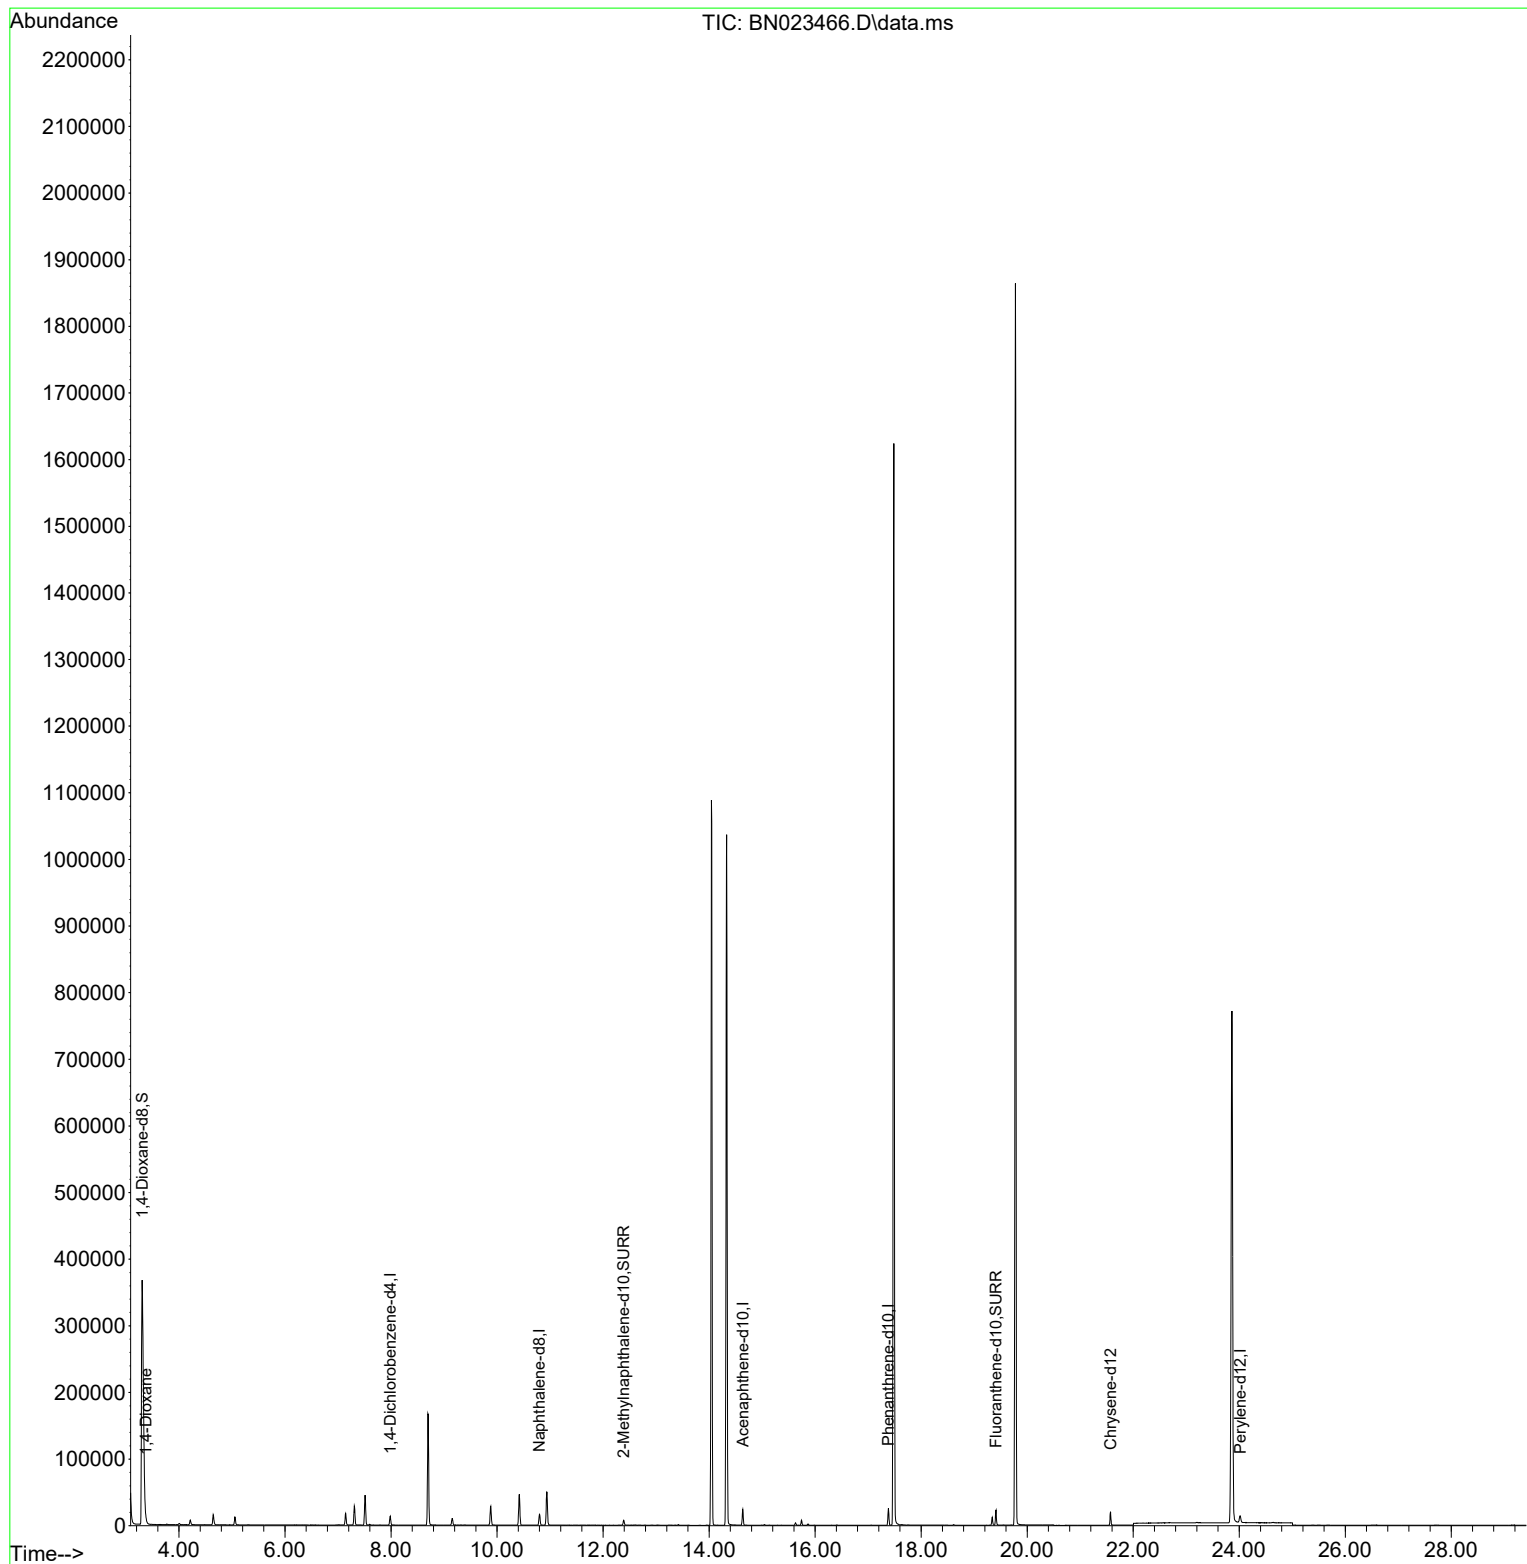

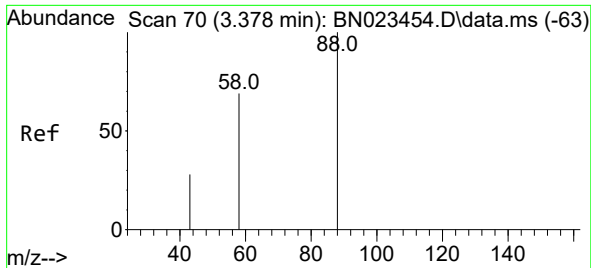

#2
 1,4-Dioxane
 Concen: 0.119 ng/ul
 RT: 3.378 min Scan# 70
 Delta R.T. 0.000 min
 Lab File: BN023466.D
 Acq: 26 Dec 2022 02:19

Instrument :
 BNA_N
 ClientSampleId :
 COLA3

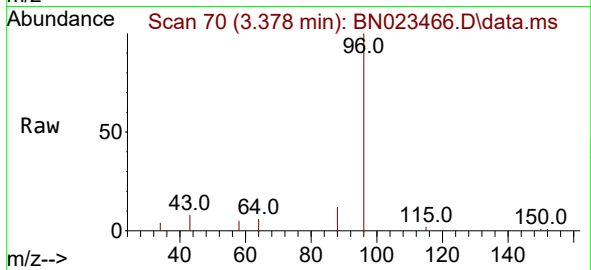

Tgt Ion: 88 Resp: 85
 Ion Ratio Lower Upper
 88 100
 43 63.7 28.4 42.6
 58 39.3 45.6 68.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

