

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023469.D
 Acq On : 26 Dec 2022 04:06
 Operator : CG/JU
 Sample : N6032-13
 Misc :
 ALS Vial : 105 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COLB7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

Quant Time: Dec 26 04:40:51 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)

Internal Standards					
1) 1,4-Dichlorobenzene-d4	7.985	152	5998	0.400 ng/ul	0.00
4) Naphthalene-d8	10.799	136	20072	0.400 ng/ul	0.00
9) Acenaphthene-d10	14.636	164	11723	0.400 ng/ul	0.00
13) Phenanthrene-d10	17.382	188	26390	0.400 ng/ul	0.00
17) Chrysene-d12	21.572	240	16364	0.400 ng/ul	0.00
23) Perylene-d12	24.013	264	13559	0.400 ng/ul	0.00
System Monitoring Compounds					
3) 1,4-Dioxane-d8	3.336	96	32608m	5.003 ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.388	152	8272	0.266 ng/ul	0.00
18) Fluoranthene-d10	19.411	212	20876	0.353 ng/ul	0.00
Target Compounds					
				Qvalue	
2) 1,4-Dioxane	3.374	88	985	0.148 ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023469.D
Acq On : 26 Dec 2022 04:06
Operator : CG/JU
Sample : N6032-13
Misc :
ALS Vial : 105 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
COLB7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/26/2022
Supervised By :Sohil Jodhani 12/26/2022


Quant Time: Dec 26 04:40:51 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

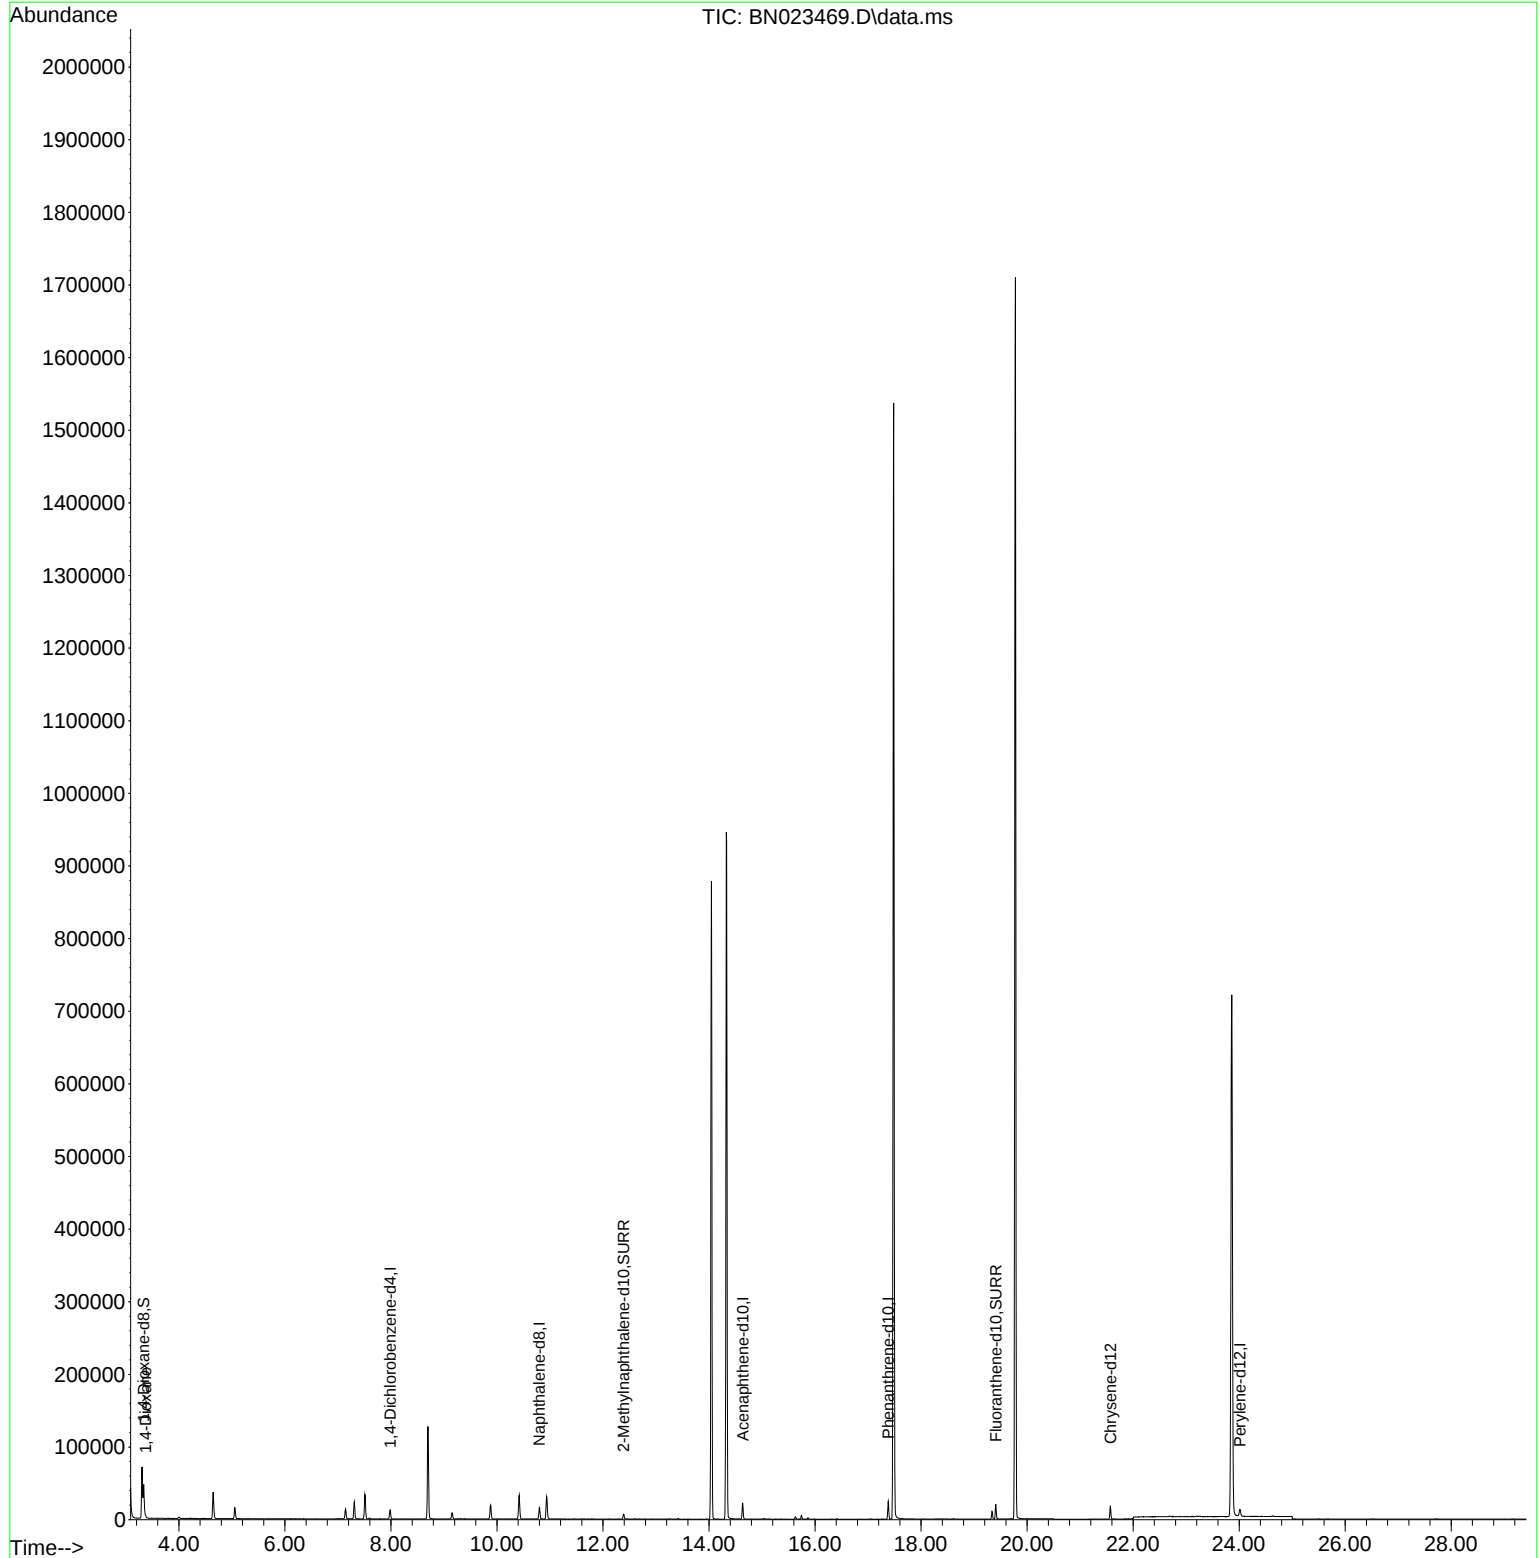

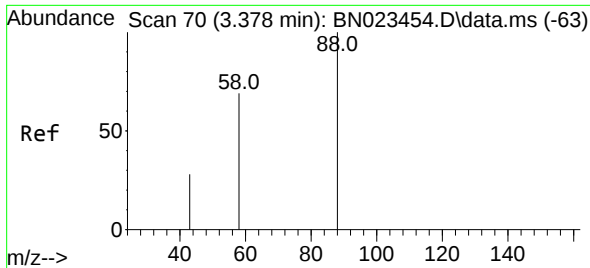

#2
 1,4-Dioxane
 Concen: 0.148 ng/ul
 RT: 3.374 min Scan# 69
 Delta R.T. -0.004 min
 Lab File: BN023469.D
 Acq: 26 Dec 2022 04:06

Instrument :
 BNA_N
 ClientSampleId :
 COLB7

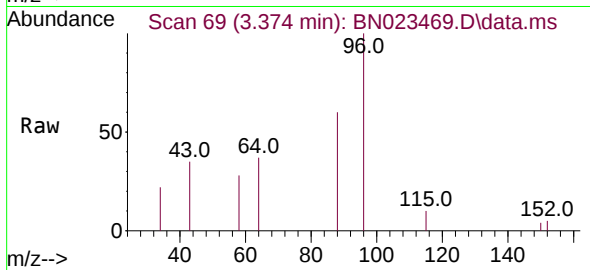

Tgt Ion: 88 Resp: 985

Ion	Ratio	Lower	Upper
88	100		
43	58.4	28.4	42.6
58	46.3	45.6	68.4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/26/2022
 Supervised By :Sohil Jodhani 12/26/2022

