

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
 Data File : BN023476.D
 Acq On : 26 Dec 2022 08:52
 Operator : CG/JU
 Sample : N6053-01
 Misc :
 ALS Vial : 113 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 B0AA8

Quant Time: Dec 27 03:41:35 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 05:17:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.986	152	6040	0.400	ng/ul	0.00
4) Naphthalene-d8	10.798	136	20265	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.630	164	11650	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.381	188	27237	0.400	ng/ul	0.00
17) Chrysene-d12	21.569	240	18551	0.400	ng/ul	# 0.00
23) Perylene-d12	24.013	264	15202	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.336	96	25385	3.868	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.387	152	6156	0.196	ng/ul	0.00
18) Fluoranthene-d10	19.409	212	24395	0.364	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.374	88	677	0.101	ng/ul#	64


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122422\
Data File : BN023476.D
Acq On : 26 Dec 2022 08:52
Operator : CG/JU
Sample : N6053-01
Misc :
ALS Vial : 113 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
B0AA8


Quant Time: Dec 27 03:41:35 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 05:17:59 2022
Response via : Initial Calibration

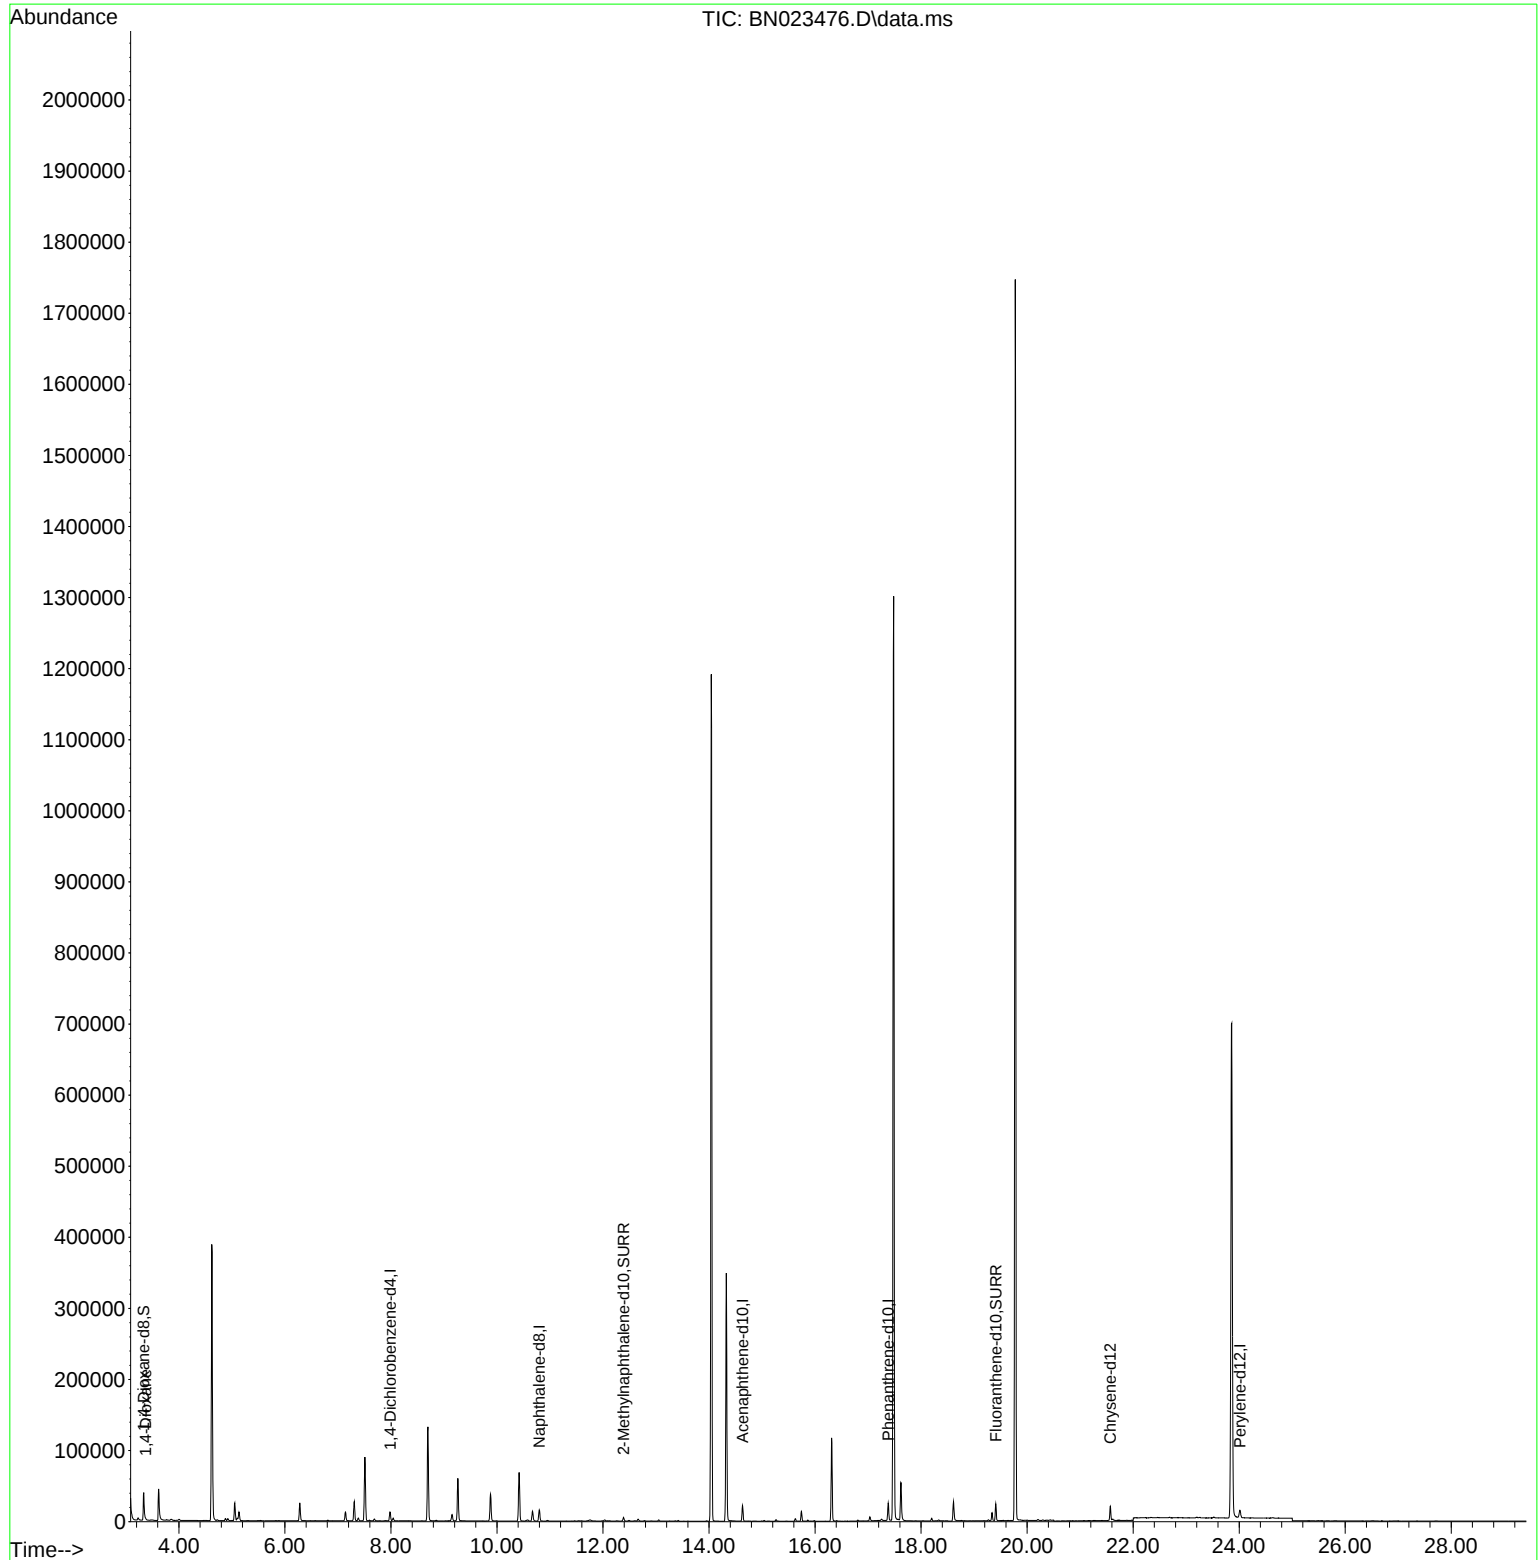

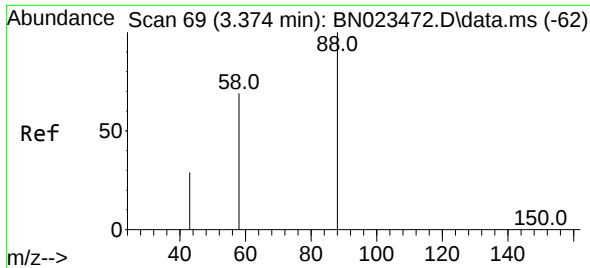

#2
 1,4-Dioxane
 Concen: 0.101 ng/ul
 RT: 3.374 min Scan# 69
 Delta R.T. -0.004 min
 Lab File: BN023476.D
 Acq: 26 Dec 2022 08:52

Instrument :
 BNA_N
 ClientSampleId :
 B0AA8

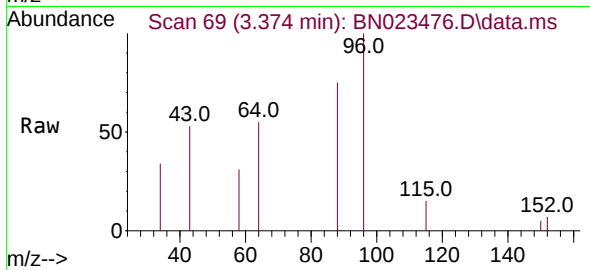

Tgt Ion: 88 Resp: 677

Ion	Ratio	Lower	Upper
88	100		
43	70.3	28.4	42.6#
58	41.9	45.6	68.4#

