

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122818\
 Data File : BN004277.D
 Acq On : 28 Dec 2018 23:46
 Operator : JU/SJ
 Sample : J6541-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F64

Quant Time: Dec 29 00:56:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 28 22:16:51 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2381	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	10968	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.46	164	6578	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1202684	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.57	264	1251867	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	5612	0.33	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.46	166	1939	0.065	ng/ul#	Qvalue 13




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122818\
Data File : BN004277.D
Acq On : 28 Dec 2018 23:46
Operator : JU/SJ
Sample : J6541-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F64

Quant Time: Dec 29 00:56:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 28 22:16:51 2018
Response via : Initial Calibration

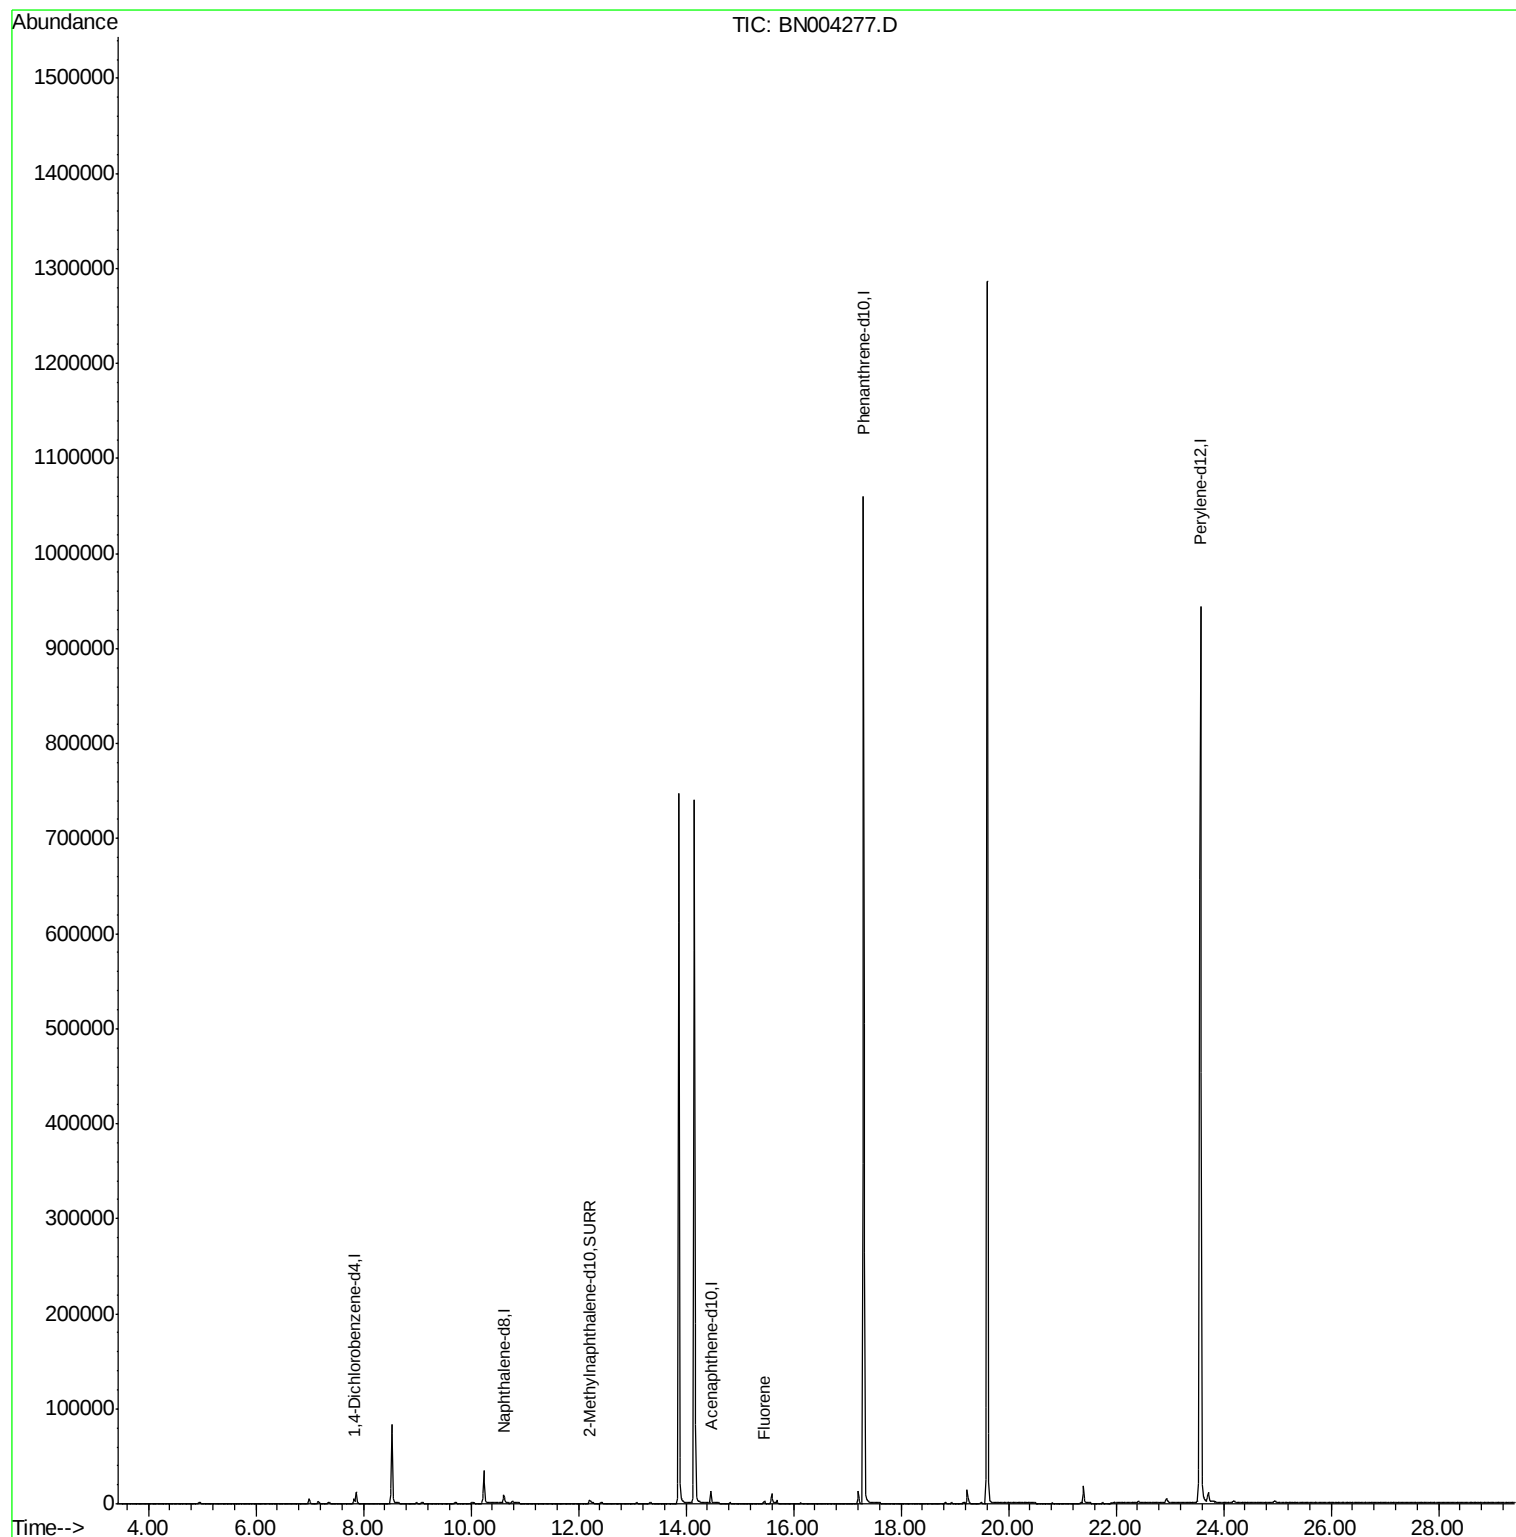

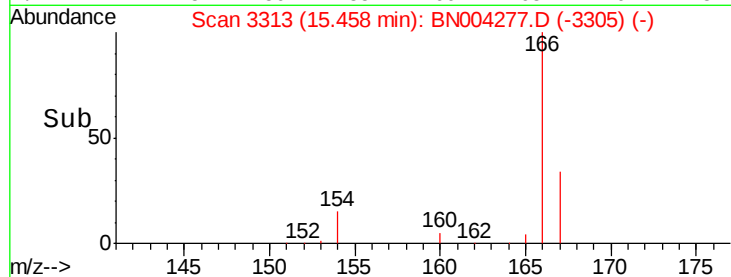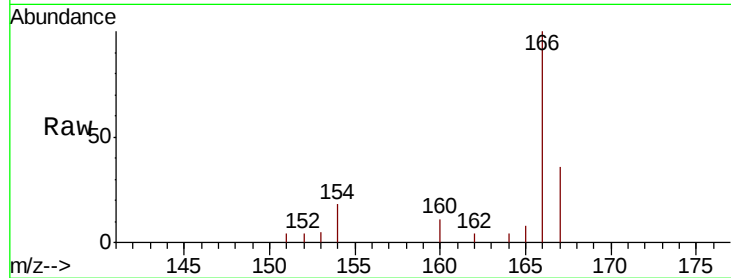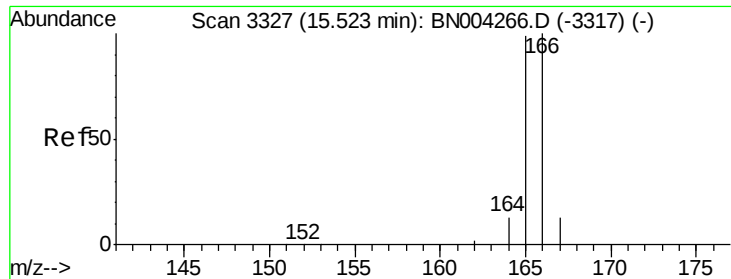

#9

Fluorene

Concen: 0.065 ng/ul

RT: 15.46 min Scan# 3313

Delta R.T. -0.06 min

Lab File: BN004277.D

Acq: 28 Dec 2018 23:46

Instrument :

BNA_N

ClientSampleId :

F9F64

Tgt Ion:166 Resp: 1939

Ion Ratio Lower Upper

166 100

165 8.2 79.0 118.6#

167 36.3 11.3 16.9#

Abundance Ion 166.00 (165.70 to 166.70): E

2000 Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

