

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122818\
 Data File : BN004280.D
 Acq On : 29 Dec 2018 01:32
 Operator : JU/SJ
 Sample : J6541-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F65

Quant Time: Dec 29 04:07:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 28 22:16:51 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2514	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	11139	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.46	164	7059	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1273386	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.57	264	1399587	0.40	ng/ul	-0.16
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	5936	0.35	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.66	128	3662	0.117	ng/ul	Qvalue 96




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122818\
Data File : BN004280.D
Acq On : 29 Dec 2018 01:32
Operator : JU/SJ
Sample : J6541-12
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9F65

Quant Time: Dec 29 04:07:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 28 22:16:51 2018
Response via : Initial Calibration

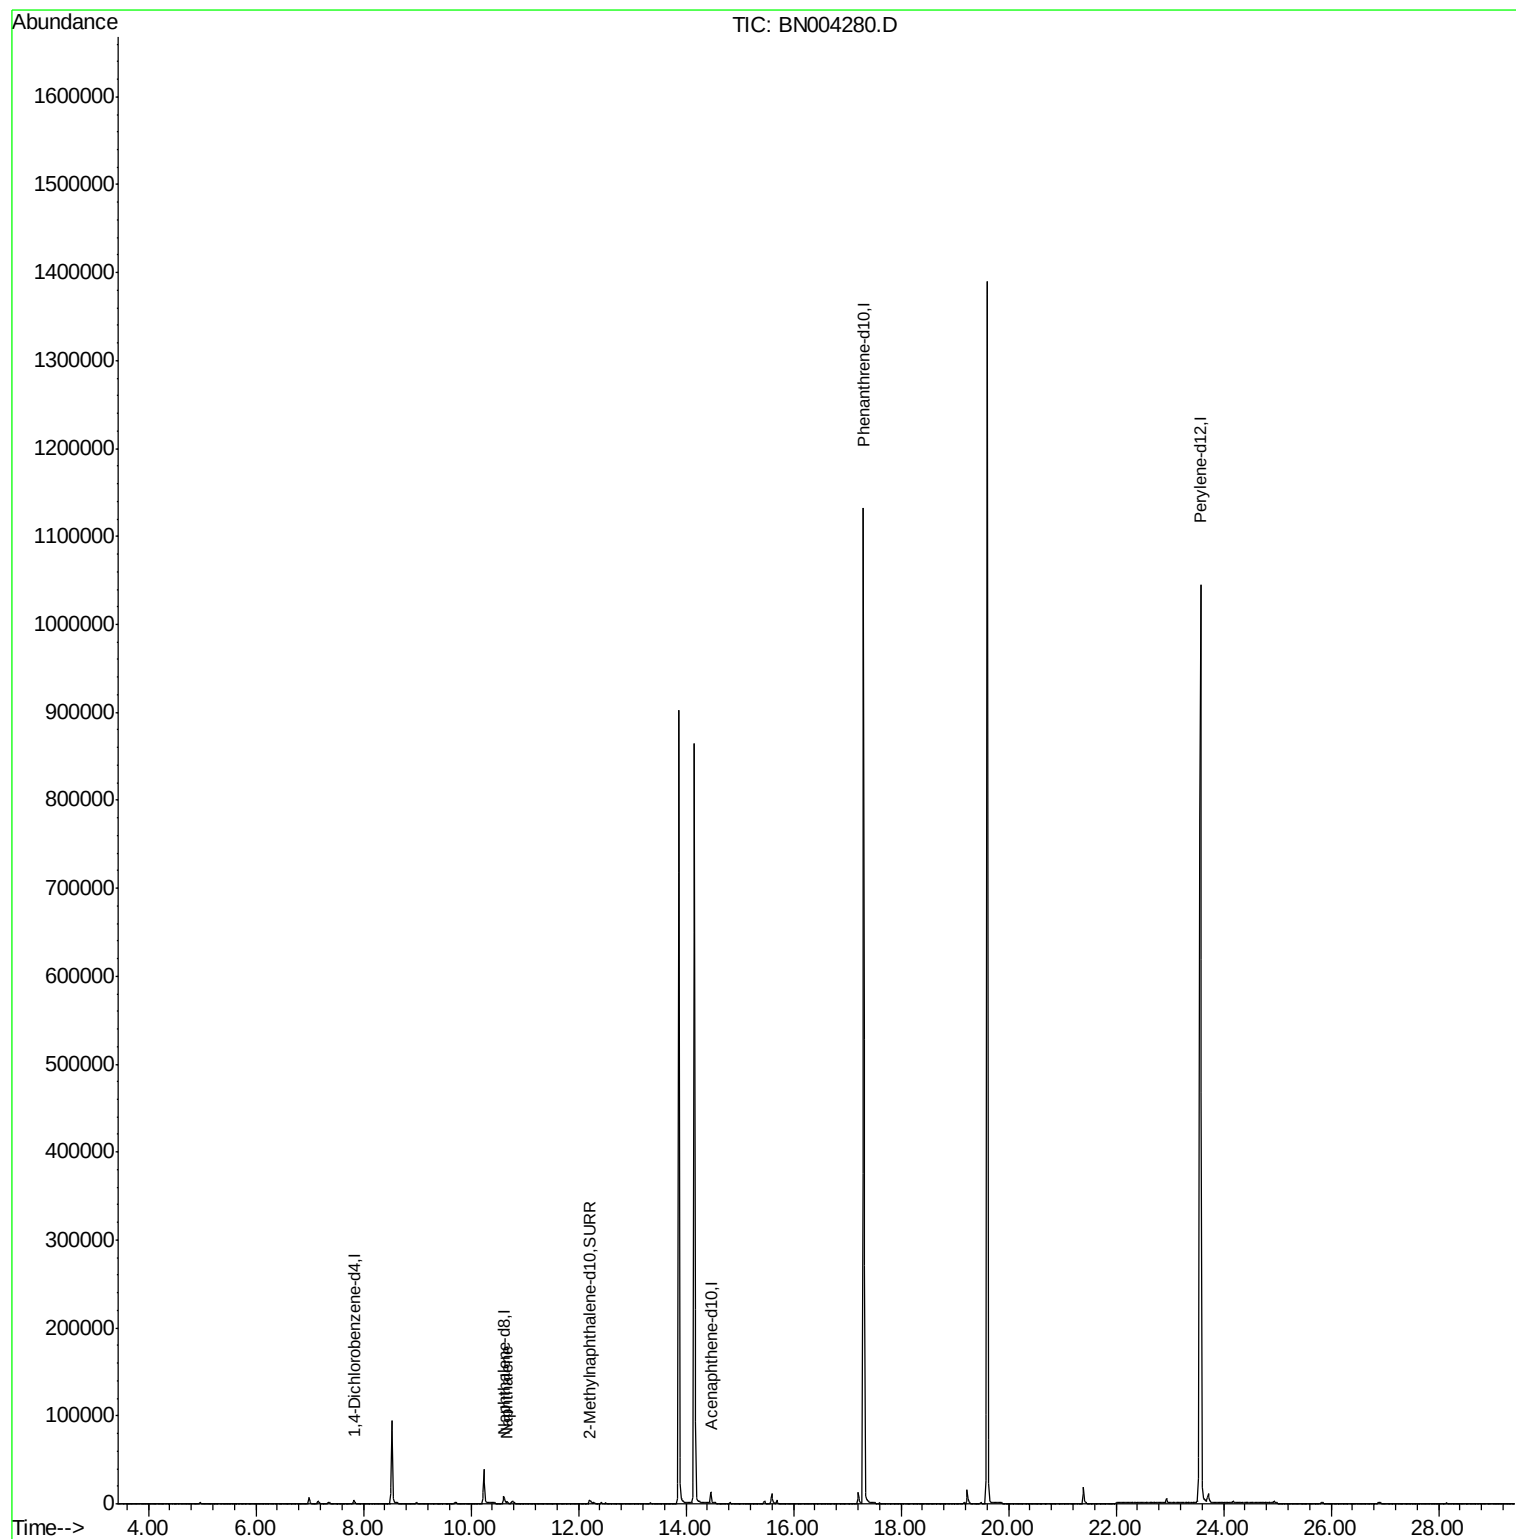

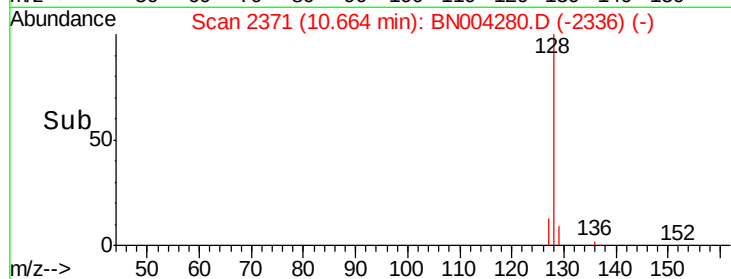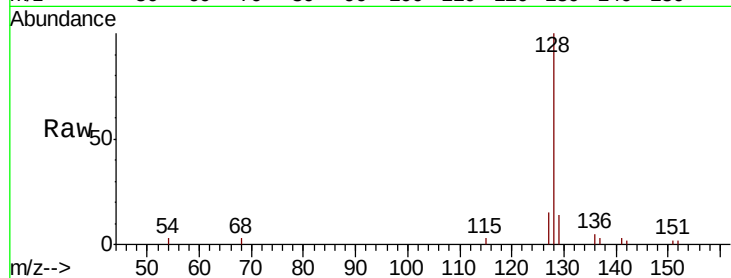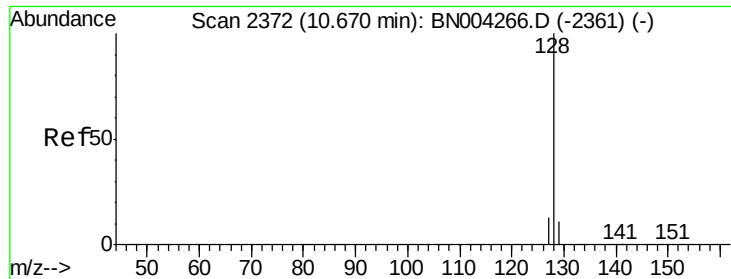

#3

Naphthalene

Concen: 0.117 ng/ul

RT: 10.66 min Scan# 2371

Delta R.T. -0.01 min

Lab File: BN004280.D

Acq: 29 Dec 2018 01:32

Instrument :

BNA_N

ClientSampleId :

F9F65

Tgt Ion:128 Resp: 3662

Ion Ratio Lower Upper

128 100

129 14.0 9.5 14.3

127 14.8 11.0 16.4

