

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122818\
 Data File : BN004273.D
 Acq On : 28 Dec 2018 21:26
 Operator : JU/SJ
 Sample : J6541-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F79

Manual Integrations
 APPROVED

Sohil
 1/2/2019 3:39:36 PM

Quant Time: Dec 29 00:55:23 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 28 22:16:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	2384	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	10952	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.46	164	6749	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	15235m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.40	240	16084m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	12641m	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.20	152	5145	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	15318m	0.34	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.25	178	1193m	0.024	ng/ul	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122818\
Data File : BN004273.D
Acq On : 28 Dec 2018 21:26
Operator : JU/SJ
Sample : J6541-05
Misc :
ALS Vial : 9 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
F9F79

Quant Time: Dec 29 00:55:23 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 28 22:16:51 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
1/2/2019 3:39:36 PM

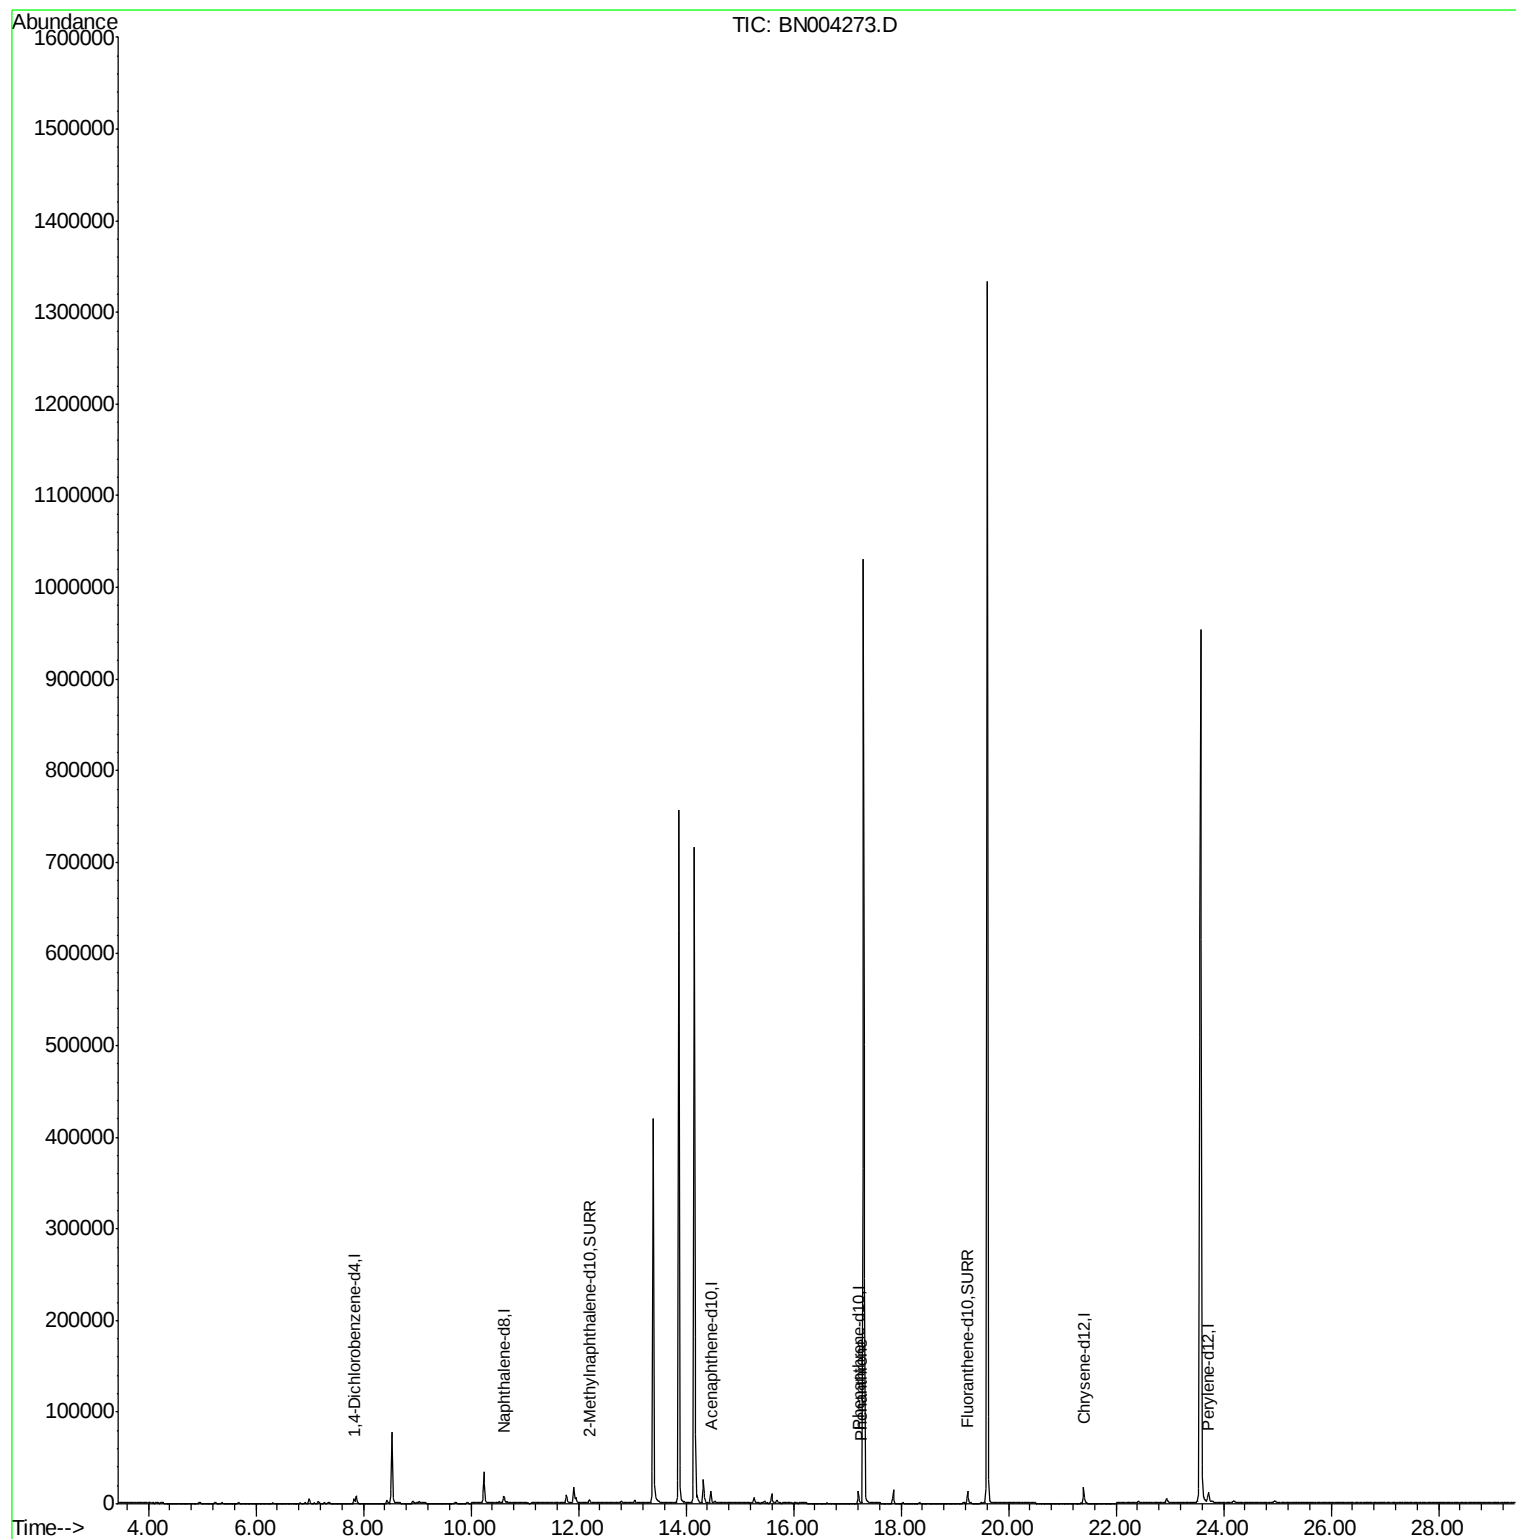

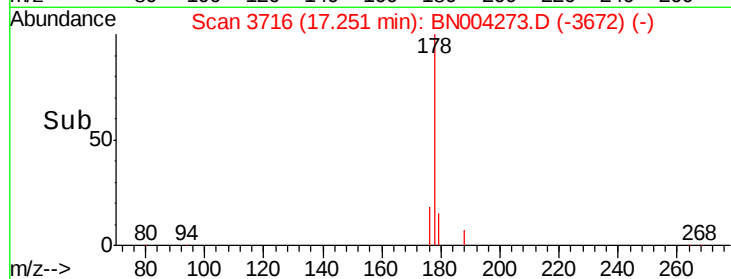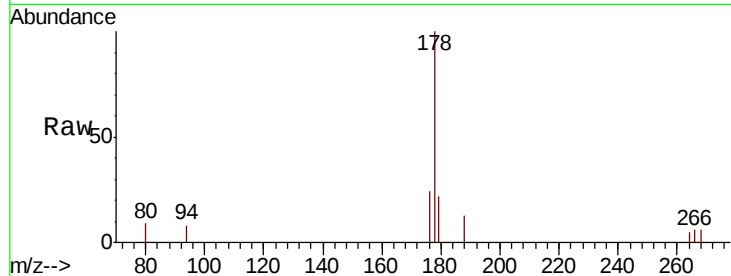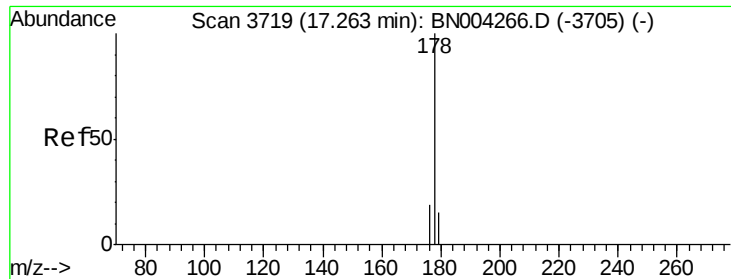

#12

Phenanthrene

Concen: 0.024 ng/ul m

RT: 17.25 min Scan# 3716

Delta R.T. -0.01 min

Lab File: BN004273.D

Acq: 28 Dec 2018 21:26

Instrument :

BNA_N

ClientSampleId :

F9F79

Tot Ion:	178	Resp:	1193
Ion Ratio	Lower	Upper	
178	100		
179	22.4	12.6	18.8#
176	23.8	15.2	22.8#

Manual Integrations
APPROVED

Sohil
1/2/2019 3:39:36 PM

