

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122818\
 Data File : BN004274.D
 Acq On : 28 Dec 2018 22:01
 Operator : JU/SJ
 Sample : J6541-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 F9F61

Manual Integrations
 APPROVED

Sohil
 1/2/2019 3:39:39 PM

Quant Time: Dec 29 03:22:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN122818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 28 22:16:51 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	2430	0.40	ng/ul	0.00
2) Naphthalene-d8	10.61	136	10955	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.46	164	6575	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	14951m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.40	240	15015m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	11723m	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.21	152	5290	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	14810m	0.34	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.66	128	3064	0.099	ng/ul#	Ovalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN122818\
Data File : BN004274.D
Acq On : 28 Dec 2018 22:01
Operator : JU/SJ
Sample : J6541-06
Misc :
ALS Vial : 10 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
F9F61

Quant Time: Dec 29 03:22:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN122818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 28 22:16:51 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
1/2/2019 3:39:39 PM

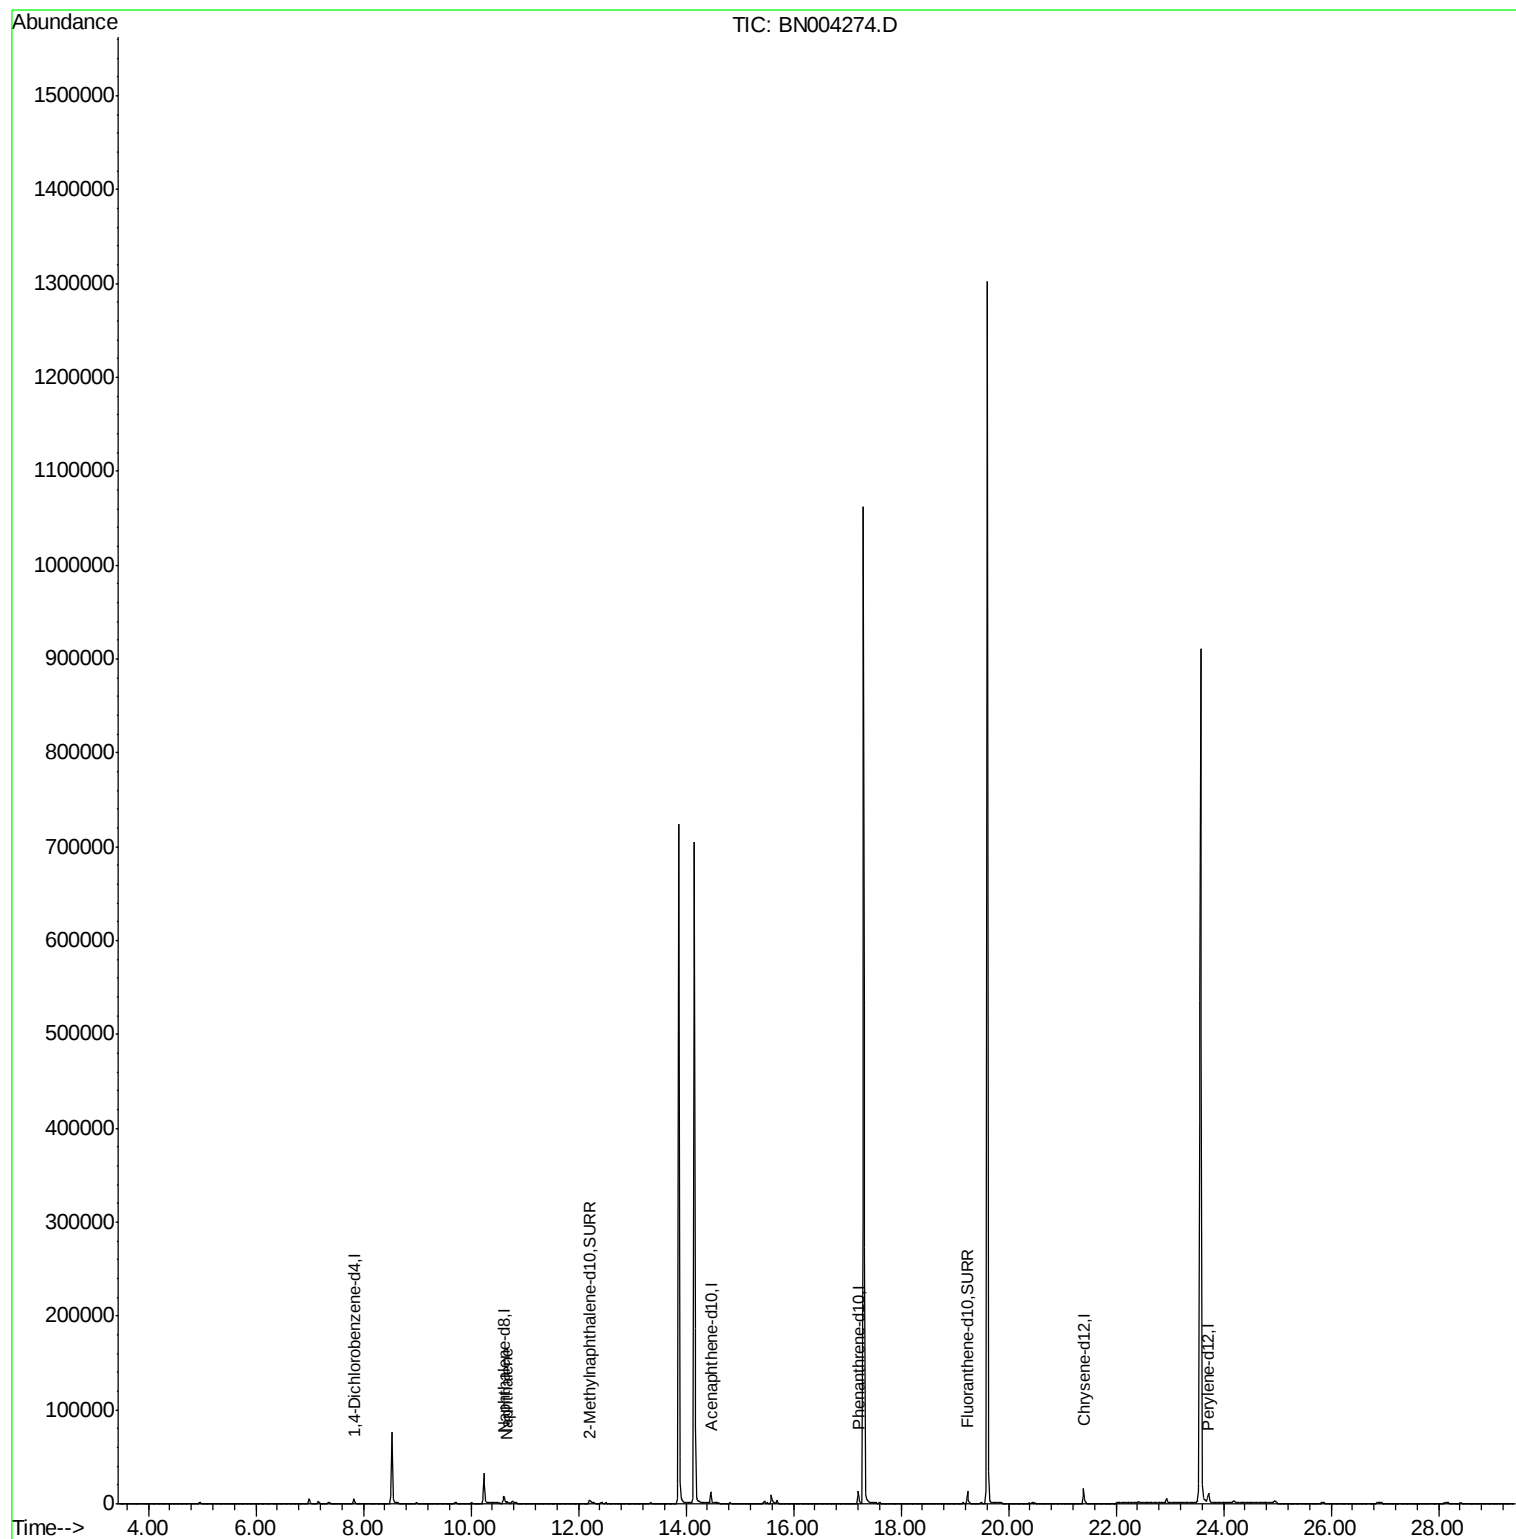

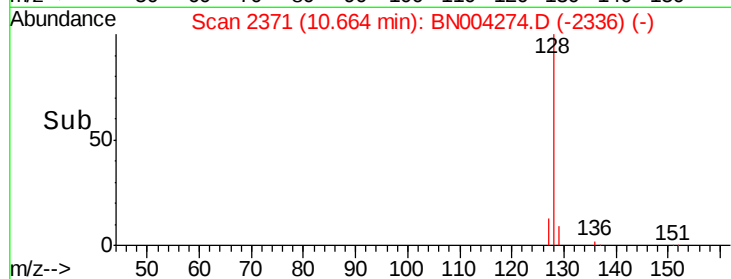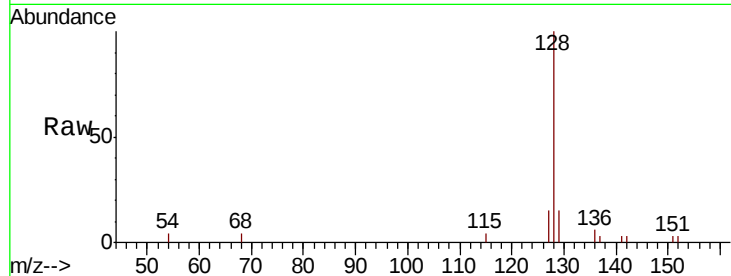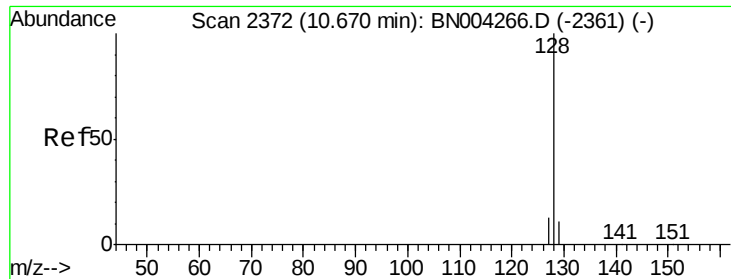

#3

Naphthalene

Concen: 0.099 ng/ul

RT: 10.66 min Scan# 2371

Delta R.T. -0.01 min

Lab File: BN004274.D

Acq: 28 Dec 2018 22:01

Tot Ion:	128	Resp:	3064
Ion Ratio	Lower	Upper	
128	100		
129	14.8	9.5	14.3#
127	15.3	11.0	16.4

Instrument :

BNA_N

ClientSampleId :

F9F61

Manual Integrations
APPROVED

Sohil
1/2/2019 3:39:39 PM

