

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
 Data File : BN018234.D
 Acq On : 28 Dec 2021 12:40
 Operator : CG/JU
 Sample : M5201-15
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P080-TW001-A-01

Quant Time: Dec 28 13:38:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	4221	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	15247	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.248	164	11531	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.990	188	26652	0.400	ng/ul	0.00
17) Chrysene-d12	21.184	240	24581	0.400	ng/ul	0.00
23) Perylene-d12	23.399	264	32529	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	19173	4.866	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.987	152	9257	0.349	ng/ul	0.00
18) Fluoranthene-d10	19.026	212	36783	0.505	ng/ul	0.00
Target Compounds						
7) 2-Methylnaphthalene	12.064	142	1081	0.033	ng/ul	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
Data File : BN018234.D
Acq On : 28 Dec 2021 12:40
Operator : CG/JU
Sample : M5201-15
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P080-TW001-A-01

Quant Time: Dec 28 13:38:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration

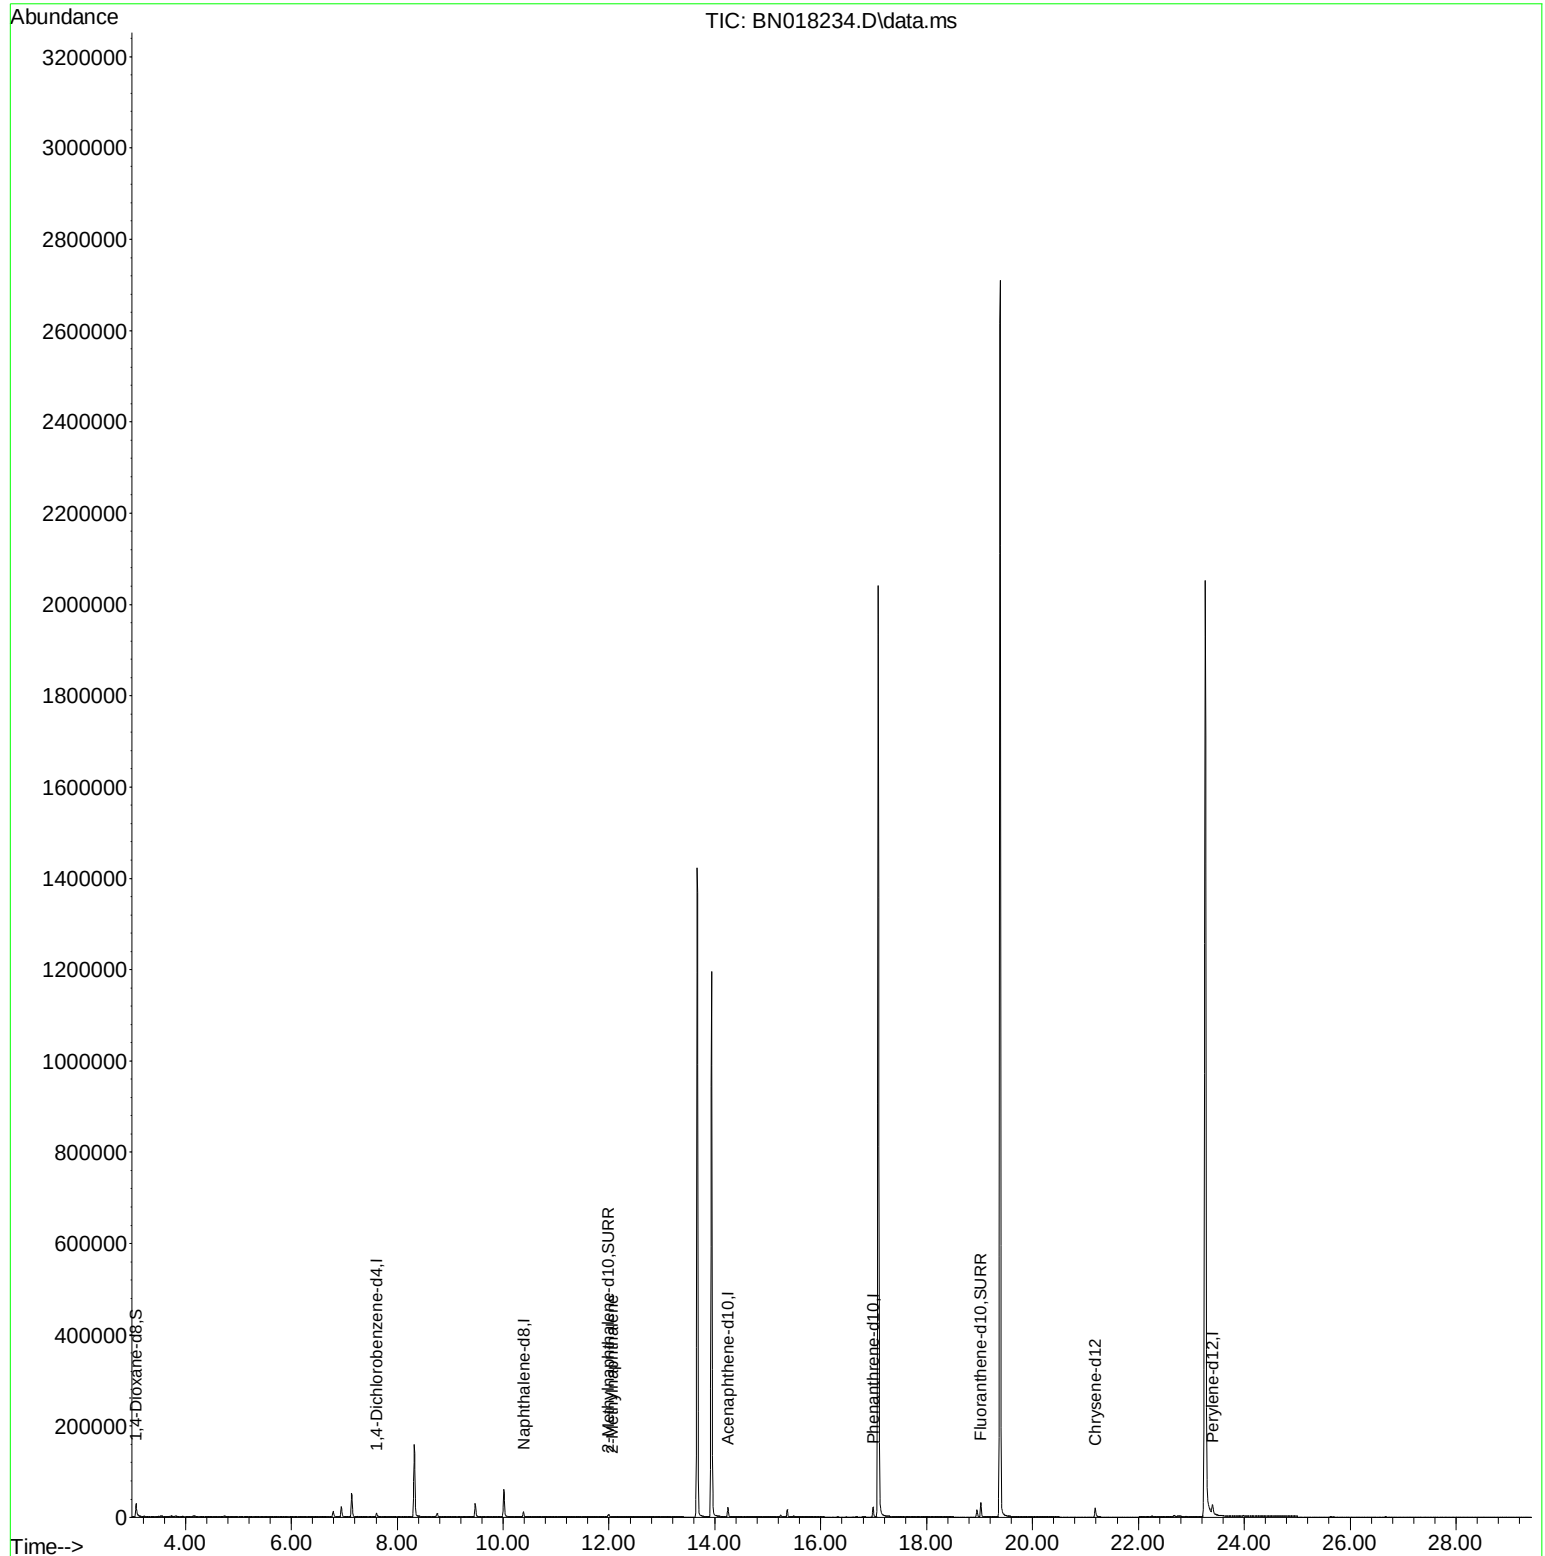

Abundance Scan 2042 (12.064 min): BN018232.D\data.ms (-2023) (-)

2-Methylnaphthalene

Concen: 0.033 ng/ul

RT: 12.064 min Scan# 1

Delta R.T. 0.005 min

Lab File: BN018234.D

Acq: 28 Dec 2021 12:40

Instrument :

BNA_N

ClientSampleId :

P080-TW001-A-01

Tgt Ion:142 Resp: 1081

Ion Ratio Lower Upper

142 100

141 89.3 70.9 106.3

Abundance Scan 2042 (12.064 min): BN018234.D\data.ms

Raw

54.0 68.0 115.0 142.0

m/z-->

Abundance Scan 2042 (12.064 min): BN018234.D\data.ms (-2023) (-)

Sub

115.0 142.0

m/z-->

Abundance

12.064

500

400

300

200

100

0

Time-->

12.00 12.10