

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
 Data File : BN018235.D
 Acq On : 28 Dec 2021 13:16
 Operator : CG/JU
 Sample : M5201-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P078-TW001-01

Quant Time: Dec 28 13:45:37 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	4183	0.400	ng/ul	0.00
4) Naphthalene-d8	10.387	136	14993	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.248	164	11288	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.990	188	27591	0.400	ng/ul	0.00
17) Chrysene-d12	21.184	240	26503	0.400	ng/ul	0.00
23) Perylene-d12	23.400	264	31495	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	14942	3.826	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.987	152	7139	0.274	ng/ul	0.00
18) Fluoranthene-d10	19.021	212	31892	0.406	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.028	178	2550	0.028	ng/ul#	87
19) Fluoranthene	19.054	202	2313	0.022	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
Data File : BN018235.D
Acq On : 28 Dec 2021 13:16
Operator : CG/JU
Sample : M5201-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P078-TW001-01

Quant Time: Dec 28 13:45:37 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration

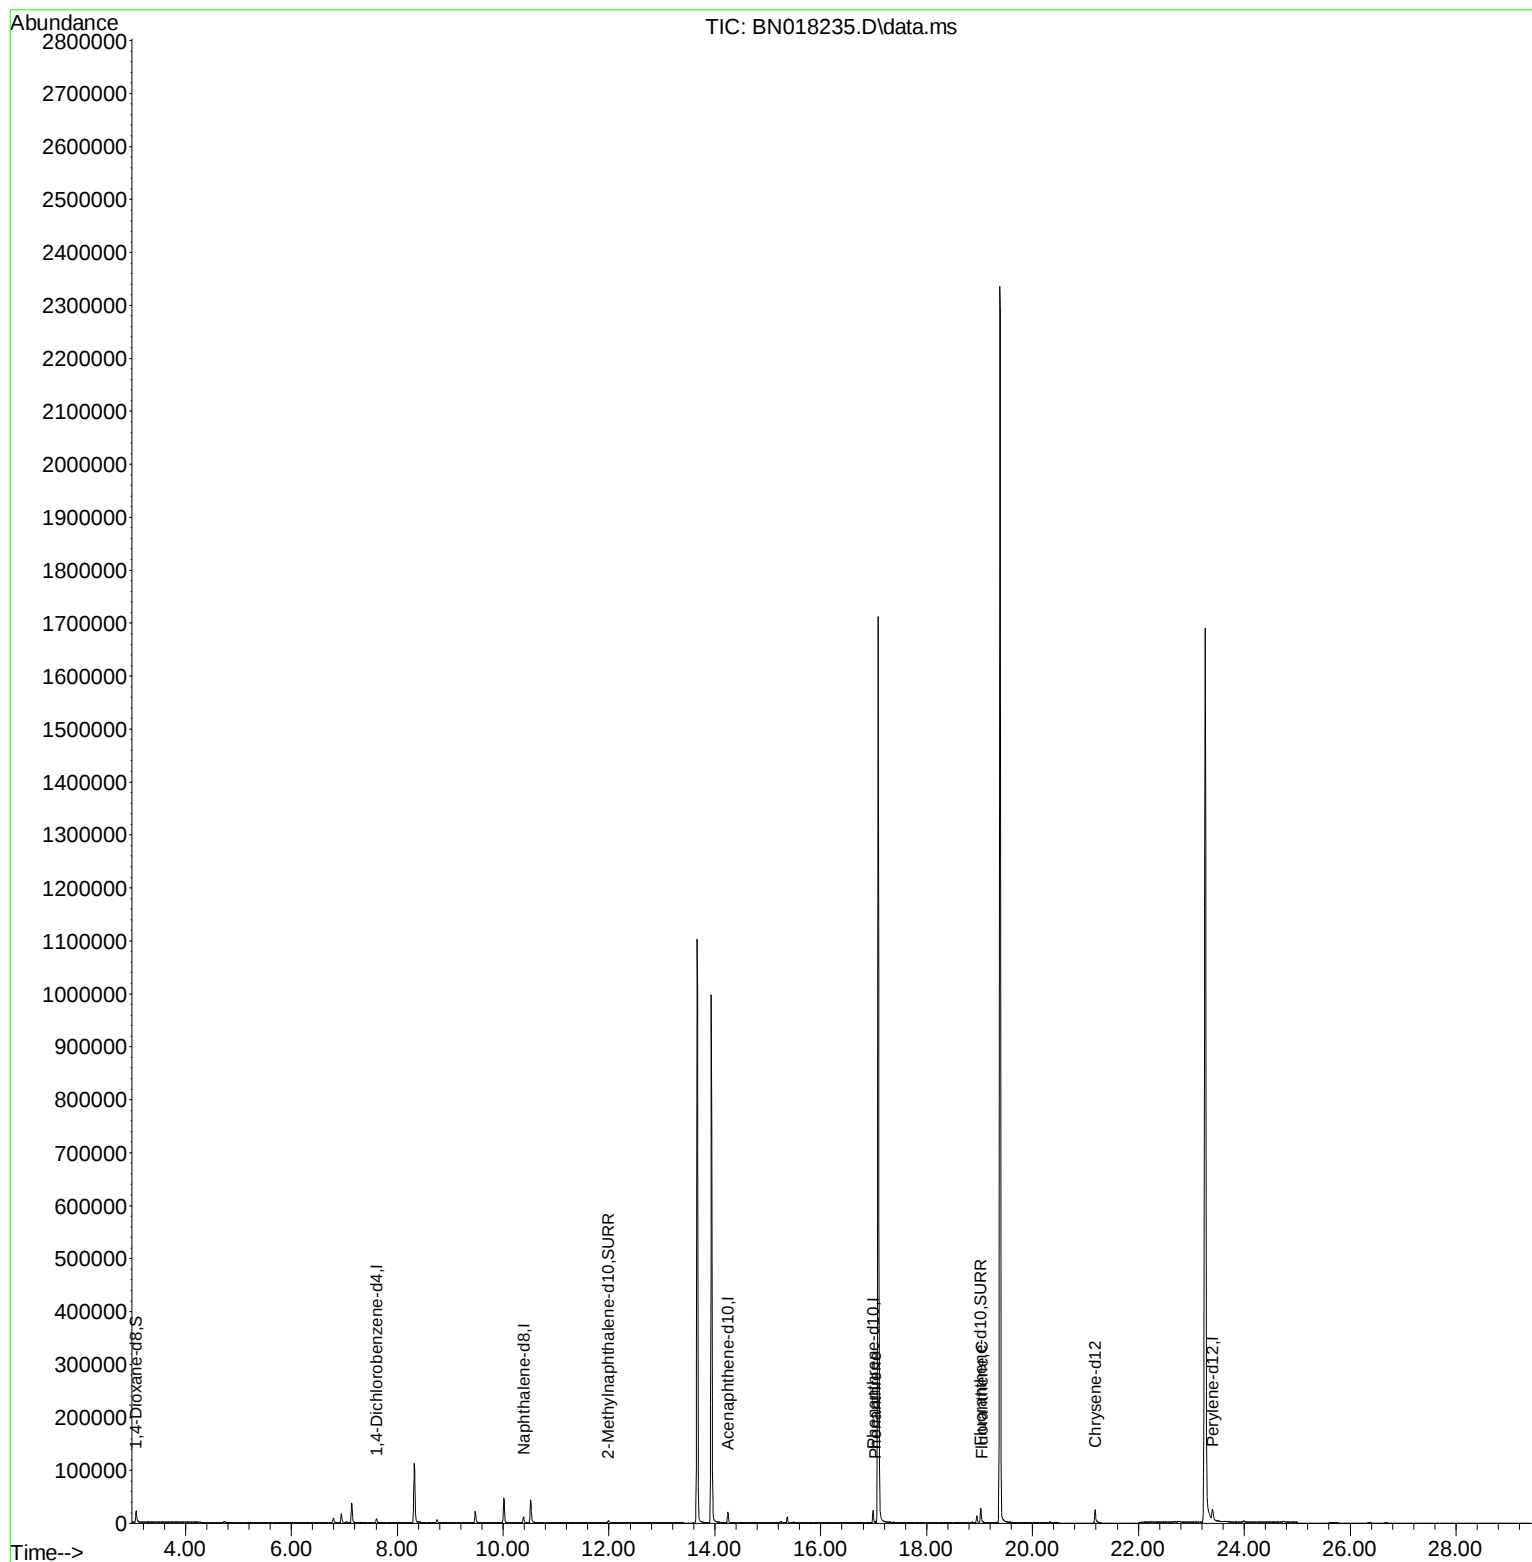

Abundance Scan 3091 (17.032 min): BN018232.D\data.ms (-30715) (-)

Phenanthrene

Concen: 0.028 ng/ul

RT: 17.028 min Scan# 3091

Delta R.T. -0.004 min

Lab File: BN018235.D


Acq: 28 Dec 2021 13:16

Instrument :

BNA_N

ClientSampleId :

P078-TW001-01

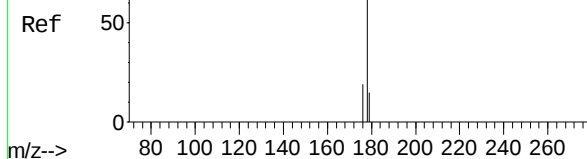



Tgt Ion:178 Resp: 2550

Ion Ratio Lower Upper


178 100

179 22.3 12.2 18.4#

176 23.5 15.4 23.2#

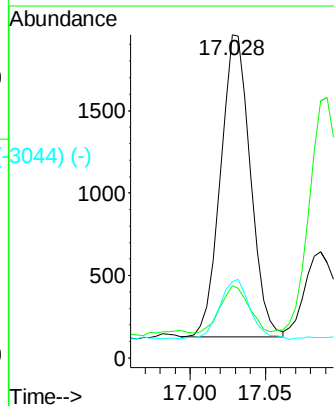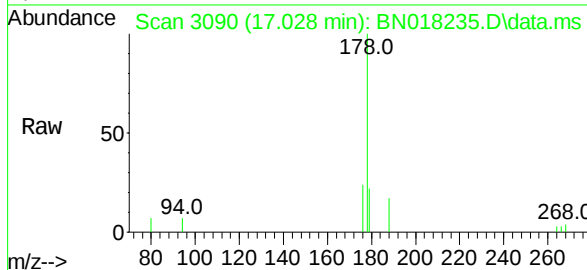

Abundance Scan 3090 (17.028 min): BN018235.D\data.ms (-3044) (-)

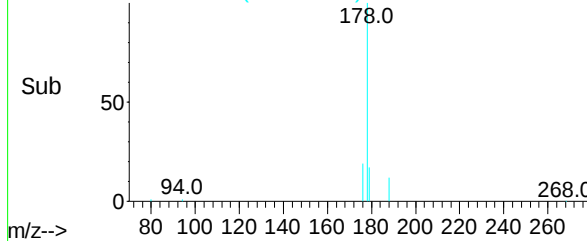

Abundance Scan 3558 (19.054 min): BN018232.D\data.ms (-3549) (-)

Fluoranthene

Concen: 0.022 ng/ul

RT: 19.054 min Scan# 3558

Delta R.T. 0.000 min

Lab File: BN018235.D

Acq: 28 Dec 2021 13:16



Tgt Ion:202 Resp: 2313

Ion Ratio Lower Upper

202 100

101 14.3 7.5 11.3#

100 11.6 5.4 8.2#

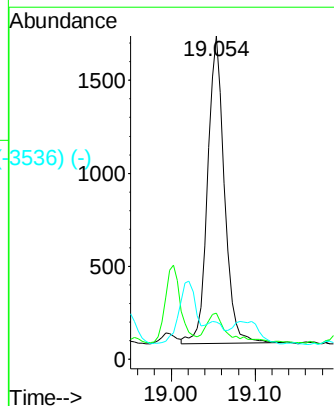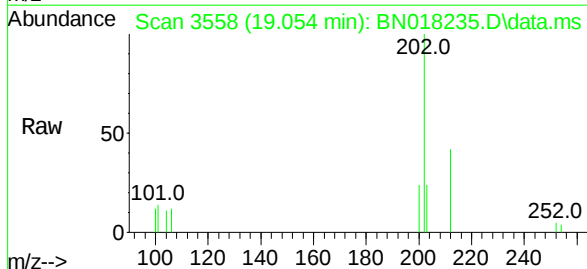

Abundance Scan 3558 (19.054 min): BN018235.D\data.ms (-3536) (-)

