

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
 Data File : BN018237.D
 Acq On : 28 Dec 2021 14:28
 Operator : CG/JU
 Sample : M5201-12
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 P077-TW001-01

Quant Time: Dec 28 15:02:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 28 00:34:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.607	152	4679	0.400	ng/ul	0.00
4) Naphthalene-d8	10.383	136	17092	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.250	164	12924	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.987	188	30983	0.400	ng/ul	0.00
17) Chrysene-d12	21.183	240	30192	0.400	ng/ul	0.00
23) Perylene-d12	23.401	264	36571	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.067	96	22126	5.065	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.989	152	10022	0.337	ng/ul	0.00
18) Fluoranthene-d10	19.023	212	41818	0.467	ng/ul	0.00
Target Compounds						
15) Phenanthrene	17.029	178	2345	0.023	ng/ul#	Qvalue 86

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122821\
Data File : BN018237.D
Acq On : 28 Dec 2021 14:28
Operator : CG/JU
Sample : M5201-12
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
P077-TW001-01

Quant Time: Dec 28 15:02:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN122721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 28 00:34:45 2021
Response via : Initial Calibration

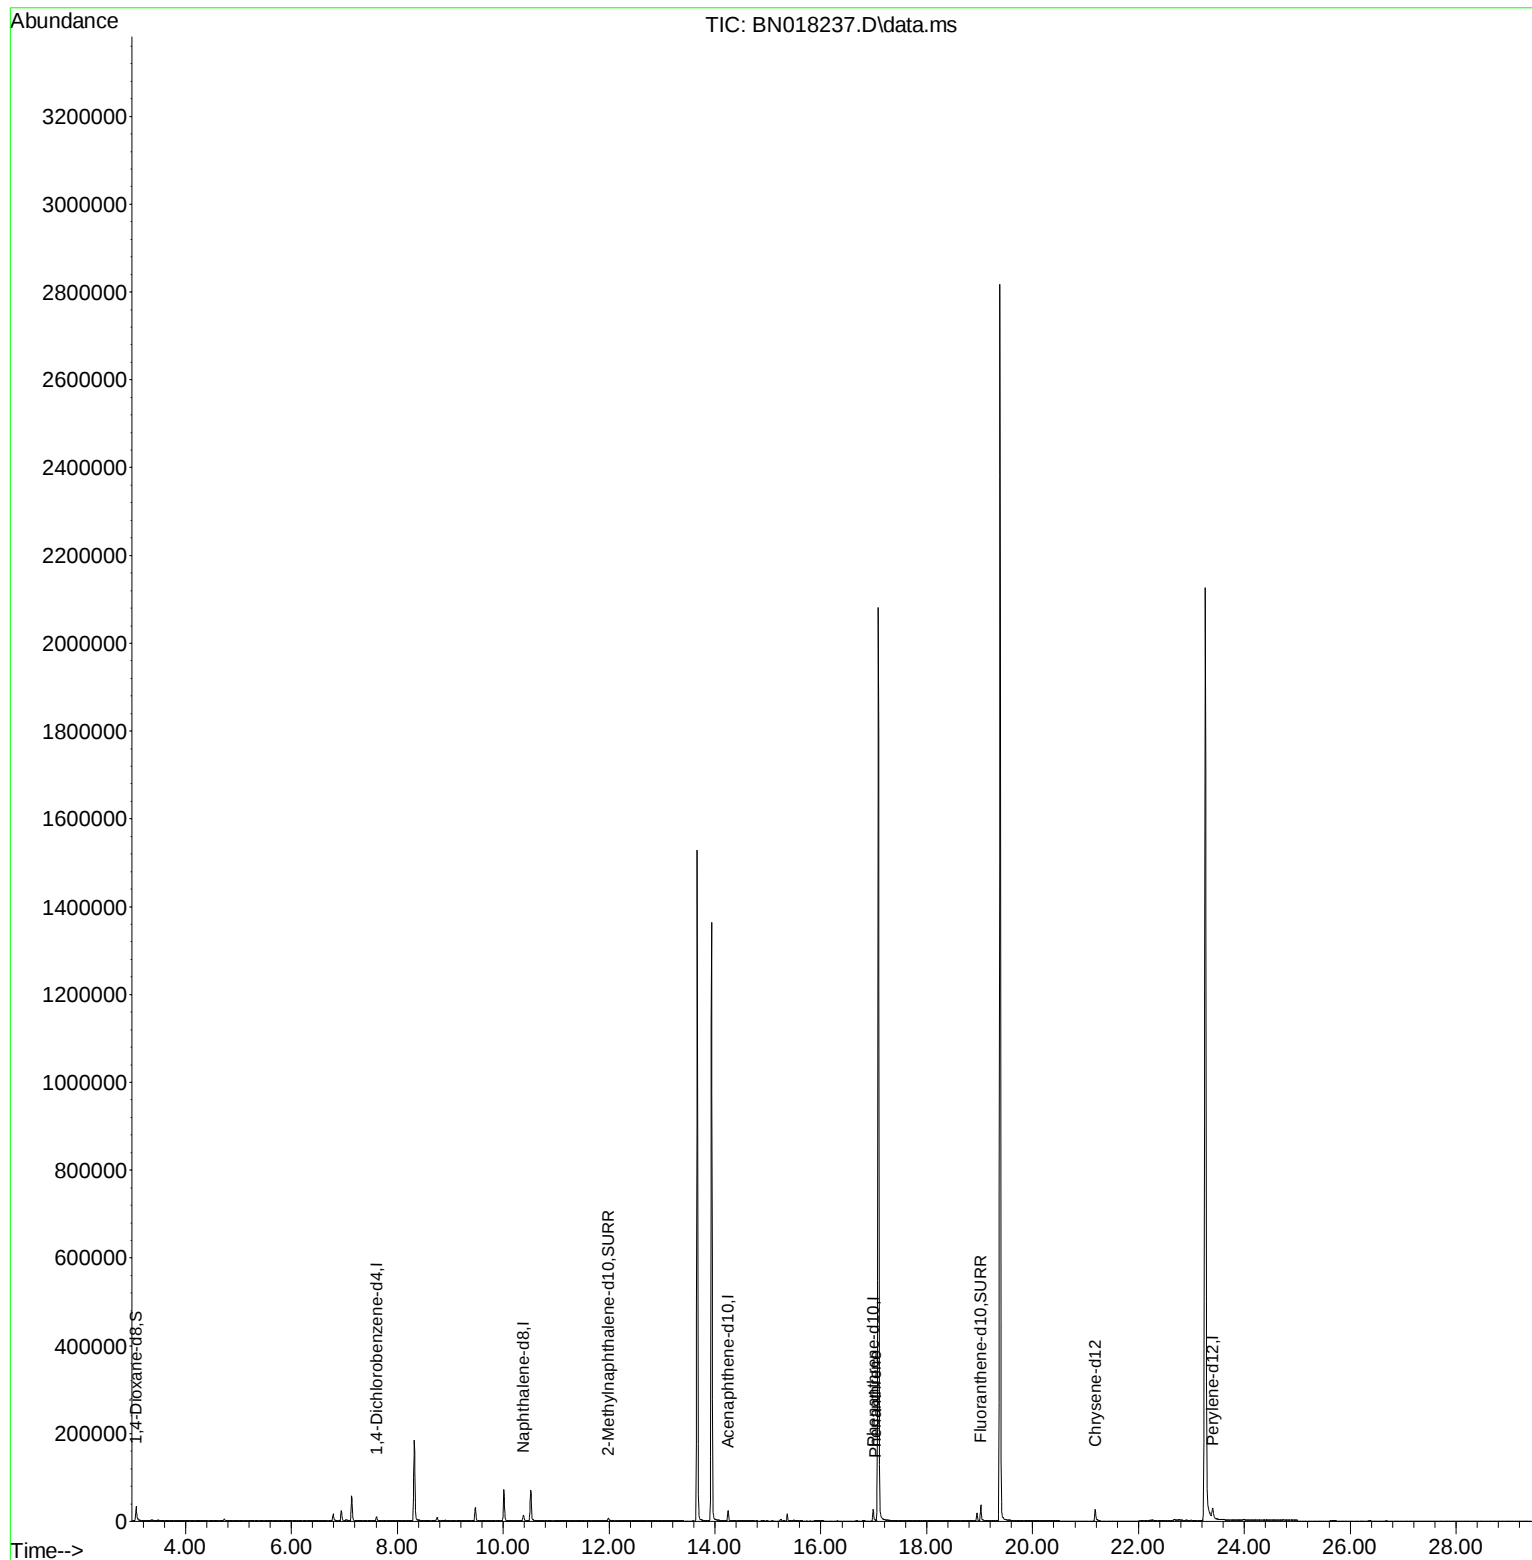

Abundance Scan 3091 (17.032 min): BN018232.D\data.ms (-30715) (-)

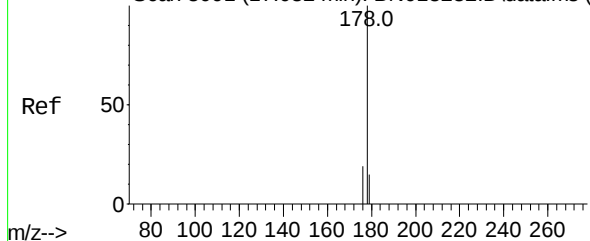

Phenanthrene

Concen: 0.023 ng/ul

RT: 17.029 min Scan#

Delta R.T. -0.003 min

Lab File: BN018237.D


Acq: 28 Dec 2021 14:28

Instrument :

BNA_N

ClientSampleId :

P077-TW001-01

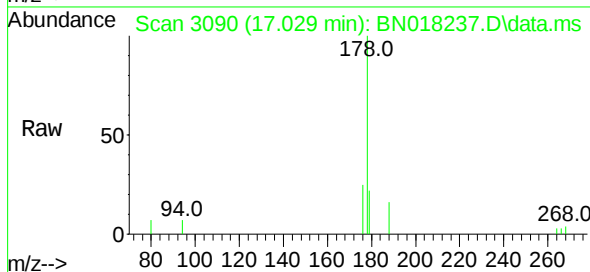


Tgt Ion:178 Resp: 2345

Ion Ratio Lower Upper

178 100

179 22.3 12.2 18.4#

176 24.9 15.4 23.2#

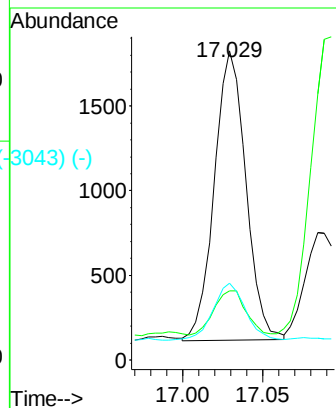

Abundance Scan 3090 (17.029 min): BN018237.D\data.ms (-3043) (-)

