


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN122918\
 Data File : BN004303.D
 Acq On : 02 Jan 2019 10:28
 Operator : JU/SJ
 Sample : DFTPP53
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP53

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN121218MA.M
 Title : SVOA CALIBRATION
 Last Update : Fri Dec 28 03:12:04 2018

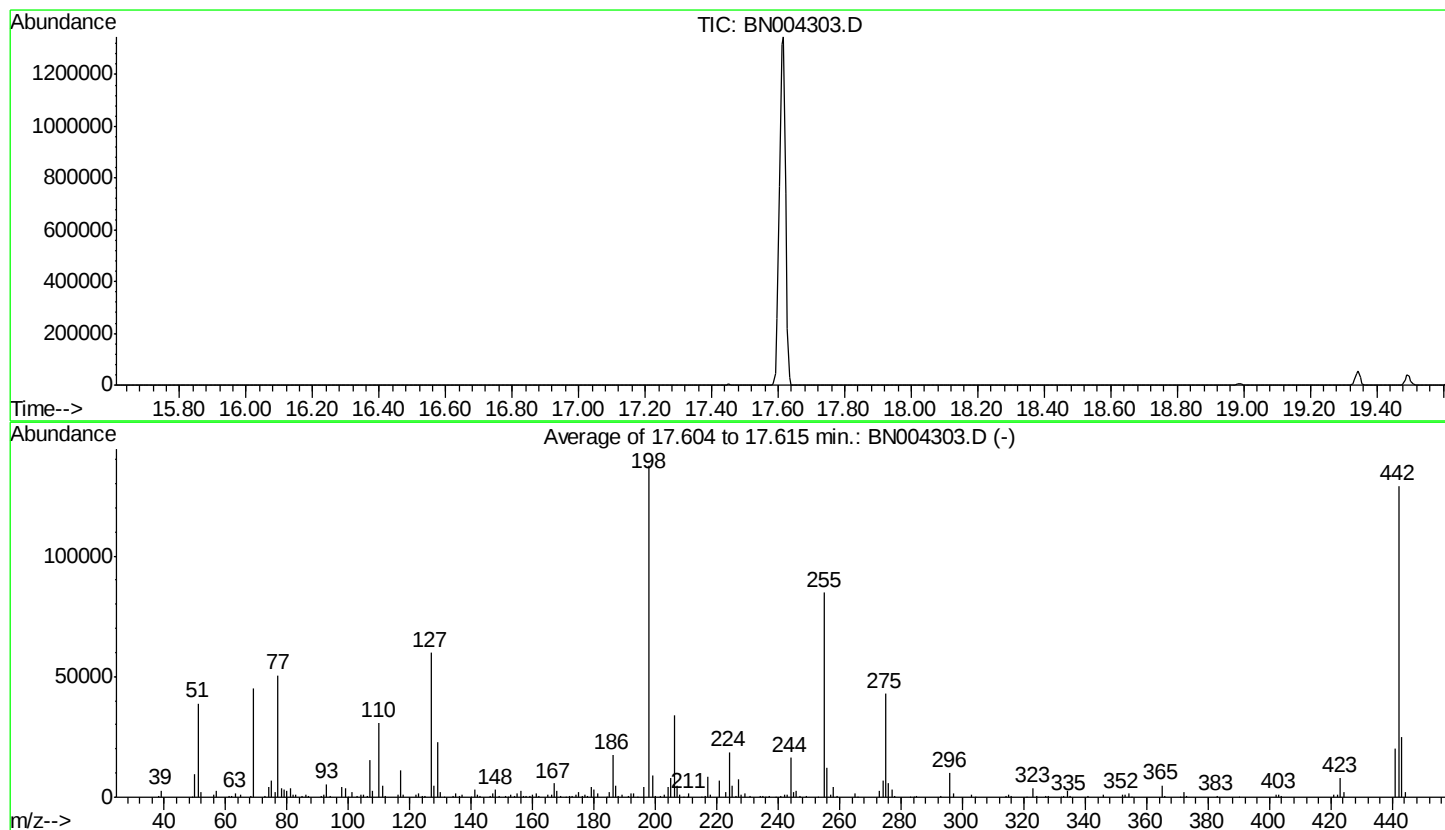

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	38829	PASS
68	69	0.00	2	0.7	322	PASS
69	198	0.00	100	32.7	44906	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.6	59930	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137437	PASS
199	198	5	9	6.7	9268	PASS
275	198	10	60	31.1	42778	PASS
365	198	1	100	3.7	5019	PASS
441	198	0.01	100	14.8	20296	PASS
442	198	50	100	93.8	128920	PASS
443	442	15	24	19.4	24952	PASS