


Nitrobenzene-d5

Response Ratio

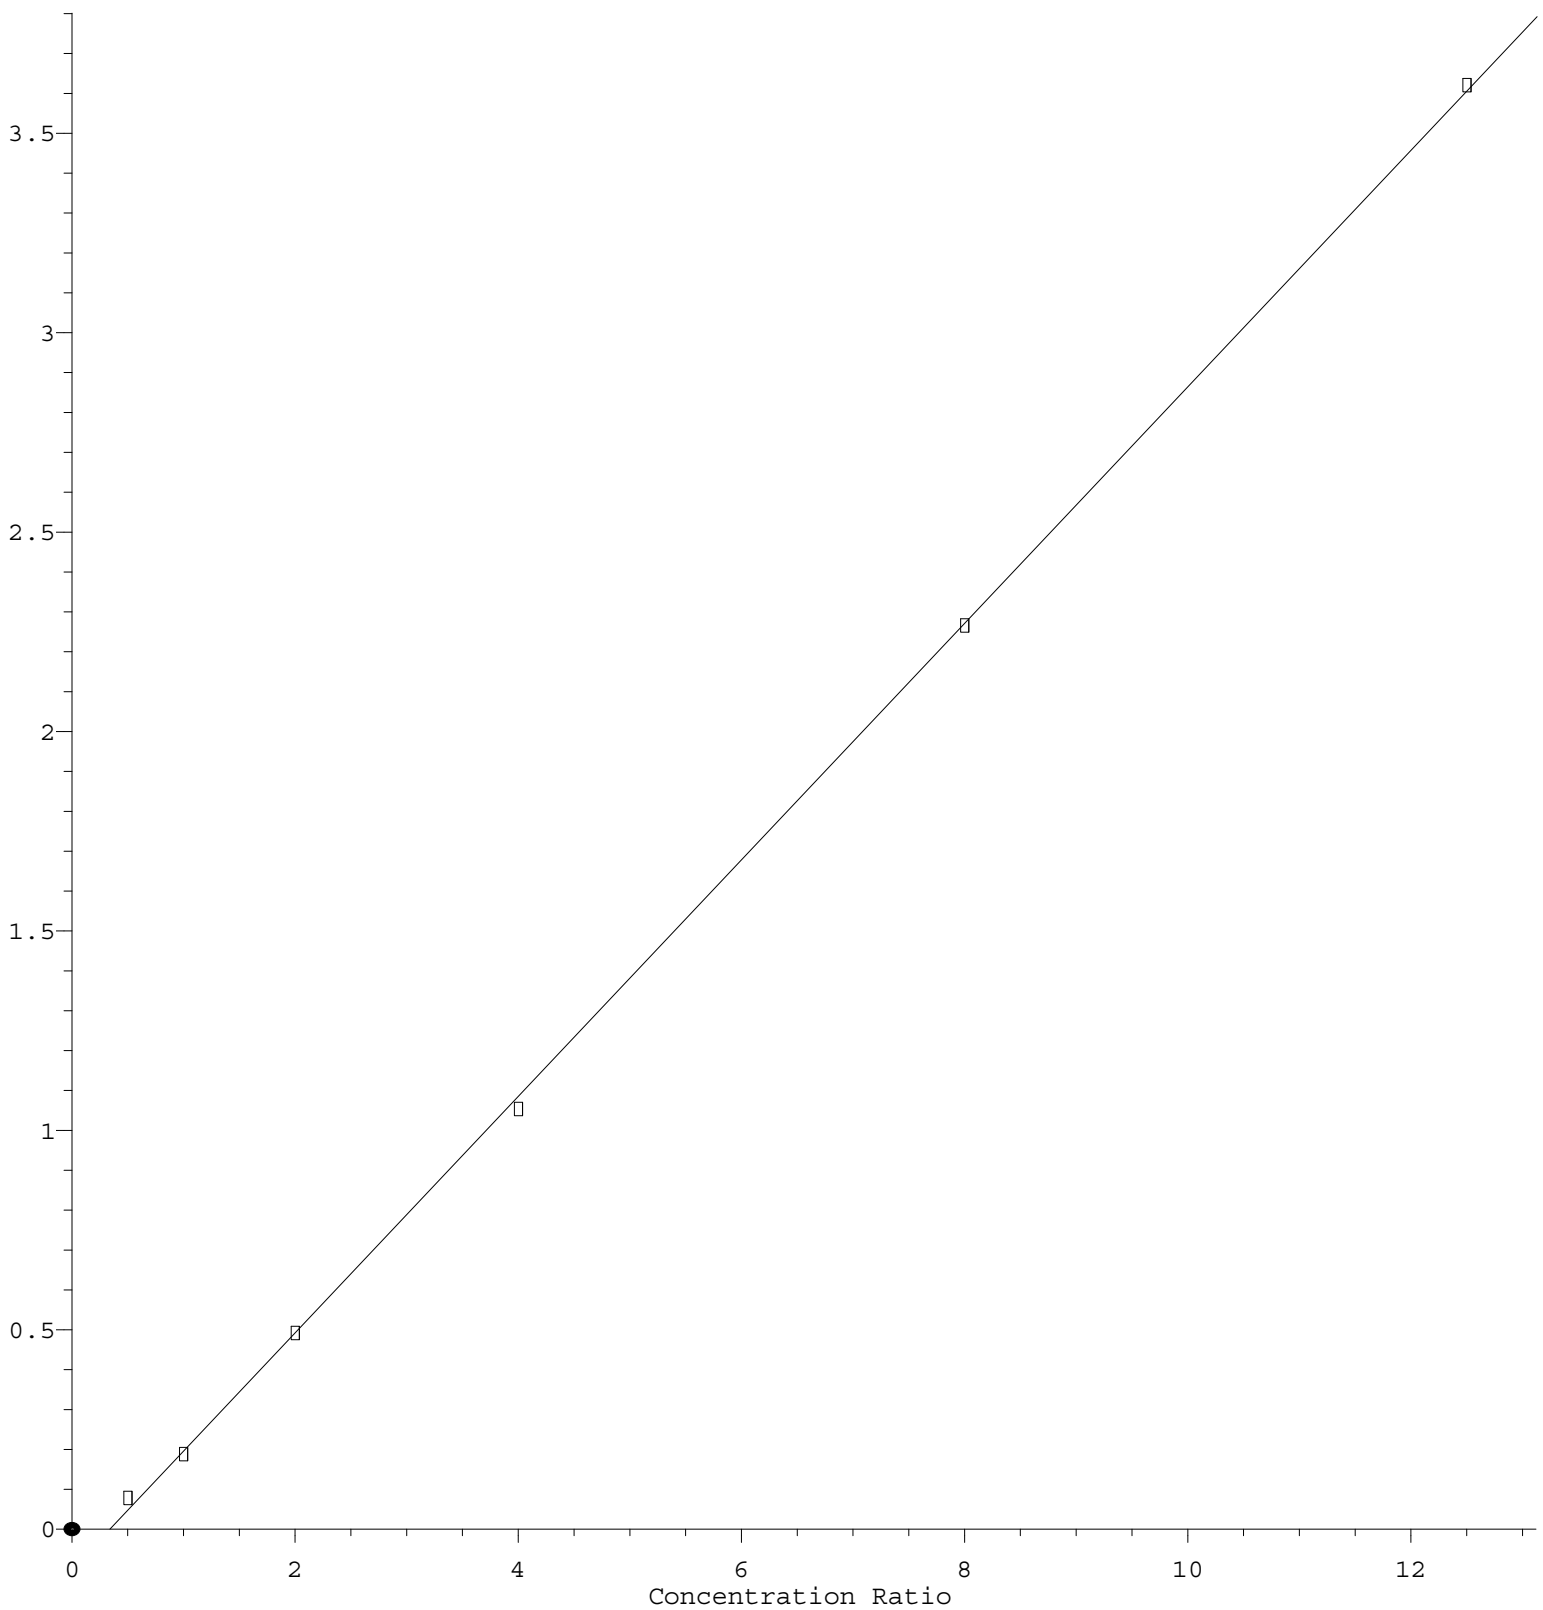

$$\text{Response} = 2.967\text{e-}001 * \text{Amt} - 1.016\text{e-}001$$


Coef of Det (r^2) = 0.999767 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M

Calibration Table Last Updated: Wed Dec 29 16:08:47 2021

2,4,6-Tribromophenol

Response Ratio

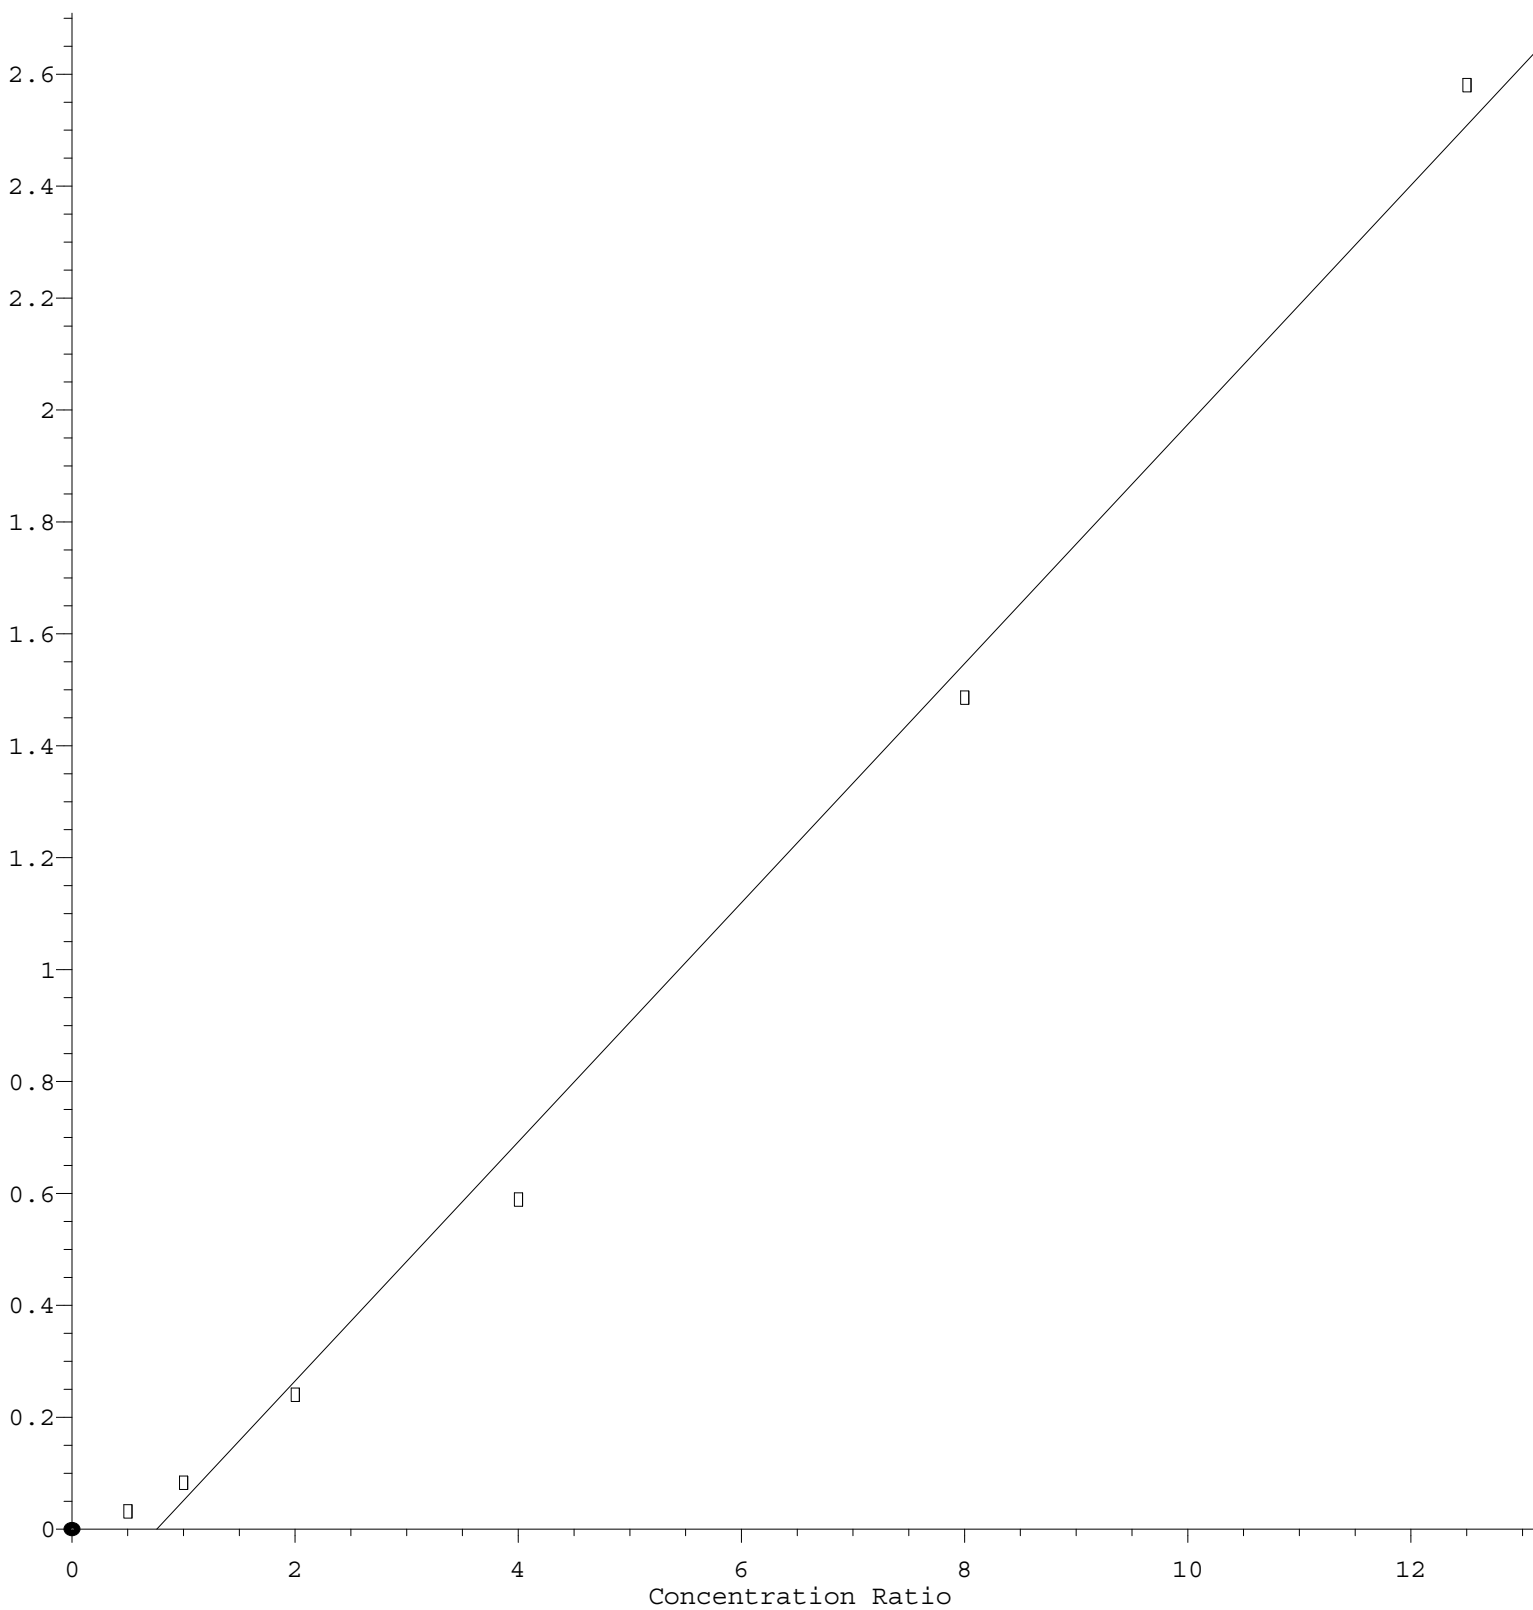


$$\text{Response} = 2.138\text{e-}001 * \text{Amt} - 1.628\text{e-}001$$

Coef of Det (r^2) = 0.994349 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M

Calibration Table Last Updated: Wed Dec 29 16:08:47 2021


4,6-Dinitro-2-methylphenol

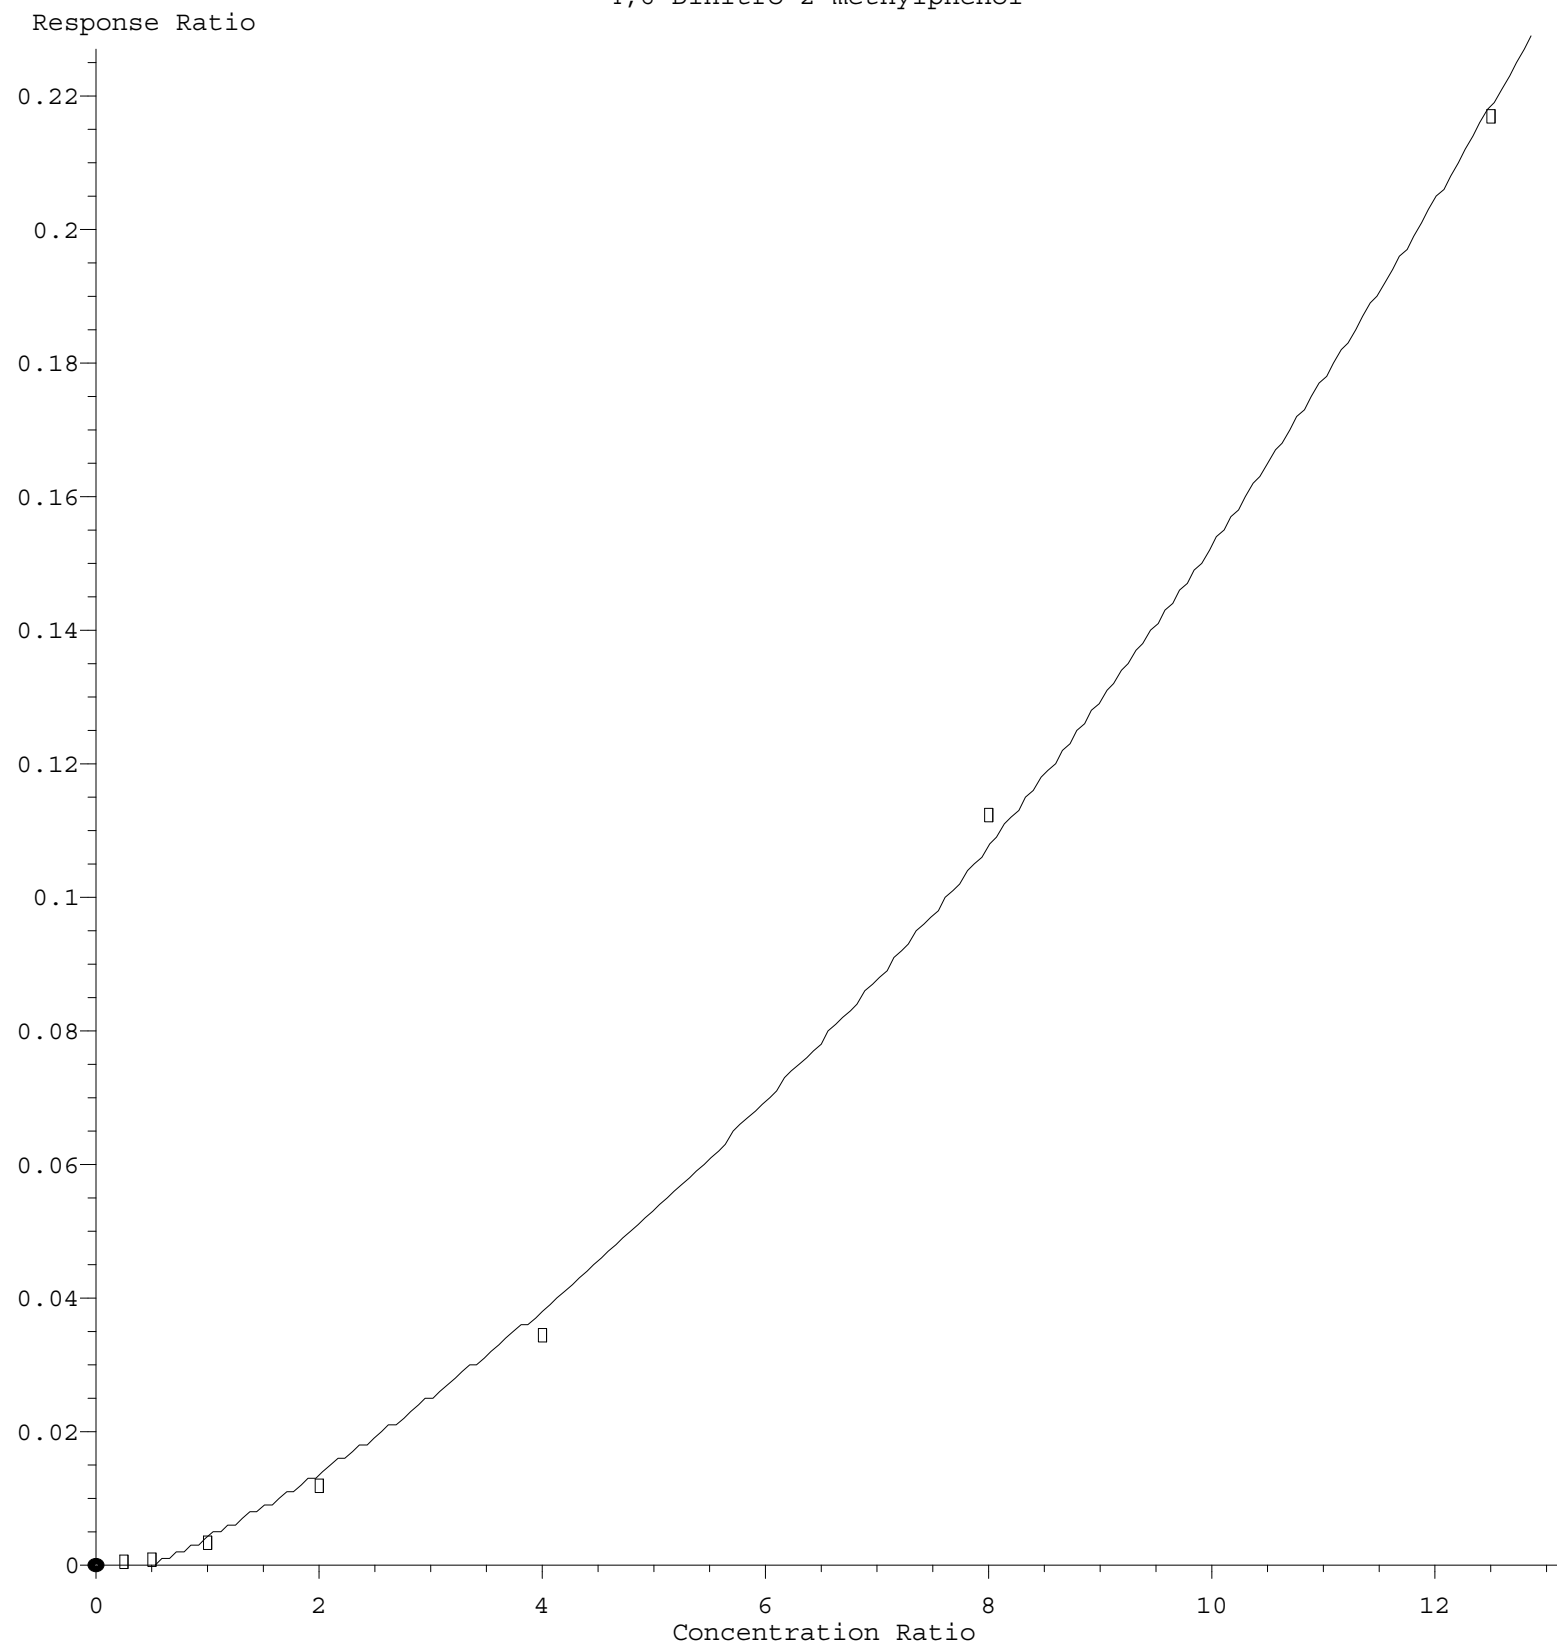

$R = 8.538e-004 A^2 + 7.105e-003 A - 3.817e-003$
 Coef of Det (r^2) = 0.998771 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M
 Calibration Table Last Updated: Wed Dec 29 16:08:47 2021

Atrazine

Response Ratio

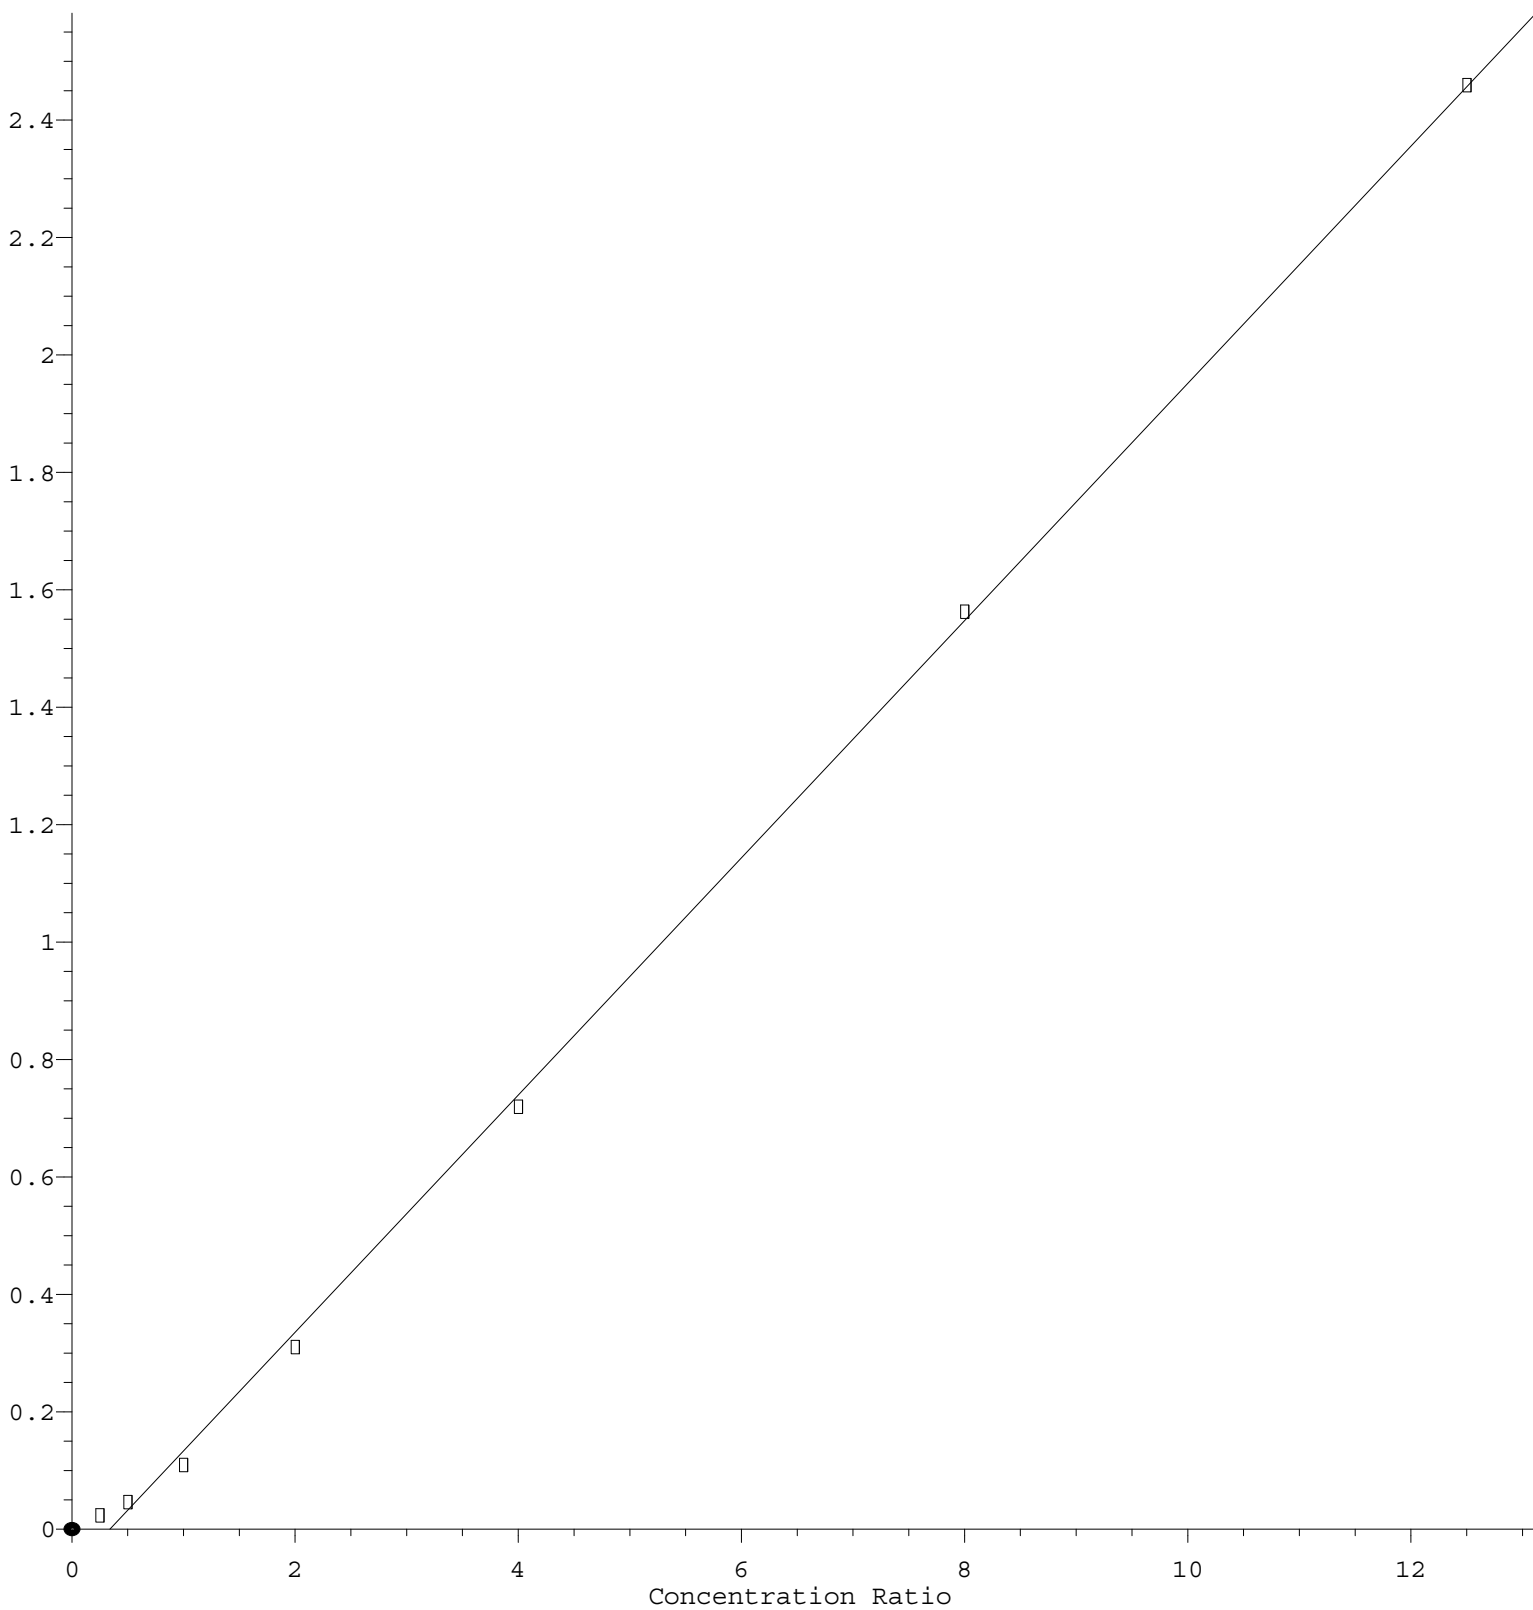

$$\text{Response} = 2.020\text{e-}001 * \text{Amt} - 6.819\text{e-}002$$


Coef of Det (r^2) = 0.999282 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M

Calibration Table Last Updated: Wed Dec 29 16:08:47 2021

Pentachlorophenol


Response Ratio

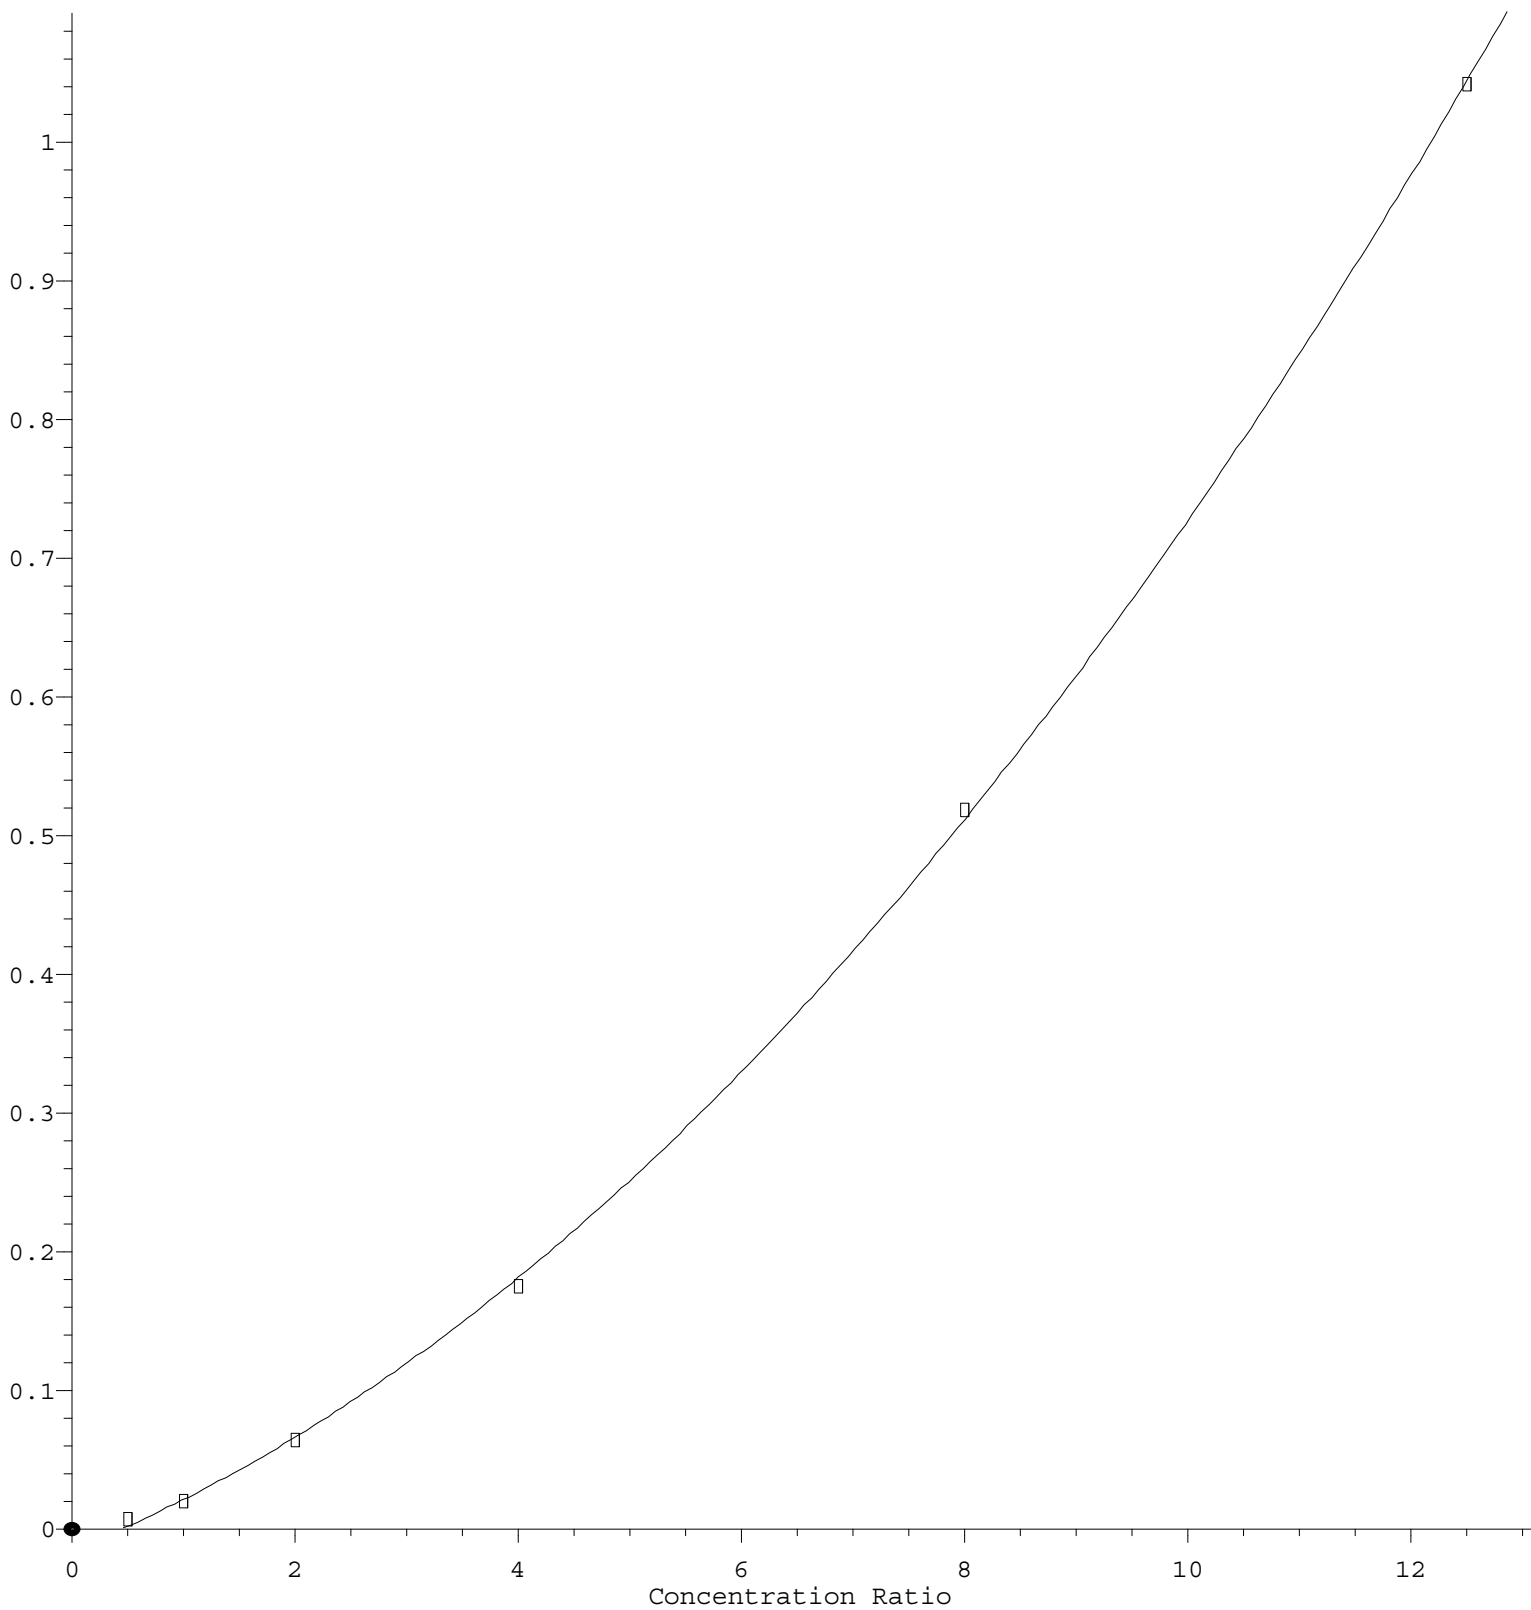

$R = 4.189e-003 A^2 + 3.236e-002 A - 1.511e-002$
 Coef of Det (r^2) = 0.999857 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M
 Calibration Table Last Updated: Wed Dec 29 16:08:47 2021

Anthracene

Response Ratio

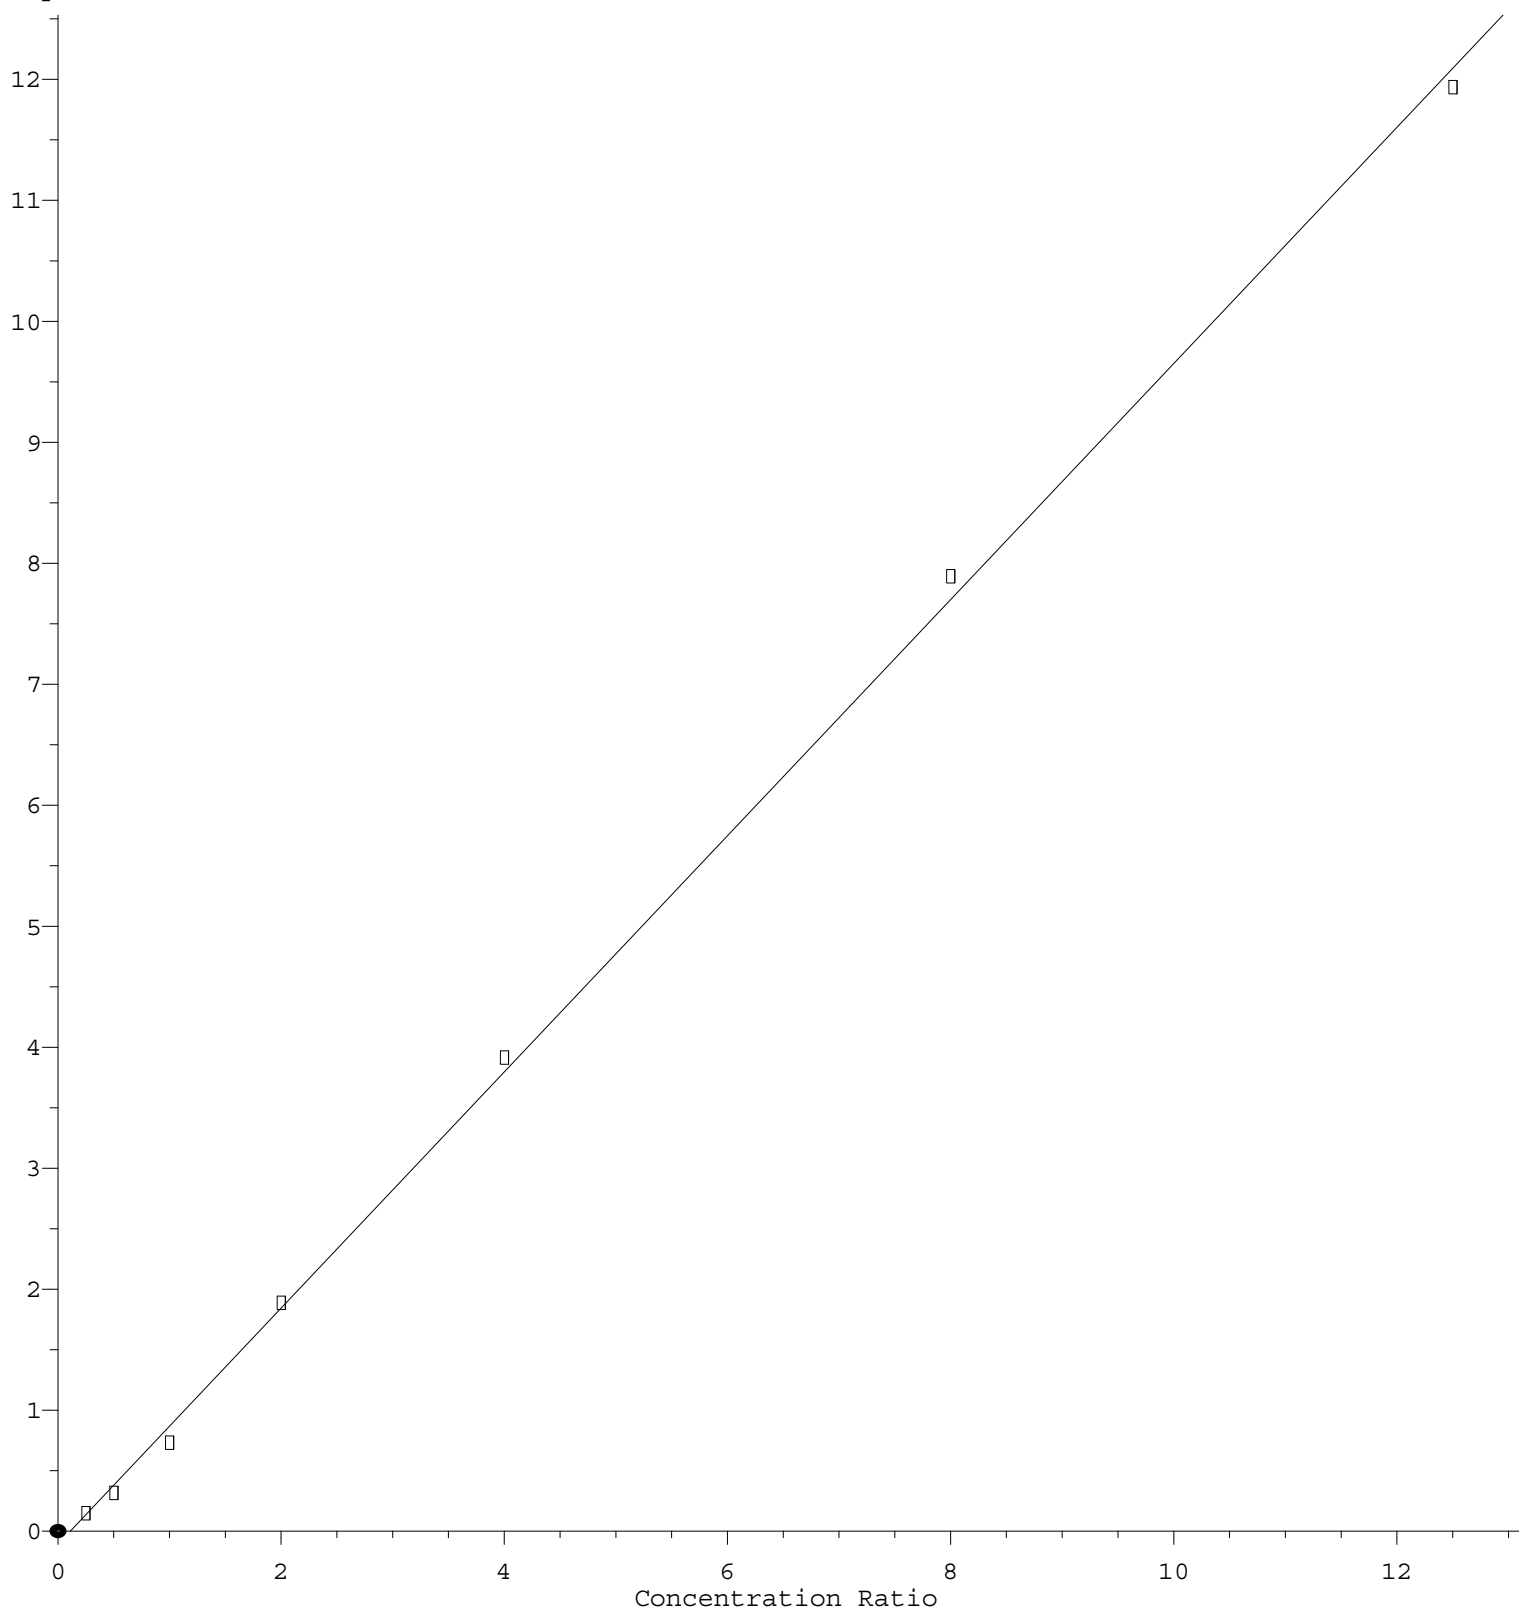

$$\text{Response} = 9.755\text{e-}001 * \text{Amt} - 1.048\text{e-}001$$


Coef of Det (r^2) = 0.999174 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M

Calibration Table Last Updated: Wed Dec 29 16:08:47 2021

Benzo (a) anthracene

Response Ratio

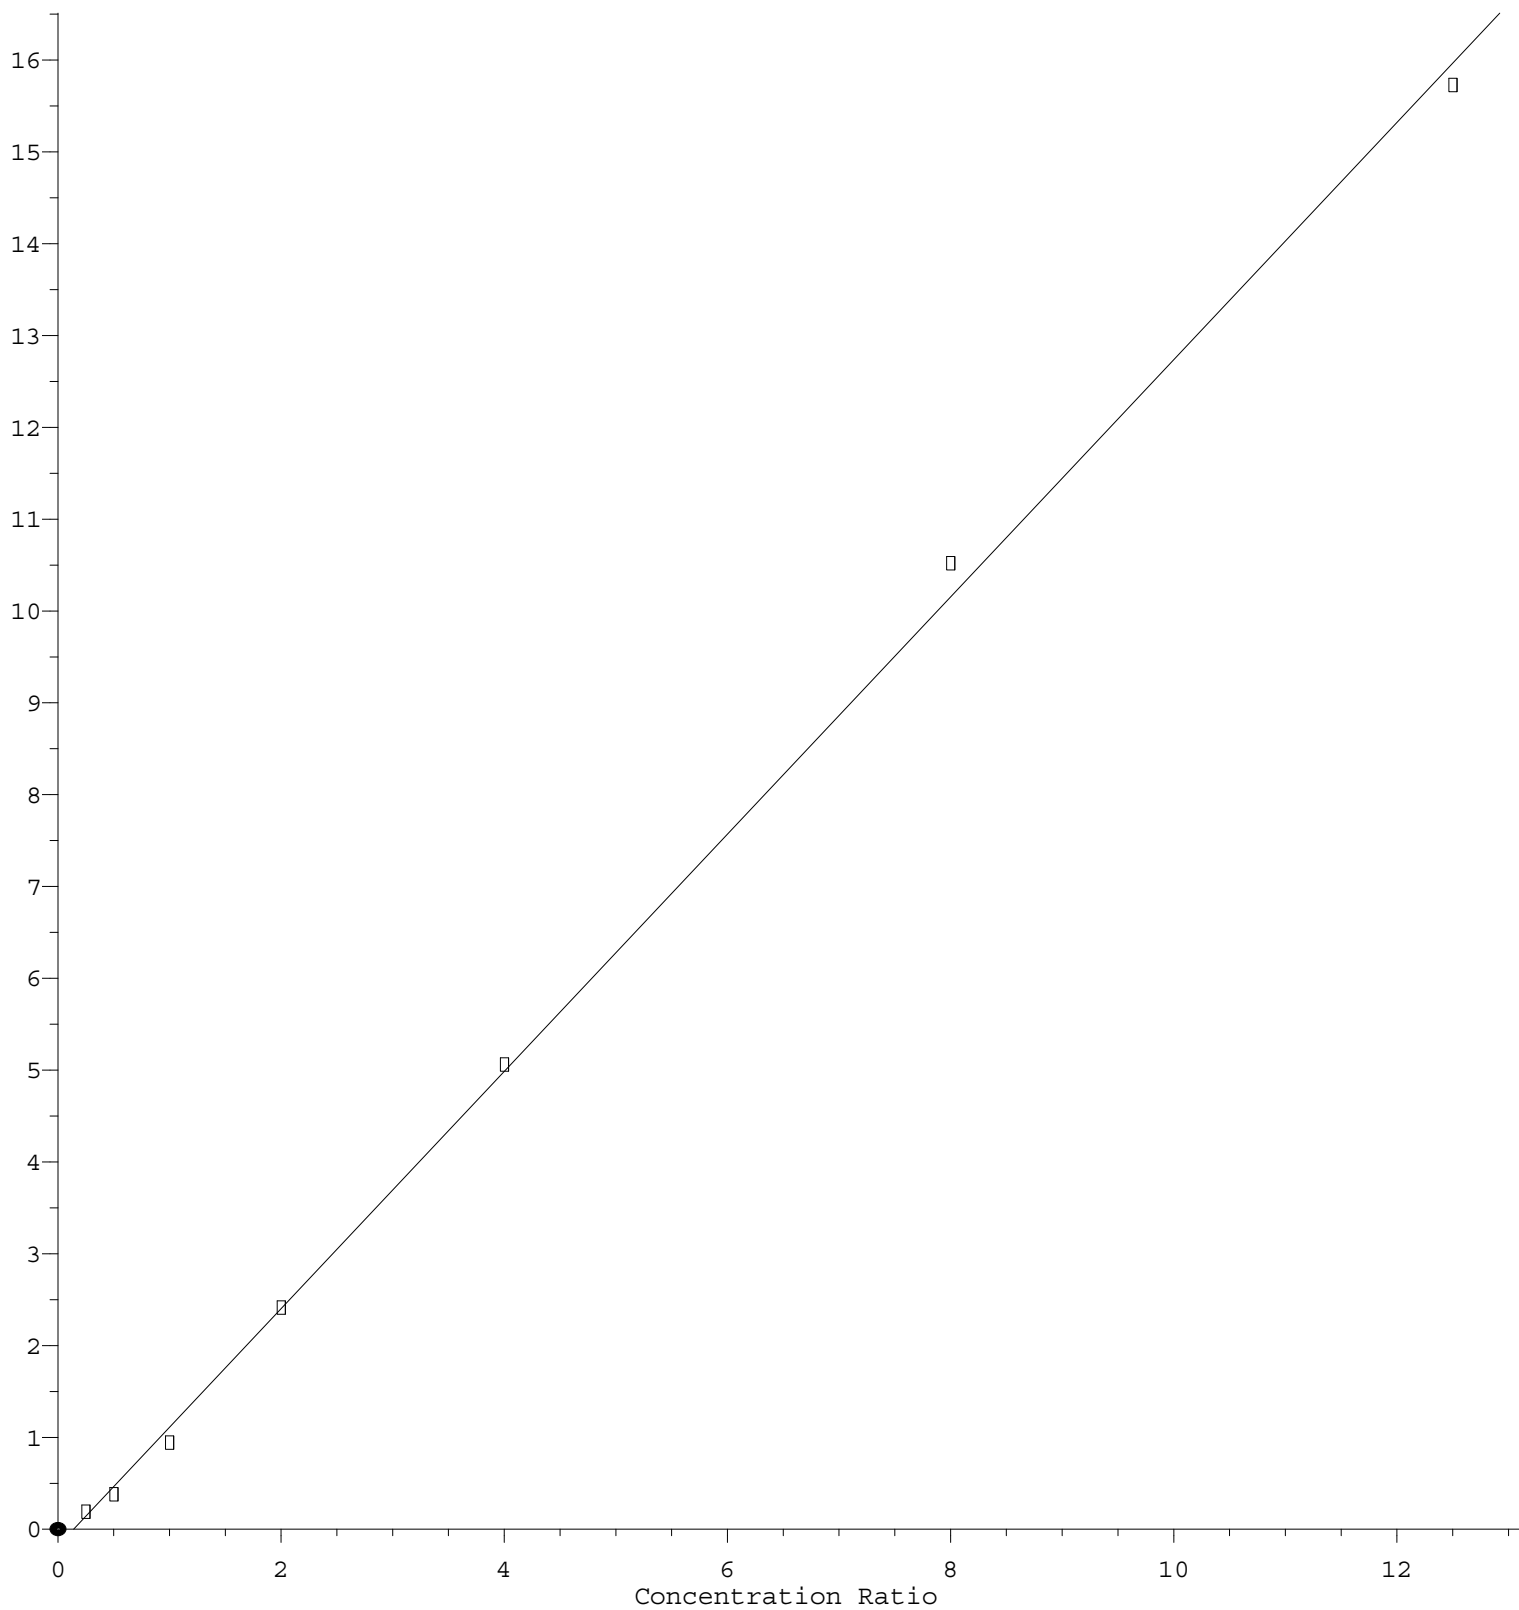

$$\text{Response} = 1.292\text{e}+000 * \text{Amt} - 1.813\text{e}-001$$

Coef of Det (r^2) = 0.998899 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN122921.M

Calibration Table Last Updated: Wed Dec 29 16:08:47 2021